

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
 Data File : VU053199.D
 Acq On : 15 Mar 2023 14:43
 Operator : JC/MD
 Sample : 01929-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053199.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.598	73	80	94	rBV	100561	115951	16.48%	2.209%
2	1.916	170	179	199	rVB	78145	107025	15.21%	2.039%
3	2.569	369	382	398	rBV	158681	258847	36.79%	4.931%
4	2.784	445	449	450	rBV	598	428	0.06%	0.008%
5	3.125	552	555	556	rBV	260	164	0.02%	0.003%
6	3.170	565	569	570	rBV2	357	248	0.04%	0.005%
7	3.270	597	600	603	rBV	178	140	0.02%	0.003%
8	3.389	634	637	641	rBV	247	192	0.03%	0.004%
9	3.414	643	645	649	rBV	191	120	0.02%	0.002%
10	3.498	668	671	676	rBV2	227	171	0.02%	0.003%
11	3.575	690	695	699	rBV2	278	317	0.05%	0.006%
12	3.671	722	725	729	rBV	173	104	0.01%	0.002%
13	3.736	741	745	748	rVB	218	180	0.03%	0.003%
14	3.755	749	751	754	rBV	151	107	0.02%	0.002%
15	3.954	811	813	814	rBV	128	35	0.00%	0.001%
16	4.054	842	844	845	rBV	107	61	0.01%	0.001%
17	4.073	846	850	852	rVV2	229	170	0.02%	0.003%
18	4.093	852	856	859	rVV	182	189	0.03%	0.004%
19	4.125	863	866	869	rBV	153	121	0.02%	0.002%
20	4.215	892	894	895	rBV	160	53	0.01%	0.001%
21	4.253	904	906	909	rVB2	136	77	0.01%	0.001%
22	4.286	914	916	919	rVB	191	74	0.01%	0.001%
23	4.556	997	1000	1002	rBV	202	179	0.03%	0.003%
24	4.623	1009	1021	1058	rBV2	40725	108531	15.43%	2.067%
25	4.900	1105	1107	1110	rBV	146	105	0.01%	0.002%
26	5.057	1139	1156	1179	rBV	127959	281669	40.04%	5.366%
27	5.208	1198	1203	1209	rBB2	211	308	0.04%	0.006%
28	5.356	1247	1249	1252	rBV	166	139	0.02%	0.003%
29	5.388	1257	1259	1262	rBV2	153	91	0.01%	0.002%
30	5.450	1274	1278	1286	rBV2	183	301	0.04%	0.006%
31	5.720	1342	1362	1384	rBV2	260205	703485	100.00%	13.401%
32	5.906	1416	1420	1423	rBV2	357	326	0.05%	0.006%
33	6.009	1450	1452	1454	rBV	227	132	0.02%	0.003%
34	6.244	1511	1525	1543	rBV	207872	392621	55.81%	7.479%
35	6.443	1583	1587	1591	rBV2	412	505	0.07%	0.010%
36	6.459	1591	1592	1594	rVV2	330	98	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
 Data File : VU053199.D
 Acq On : 15 Mar 2023 14:43
 Operator : JC/MD
 Sample : 01929-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.485	1595	1600	1604	rVB2	208	225	0.03%	0.004%
38	6.565	1622	1625	1628	rBV	198	124	0.02%	0.002%
39	6.594	1629	1634	1636	rBV2	177	178	0.03%	0.003%
40	6.684	1649	1662	1683	rBV	163939	318480	45.27%	6.067%
41	6.903	1726	1730	1732	rVB	219	165	0.02%	0.003%
42	6.922	1732	1736	1741	rBB2	197	170	0.02%	0.003%
43	6.974	1750	1752	1755	rVB2	160	94	0.01%	0.002%
44	7.012	1760	1764	1771	rVV2	202	204	0.03%	0.004%
45	7.054	1771	1777	1781	rVV2	203	249	0.04%	0.005%
46	7.080	1783	1785	1788	rVV2	176	102	0.01%	0.002%
47	7.096	1788	1790	1793	rVB	204	91	0.01%	0.002%
48	7.134	1799	1802	1804	rVB2	237	133	0.02%	0.003%
49	7.189	1814	1819	1823	rBV4	810	847	0.12%	0.016%
50	7.366	1871	1874	1878	rVB2	244	170	0.02%	0.003%
51	7.392	1880	1882	1888	rVB	269	166	0.02%	0.003%
52	7.417	1888	1890	1892	rBV	147	89	0.01%	0.002%
53	7.430	1892	1894	1898	rVB	224	114	0.02%	0.002%
54	7.453	1898	1901	1904	rBV	223	115	0.02%	0.002%
55	7.559	1923	1934	1957	rBV	96457	169726	24.13%	3.233%
56	7.691	1971	1975	1981	rBV3	920	1118	0.16%	0.021%
57	7.784	2002	2004	2005	rBV	250	133	0.02%	0.003%
58	7.893	2025	2038	2066	rBV	333015	578662	82.26%	11.023%
59	8.173	2112	2125	2145	rBV2	63586	109991	15.64%	2.095%
60	8.318	2166	2170	2173	rBV2	168	164	0.02%	0.003%
61	8.337	2174	2176	2178	rBV2	217	127	0.02%	0.002%
62	8.395	2191	2194	2200	rBV2	245	160	0.02%	0.003%
63	8.472	2215	2218	2222	rBV2	275	197	0.03%	0.004%
64	8.514	2227	2231	2234	rBV2	334	302	0.04%	0.006%
65	8.629	2256	2267	2294	rBV2	132075	258089	36.69%	4.916%
66	8.787	2314	2316	2318	rBV2	236	114	0.02%	0.002%
67	8.851	2333	2336	2338	rBV	250	195	0.03%	0.004%
68	8.896	2347	2350	2353	rBV	210	133	0.02%	0.003%
69	8.980	2373	2376	2379	rVB	165	87	0.01%	0.002%
70	9.006	2379	2384	2388	rBV2	233	269	0.04%	0.005%
71	9.199	2442	2444	2446	rBV	193	133	0.02%	0.003%
72	9.343	2483	2489	2492	rBV2	305	358	0.05%	0.007%
73	9.411	2498	2510	2534	rBV	294741	494142	70.24%	9.413%
74	9.601	2566	2569	2574	rBV	301	247	0.04%	0.005%
75	9.694	2593	2598	2602	rBV2	564	538	0.08%	0.010%
76	9.716	2602	2605	2611	rBV2	254	287	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
 Data File : VU053199.D
 Acq On : 15 Mar 2023 14:43
 Operator : JC/MD
 Sample : 01929-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	9.877	2652	2655	2657	rBV2	180	98	0.01%	0.002%
78	9.941	2671	2675	2679	rBV	331	303	0.04%	0.006%
79	10.019	2697	2699	2701	rVB	186	93	0.01%	0.002%
80	10.163	2741	2744	2745	rBV2	179	110	0.02%	0.002%
81	10.446	2830	2832	2834	rBV	215	147	0.02%	0.003%
82	10.485	2838	2844	2847	rBV2	539	532	0.08%	0.010%
83	10.752	2914	2927	2945	rBV	205335	326113	46.36%	6.212%
84	10.842	2951	2955	2959	rBV2	387	334	0.05%	0.006%
85	10.864	2959	2962	2964	rBV	197	152	0.02%	0.003%
86	11.031	3011	3014	3018	rBV2	274	201	0.03%	0.004%
87	11.269	3086	3088	3093	rVB2	255	194	0.03%	0.004%
88	11.301	3095	3098	3101	rVB2	273	174	0.02%	0.003%
89	11.321	3101	3104	3107	rBV2	227	162	0.02%	0.003%
90	11.369	3116	3119	3123	rBB	248	157	0.02%	0.003%
91	11.433	3136	3139	3142	rVB2	195	131	0.02%	0.002%
92	11.469	3143	3150	3153	rBV3	624	797	0.11%	0.015%
93	11.745	3231	3236	3241	rVB3	891	891	0.13%	0.017%
94	11.806	3243	3255	3283	rBV	320378	517232	73.52%	9.853%
95	12.102	3345	3347	3350	rBV	274	158	0.02%	0.003%
96	12.189	3362	3374	3396	rBV	300064	489181	69.54%	9.319%
97	12.690	3527	3530	3534	rVB	247	159	0.02%	0.003%
98	12.919	3598	3601	3603	rBV	298	183	0.03%	0.003%
99	13.842	3884	3888	3896	rVB3	1526	1458	0.21%	0.028%
100	14.539	4102	4105	4109	rBV2	419	379	0.05%	0.007%


Sum of corrected areas: 5249491

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
Data File : VU053199.D
Acq On : 15 Mar 2023 14:43
Operator : JC/MD
Sample : 01929-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

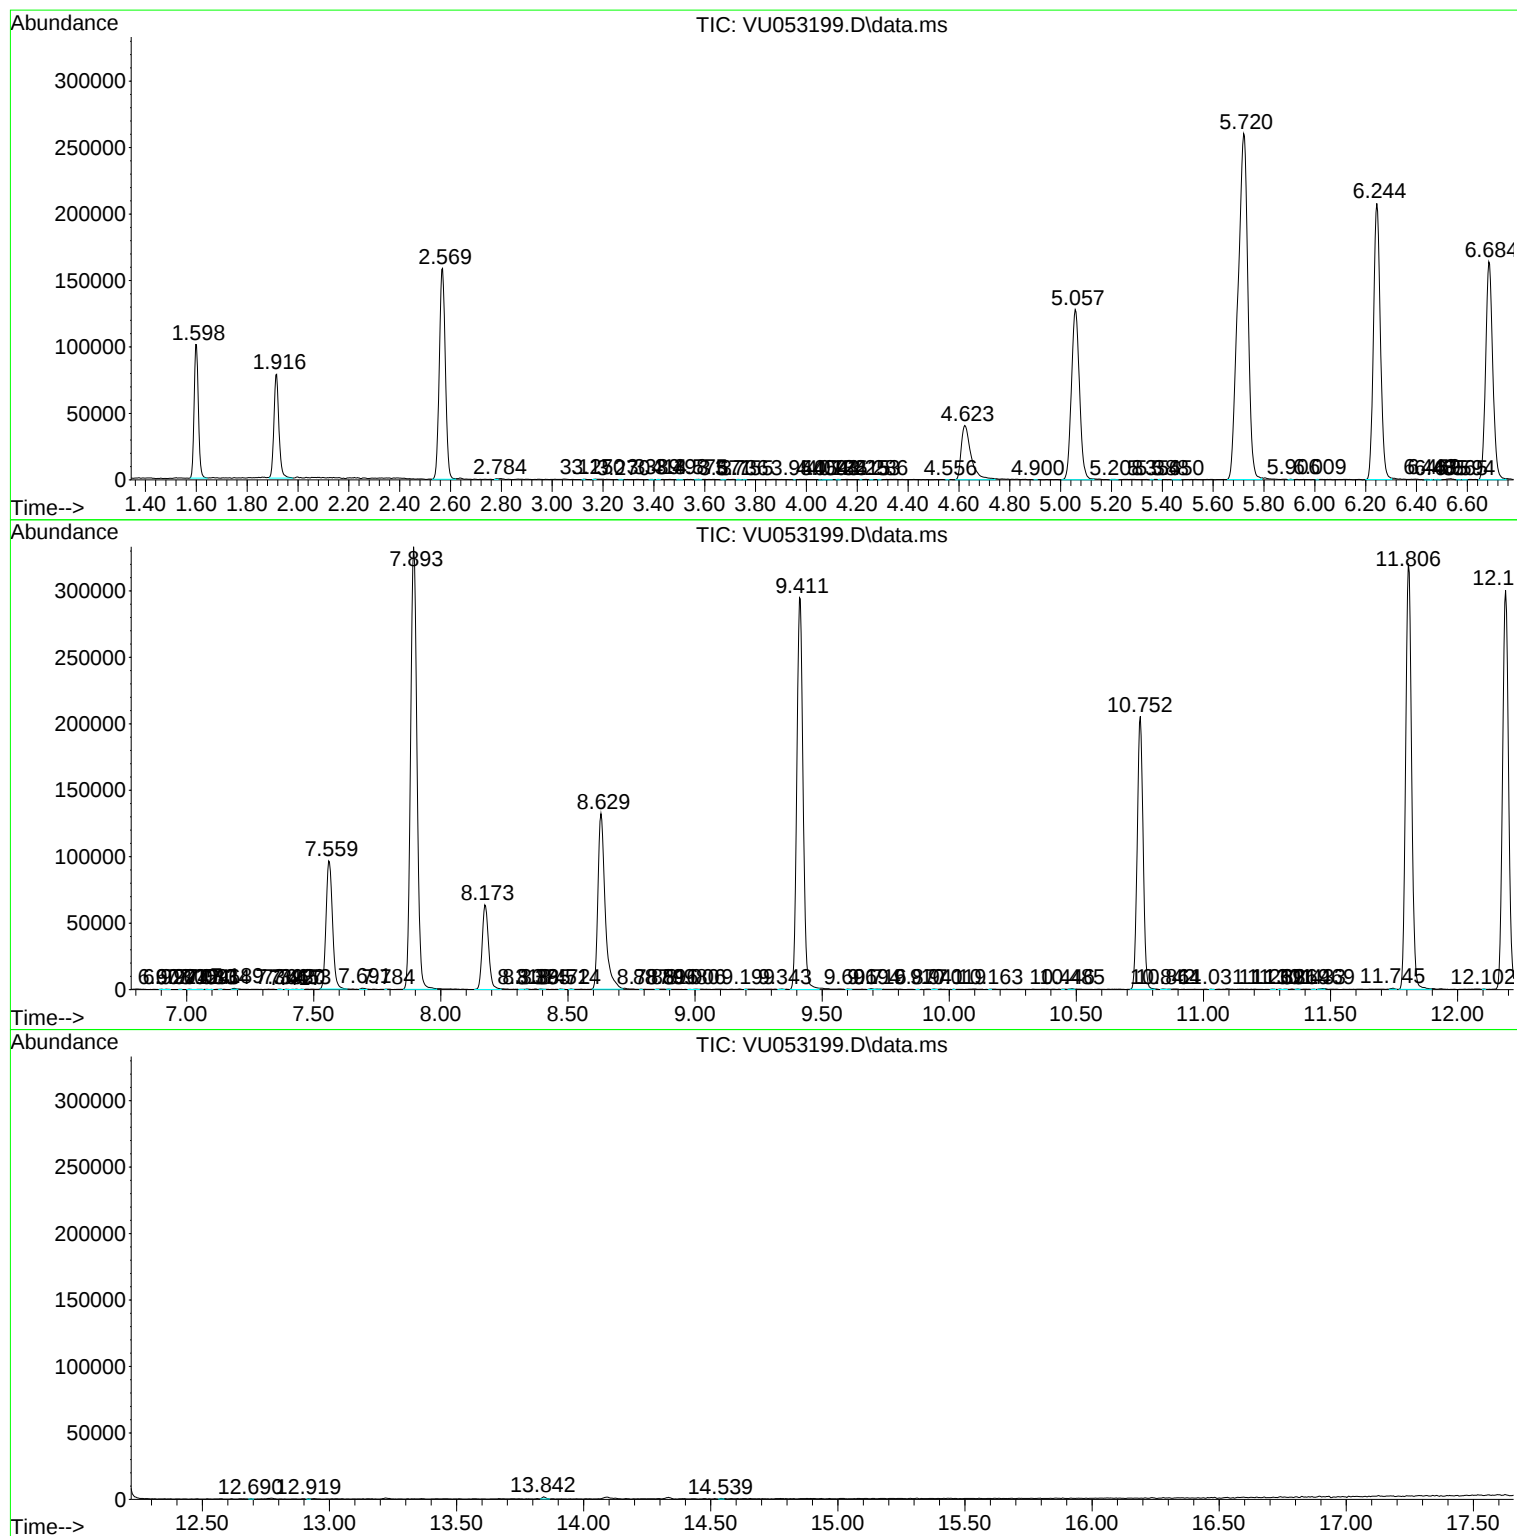

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
Data File : VU053199.D
Acq On : 15 Mar 2023 14:43
Operator : JC/MD
Sample : 01929-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
Data File : VU053199.D
Acq On : 15 Mar 2023 14:43
Operator : JC/MD
Sample : 01929-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------