

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
 Data File : VU053213.D
 Acq On : 15 Mar 2023 20:11
 Operator : JC/MD
 Sample : VIBLK112
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK112

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053213.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	96	rVB	100646	116164	17.27%	2.253%
2	1.912	171	178	195	rVB	76385	102363	15.22%	1.985%
3	2.568	370	382	397	rBV	148344	242466	36.05%	4.703%
4	3.044	523	530	541	rVB3	4066	7273	1.08%	0.141%
5	3.166	565	568	569	rBV	314	179	0.03%	0.003%
6	3.382	631	635	637	rBV	234	187	0.03%	0.004%
7	3.481	665	666	667	rBV	131	41	0.01%	0.001%
8	3.546	683	686	690	rBV	209	129	0.02%	0.003%
9	3.800	762	765	767	rBV2	134	98	0.01%	0.002%
10	3.838	774	777	778	rBV	160	94	0.01%	0.002%
11	3.951	810	812	813	rBV	158	50	0.01%	0.001%
12	4.147	868	873	876	rBV2	243	283	0.04%	0.005%
13	4.186	882	885	887	rBV	224	126	0.02%	0.002%
14	4.285	908	916	918	rBV	332	409	0.06%	0.008%
15	4.533	990	993	996	rBV	213	132	0.02%	0.003%
16	4.623	1008	1021	1026	rBV2	44283	89840	13.36%	1.743%
17	4.883	1098	1102	1104	rBV	322	229	0.03%	0.004%
18	4.919	1111	1113	1114	rBV	132	53	0.01%	0.001%
19	4.973	1128	1130	1135	rVB2	207	187	0.03%	0.004%
20	5.057	1140	1156	1180	rBV	124379	268644	39.95%	5.211%
21	5.166	1186	1190	1192	rBV	230	174	0.03%	0.003%
22	5.215	1201	1205	1208	rVB	196	163	0.02%	0.003%
23	5.295	1228	1230	1231	rBV	161	45	0.01%	0.001%
24	5.388	1255	1259	1263	rBV	210	185	0.03%	0.004%
25	5.481	1287	1288	1289	rBV	221	73	0.01%	0.001%
26	5.584	1317	1320	1325	rVB	219	155	0.02%	0.003%
27	5.607	1325	1327	1328	rBV	116	36	0.01%	0.001%
28	5.620	1328	1331	1337	rVB	200	117	0.02%	0.002%
29	5.719	1341	1362	1385	rBV2	249048	672517	100.00%	13.045%
30	5.915	1419	1423	1425	rBV2	182	182	0.03%	0.004%
31	5.954	1434	1435	1437	rBV	110	25	0.00%	0.000%
32	5.996	1444	1448	1452	rVB2	242	218	0.03%	0.004%
33	6.041	1459	1462	1463	rBV	297	188	0.03%	0.004%
34	6.079	1472	1474	1475	rBV	150	81	0.01%	0.002%
35	6.121	1484	1487	1490	rBV2	304	228	0.03%	0.004%
36	6.157	1495	1498	1501	rVV2	264	171	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
 Data File : VU053213.D
 Acq On : 15 Mar 2023 20:11
 Operator : JC/MD
 Sample : VIBLK112
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK112

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.243	1513	1525	1547	rBV	203079	382070	56.81%	7.411%
38	6.420	1576	1580	1581	rBV2	188	127	0.02%	0.002%
39	6.497	1601	1604	1605	rBV	206	110	0.02%	0.002%
40	6.539	1605	1617	1634	rVB	54936	101390	15.08%	1.967%
41	6.684	1648	1662	1683	rBV	156091	301099	44.77%	5.840%
42	6.796	1692	1697	1699	rBV	518	518	0.08%	0.010%
43	6.867	1717	1719	1721	rBV	144	79	0.01%	0.002%
44	6.886	1721	1725	1728	rVB2	205	126	0.02%	0.002%
45	6.906	1728	1731	1734	rBV2	214	145	0.02%	0.003%
46	6.925	1734	1737	1741	rBV2	186	157	0.02%	0.003%
47	6.970	1748	1751	1752	rBV2	139	66	0.01%	0.001%
48	7.002	1759	1761	1764	rBV	190	90	0.01%	0.002%
49	7.083	1781	1786	1787	rBV	205	215	0.03%	0.004%
50	7.179	1810	1816	1822	rBV4	981	1256	0.19%	0.024%
51	7.205	1822	1824	1827	rVV	312	191	0.03%	0.004%
52	7.234	1831	1833	1836	rVB	201	77	0.01%	0.001%
53	7.263	1838	1842	1846	rVV	296	216	0.03%	0.004%
54	7.366	1871	1874	1877	rBV2	163	158	0.02%	0.003%
55	7.562	1922	1935	1955	rBV	90515	158591	23.58%	3.076%
56	7.729	1984	1987	1988	rBV2	114	62	0.01%	0.001%
57	7.825	2013	2017	2020	rBV2	268	196	0.03%	0.004%
58	7.893	2022	2038	2069	rBV	313913	542653	80.69%	10.526%
59	8.176	2113	2126	2150	rVB	61852	104900	15.60%	2.035%
60	8.256	2150	2151	2152	rBV	114	26	0.00%	0.001%
61	8.285	2157	2160	2161	rBV	138	58	0.01%	0.001%
62	8.362	2182	2184	2187	rVB	200	108	0.02%	0.002%
63	8.629	2255	2267	2298	rBV2	139282	263949	39.25%	5.120%
64	8.739	2298	2301	2305	rBV2	401	270	0.04%	0.005%
65	9.221	2448	2451	2453	rBV	235	161	0.02%	0.003%
66	9.250	2458	2460	2465	rBV2	205	126	0.02%	0.002%
67	9.317	2479	2481	2485	rVB	199	92	0.01%	0.002%
68	9.414	2498	2511	2530	rBV	288541	482327	71.72%	9.355%
69	9.562	2555	2557	2559	rBV	254	119	0.02%	0.002%
70	9.578	2559	2562	2568	rVB	234	167	0.02%	0.003%
71	9.636	2577	2580	2582	rBV	254	181	0.03%	0.004%
72	9.877	2652	2655	2657	rBV	228	156	0.02%	0.003%
73	9.944	2673	2676	2682	rVB2	212	183	0.03%	0.004%
74	10.163	2742	2744	2745	rBV2	153	74	0.01%	0.001%
75	10.304	2785	2788	2789	rBV	113	65	0.01%	0.001%
76	10.337	2794	2798	2802	rBV	240	282	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
 Data File : VU053213.D
 Acq On : 15 Mar 2023 20:11
 Operator : JC/MD
 Sample : VIBLK112
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK112

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.472	2838	2840	2842	rBV	155	58	0.01%	0.001%
78	10.623	2884	2887	2889	rVB	210	103	0.02%	0.002%
79	10.751	2914	2927	2953	rVB	199659	318657	47.38%	6.181%
80	11.012	3005	3008	3010	rBV	198	112	0.02%	0.002%
81	11.195	3062	3065	3067	rBV2	204	129	0.02%	0.003%
82	11.266	3085	3087	3090	rVB2	252	135	0.02%	0.003%
83	11.497	3156	3159	3162	rVB	271	167	0.02%	0.003%
84	11.623	3197	3198	3199	rBV	115	32	0.00%	0.001%
85	11.713	3223	3226	3228	rBV	258	151	0.02%	0.003%
86	11.806	3243	3255	3278	rBV	320008	515022	76.58%	9.990%
87	12.002	3313	3316	3320	rBV	191	114	0.02%	0.002%
88	12.189	3361	3374	3396	rBV	288848	472203	70.21%	9.159%
89	12.417	3442	3445	3447	rBV2	253	153	0.02%	0.003%
90	12.578	3493	3495	3497	rBV	215	100	0.01%	0.002%
91	13.057	3642	3644	3647	rVB2	287	152	0.02%	0.003%
92	13.224	3693	3696	3701	rBV2	321	313	0.05%	0.006%
93	13.545	3793	3796	3800	rVB	267	180	0.03%	0.003%
94	13.934	3914	3917	3919	rBV2	237	172	0.03%	0.003%
95	14.327	4034	4039	4043	rBV3	377	379	0.06%	0.007%
96	14.449	4074	4077	4081	rVB2	222	154	0.02%	0.003%
97	14.635	4132	4135	4140	rBV2	376	362	0.05%	0.007%
98	14.957	4231	4235	4240	rBV2	311	364	0.05%	0.007%




Sum of corrected areas: 5155553

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
Data File : VU053213.D
Acq On : 15 Mar 2023 20:11
Operator : JC/MD
Sample : VIBLK112
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK112

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

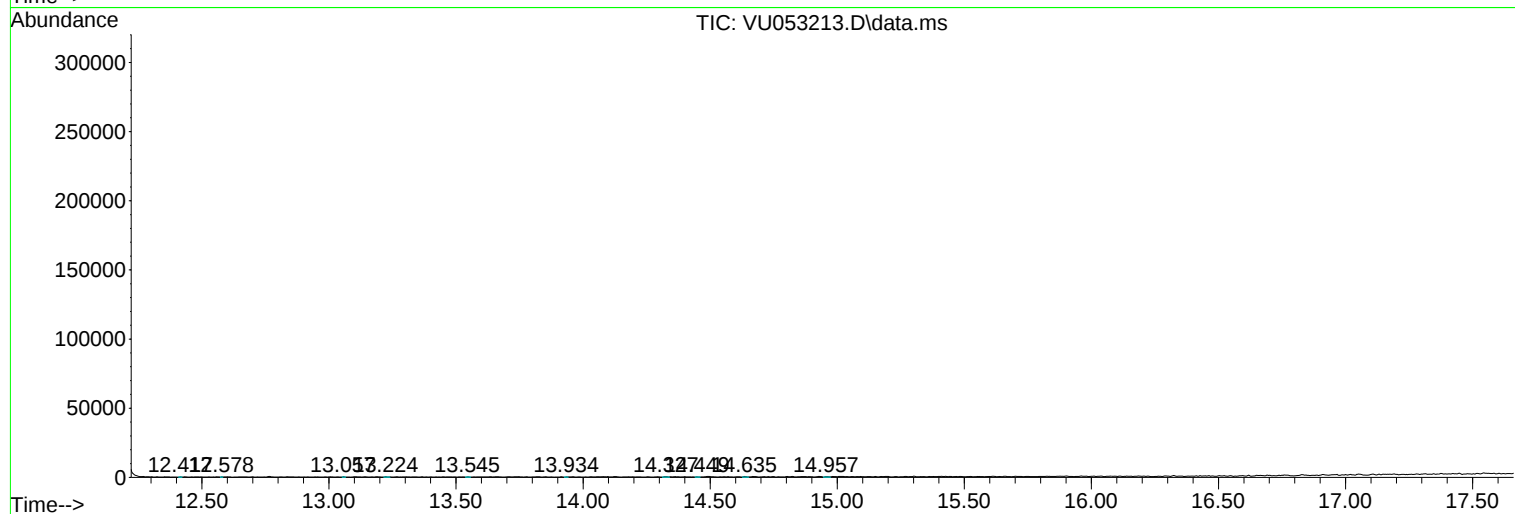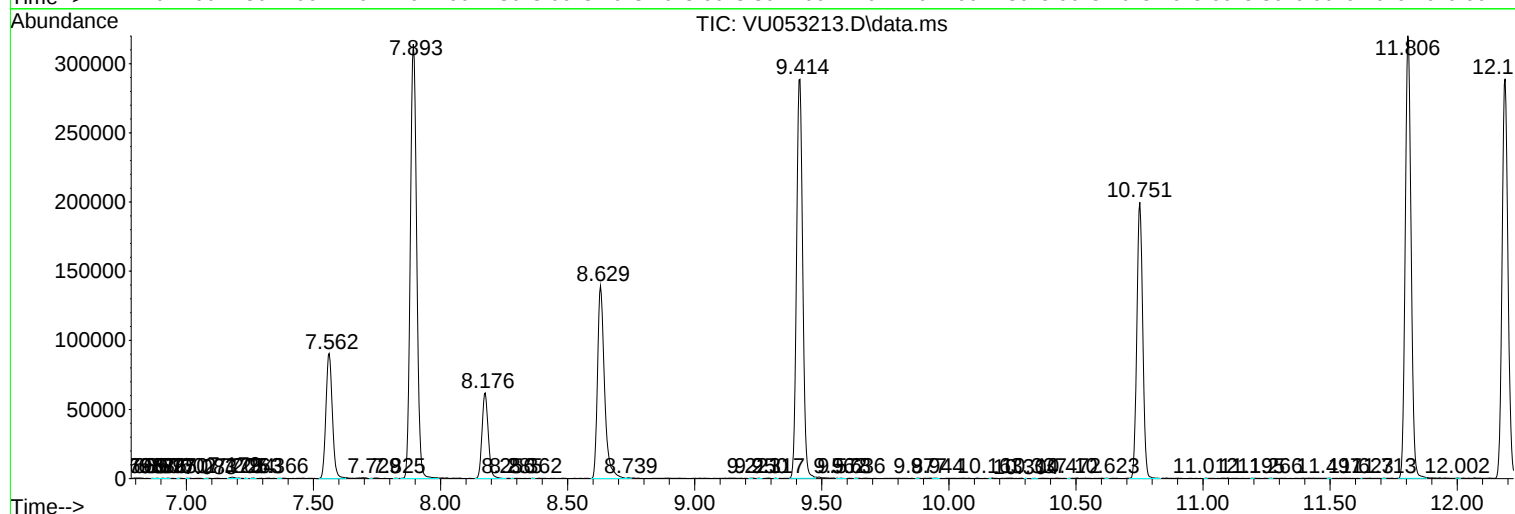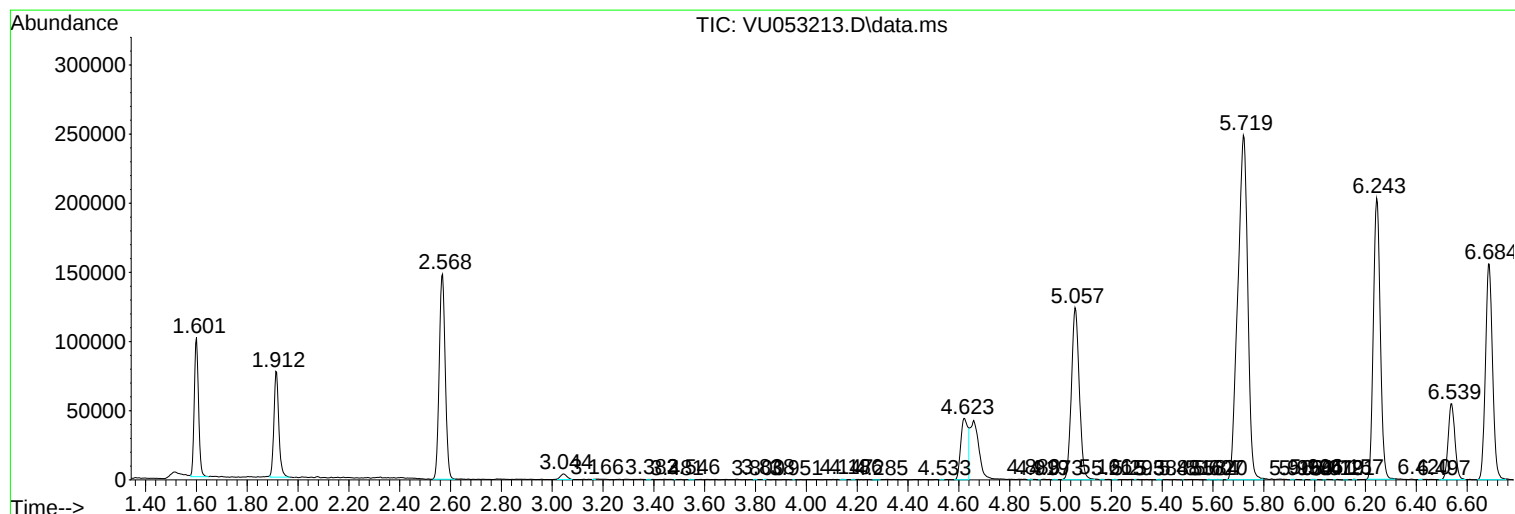

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
Data File : VU053213.D
Acq On : 15 Mar 2023 20:11
Operator : JC/MD
Sample : VIBLK112
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK112

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
Data File : VU053213.D
Acq On : 15 Mar 2023 20:11
Operator : JC/MD
Sample : VIBLK112
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK112

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
