
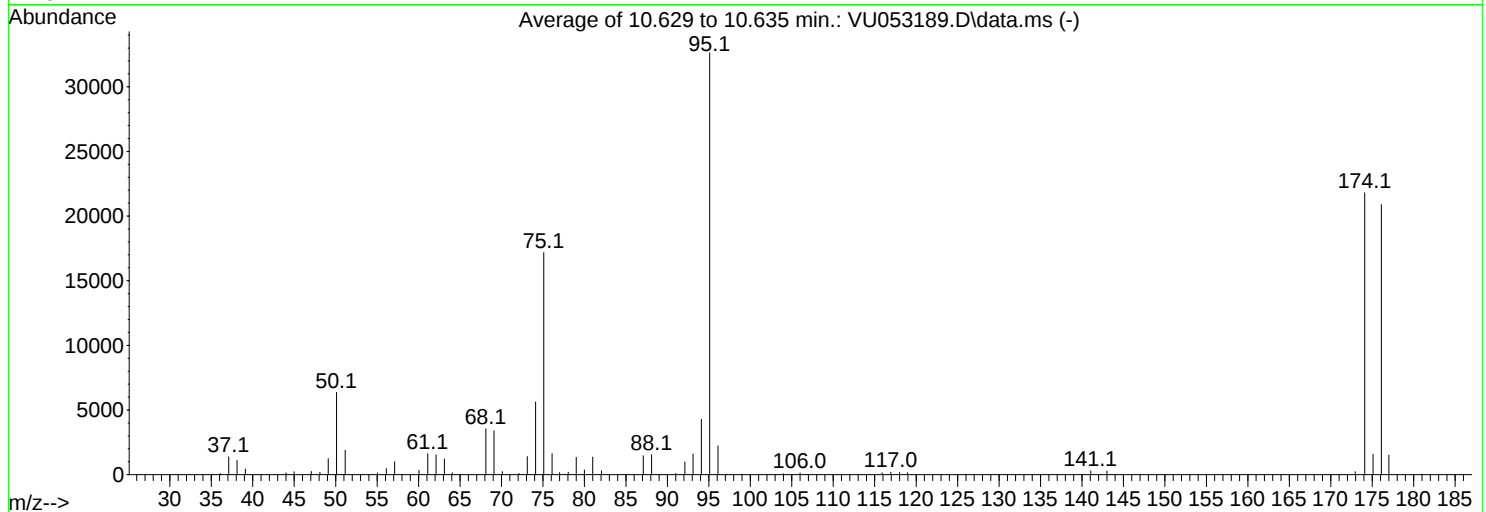


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
Data File : VU053189.D
Acq On : 15 Mar 2023 09:12
Operator : JC/MD
Sample : BFB163
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB163

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Title : VOC Analysis
Last Update : Sat Mar 18 04:29:10 2023

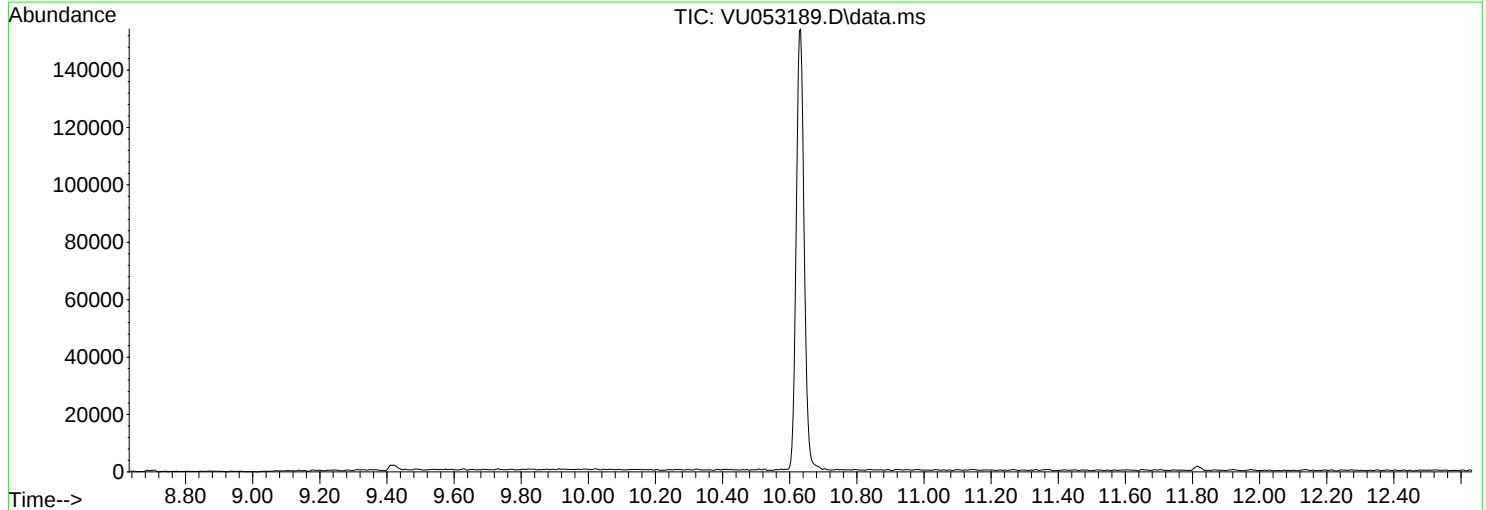

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	6359	PASS
75	95	30	80	52.7	17184	PASS
95	95	100	100	100.0	32627	PASS
96	95	5	9	6.8	2229	PASS
173	174	0.00	2	1.0	219	PASS
174	95	50	120	66.8	21811	PASS
175	174	5	9	7.3	1589	PASS
176	174	95	101	95.8	20893	PASS
177	176	5	9	7.2	1512	PASS

Scan 2877 (10.590 min): VU053189.D\data.ms
BFB163

m/z	Abundance
36.10	476.0
38.10	179.0
40.00	105.0
44.00	152.0

Instrument :
MSVOA_U
ClientSampleId :
BFB163

m/z	Abundance
35.10	102.0
36.10	582.0
37.10	1425.0
38.10	1309.0
39.10	424.0
40.10	151.0
44.00	256.0
45.00	213.0
47.10	268.0
48.10	186.0
49.10	1371.0
50.10	6515.0
51.20	2045.0
55.00	123.0
56.10	514.0
57.10	1070.0
60.10	355.0
61.10	1790.0
62.10	1502.0
63.10	1182.0
64.00	151.0
68.10	3616.0
69.10	3456.0
70.10	252.0
72.10	167.0
73.10	1508.0
74.10	5520.0
75.10	17656.0
76.10	1765.0
77.00	179.0
78.00	184.0
79.00	1334.0
80.00	403.0
81.00	1415.0
82.00	279.0
87.10	1552.0
88.10	1560.0
91.00	148.0
92.10	1012.0
93.10	1594.0
94.10	4271.0
95.10	33408.0
96.10	2552.0
97.10	110.0
104.00	122.0
106.00	132.0
115.90	140.0
116.90	193.0
118.00	173.0
119.00	162.0
141.00	244.0
143.00	301.0
172.90	178.0
174.10	22432.0
175.10	1668.0
176.10	20816.0
177.00	1629.0

Instrument :
MSVOA_U
ClientSampleId :
BFB163

m/z	Abundance
36.10	575.0
37.10	1401.0
38.10	1346.0
39.10	454.0
40.00	115.0
44.00	277.0
45.00	233.0
47.00	255.0
48.10	173.0
49.10	1270.0
50.10	6564.0
51.20	1955.0
55.00	155.0
56.10	486.0
57.10	1024.0
60.10	335.0
61.10	1664.0
62.10	1578.0
63.10	1266.0
64.10	160.0
68.10	3663.0
69.10	3495.0
70.10	234.0
72.10	118.0
73.10	1417.0
74.10	5752.0
75.10	17664.0
76.10	1655.0
77.00	162.0
78.10	197.0
79.00	1389.0
80.00	366.0
81.00	1410.0
82.10	302.0
87.10	1532.0
88.10	1619.0
91.00	128.0
92.10	1004.0
93.10	1664.0
94.10	4402.0
95.10	33728.0
96.10	2272.0
104.00	105.0
106.00	112.0
115.90	151.0
117.00	191.0
118.00	192.0
118.90	142.0
135.00	111.0
141.00	303.0
143.00	281.0
172.90	226.0
174.10	22320.0
175.10	1640.0
176.10	21480.0
177.00	1577.0

Instrument :
MSVOA_U
ClientSampleId :
BFB163

m/z	Abundance
36.10	551.0
37.10	1292.0
38.10	1200.0
39.10	429.0
44.10	344.0
45.00	241.0
47.10	237.0
48.10	146.0
49.10	1095.0
50.10	5998.0
51.10	1704.0
55.10	152.0
56.10	415.0
57.10	911.0
60.00	321.0
61.10	1398.0
62.10	1517.0
63.10	1180.0
64.10	141.0
68.10	3367.0
69.10	3236.0
70.10	216.0
73.10	1273.0
74.10	5577.0
75.10	16231.0
76.10	1440.0
77.00	143.0
78.10	178.0
79.00	1286.0
80.00	305.0
81.00	1270.0
82.10	322.0
87.10	1309.0
88.10	1462.0
92.10	907.0
93.10	1541.0
94.10	4162.0
95.10	30744.0
96.10	1864.0
106.00	117.0
115.90	132.0
117.00	176.0
118.00	150.0
118.90	153.0
141.10	334.0
143.00	272.0
173.00	254.0
174.10	20680.0
175.10	1458.0
176.10	20384.0
177.00	1329.0

Instrument :
MSVOA_U
ClientSampleId :
BFB163