

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031619\
 Data File : VU030100.D
 Acq On : 15 Mar 2019 10:59
 Operator : JC/SP
 Sample : K1859-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	37	rVB2	10222	9698	0.60%	0.073%
2	1.350	78	81	83	rBV	1051	614	0.04%	0.005%
3	1.399	88	96	108	rBV	238133	240664	14.91%	1.822%
4	1.678	175	183	199	rBV	170532	223360	13.83%	1.691%
5	1.884	243	247	253	rBV3	3170	3516	0.22%	0.027%
6	2.270	356	367	381	rBV	377303	583246	36.12%	4.416%
7	2.376	398	400	402	rBV2	427	247	0.02%	0.002%
8	2.437	416	419	421	rBV3	796	444	0.03%	0.003%
9	2.476	425	431	443	rVB3	2566	4441	0.28%	0.034%
10	2.530	443	448	450	rBV2	496	422	0.03%	0.003%
11	2.543	450	452	455	rVB	405	196	0.01%	0.001%
12	2.556	455	456	459	rVB	762	314	0.02%	0.002%
13	2.591	459	467	469	rBV2	970	915	0.06%	0.007%
14	2.608	469	472	474	rBV	866	590	0.04%	0.004%
15	2.636	478	481	482	rBV2	377	160	0.01%	0.001%
16	2.691	494	498	501	rBV3	1674	1426	0.09%	0.011%
17	2.733	508	511	513	rBV	653	407	0.03%	0.003%
18	2.746	513	515	518	rVB2	737	399	0.02%	0.003%
19	2.762	518	520	522	rBV2	683	434	0.03%	0.003%
20	2.775	522	524	526	rVB2	709	326	0.02%	0.002%
21	2.794	526	530	531	rBV2	444	325	0.02%	0.002%
22	2.881	554	557	561	rBV	984	677	0.04%	0.005%
23	2.903	561	564	567	rVV2	565	426	0.03%	0.003%
24	2.929	569	572	575	rVB	770	480	0.03%	0.004%
25	2.945	575	577	580	rBV	577	436	0.03%	0.003%
26	2.984	581	589	592	rBV4	1528	1503	0.09%	0.011%
27	3.019	597	600	605	rVV3	508	651	0.04%	0.005%
28	3.042	605	607	611	rVB2	621	337	0.02%	0.003%
29	3.093	611	623	627	rBV3	1025	1585	0.10%	0.012%
30	3.112	627	629	630	rBV	230	105	0.01%	0.001%
31	3.125	630	633	637	rBV2	629	434	0.03%	0.003%
32	3.170	640	647	650	rVV	1390	1307	0.08%	0.010%
33	3.231	663	666	667	rBV2	591	328	0.02%	0.002%
34	3.263	672	676	678	rVB	336	242	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031619\
 Data File : VU030100.D
 Acq On : 15 Mar 2019 10:59
 Operator : JC/SP
 Sample : K1859-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

35	3.305	686	689	691	rVB3	356	167	0.01%	0.001%
36	3.321	691	694	698	rBV	664	593	0.04%	0.004%
37	3.344	698	701	705	rVV2	459	313	0.02%	0.002%
38	3.366	705	708	709	rVV2	390	205	0.01%	0.002%
39	3.379	709	712	714	rVV3	777	531	0.03%	0.004%
40	3.402	716	719	723	rVB	1238	866	0.05%	0.007%
41	3.431	723	728	730	rVB2	368	311	0.02%	0.002%
42	3.453	730	735	737	rBV	707	582	0.04%	0.004%
43	3.489	743	746	747	rBV2	651	350	0.02%	0.003%
44	3.556	764	767	771	rVB	1093	743	0.05%	0.006%
45	3.579	771	774	776	rBV	756	523	0.03%	0.004%
46	3.624	785	788	790	rBV2	618	330	0.02%	0.002%
47	3.672	800	803	806	rBV	536	336	0.02%	0.003%
48	3.688	806	808	811	rVB	655	354	0.02%	0.003%
49	3.710	811	815	821	rBV2	810	958	0.06%	0.007%
50	3.771	832	834	837	rBV	703	492	0.03%	0.004%
51	3.800	837	843	850	rVB3	1306	1753	0.11%	0.013%
52	3.862	859	862	863	rBV	321	188	0.01%	0.001%
53	3.874	863	866	868	rVV2	706	442	0.03%	0.003%
54	3.916	874	879	880	rBV3	490	453	0.03%	0.003%
55	3.948	887	889	891	rBV2	315	147	0.01%	0.001%
56	3.961	891	893	896	rVB	506	231	0.01%	0.002%
57	3.984	896	900	903	rBV	846	720	0.04%	0.005%
58	4.071	925	927	933	rBV	584	595	0.04%	0.005%
59	4.173	946	959	993	rBV	155057	409917	25.39%	3.104%
60	4.447	1041	1044	1047	rVB	957	639	0.04%	0.005%
61	4.646	1088	1106	1128	rBV	266151	634819	39.32%	4.807%
62	5.337	1298	1321	1354	rBV2	543279	1614603	100.00%	12.225%
63	5.794	1460	1463	1465	rBV2	1082	736	0.05%	0.006%
64	5.884	1478	1491	1522	rBV	520383	1051178	65.10%	7.959%
65	6.119	1561	1564	1568	rBV2	1447	1086	0.07%	0.008%
66	6.328	1615	1629	1657	rBV	349994	724525	44.87%	5.486%
67	6.598	1710	1713	1718	rVB	1112	852	0.05%	0.006%
68	6.652	1728	1730	1733	rBV3	656	403	0.02%	0.003%
69	6.820	1778	1782	1785	rBV	1115	1023	0.06%	0.008%
70	6.926	1811	1815	1822	rBV2	962	1153	0.07%	0.009%
71	7.016	1839	1843	1850	rBV2	1327	1546	0.10%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031619\
 Data File : VU030100.D
 Acq On : 15 Mar 2019 10:59
 Operator : JC/SP
 Sample : K1859-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

72	7.138	1878	1881	1883	rBV	998	784	0.05%	0.006%
73	7.225	1896	1908	1932	rBV	205133	375599	23.26%	2.844%
74	7.385	1956	1958	1959	rBV	834	333	0.02%	0.003%
75	7.463	1979	1982	1984	rBV2	1422	852	0.05%	0.006%
76	7.562	2001	2013	2053	rBV	736479	1339824	82.98%	10.144%
77	7.845	2091	2101	2121	rBV	139574	245456	15.20%	1.858%
78	8.176	2193	2204	2216	rBV2	22972	43370	2.69%	0.328%
79	8.308	2234	2245	2278	rVB	523994	920376	57.00%	6.969%
80	9.086	2474	2487	2513	rBV	767050	1301081	80.58%	9.851%
81	9.463	2602	2604	2605	rBV	513	205	0.01%	0.002%
82	9.511	2616	2619	2623	rBV	1163	684	0.04%	0.005%
83	9.588	2641	2643	2649	rBV3	524	568	0.04%	0.004%
84	9.617	2649	2652	2654	rBV	834	596	0.04%	0.005%
85	10.125	2804	2810	2813	rBV	1456	1525	0.09%	0.012%
86	10.366	2883	2885	2888	rBV	793	450	0.03%	0.003%
87	10.427	2892	2904	2924	rBV	544764	878039	54.38%	6.648%
88	10.604	2951	2959	2970	rBV4	6278	11409	0.71%	0.086%
89	10.864	3038	3040	3042	rBV2	922	540	0.03%	0.004%
90	10.913	3053	3055	3058	rBV2	962	587	0.04%	0.004%
91	11.411	3207	3210	3214	rBV4	1871	1821	0.11%	0.014%
92	11.482	3220	3232	3256	rBV	797561	1294035	80.15%	9.798%
93	11.810	3331	3334	3335	rBV	1217	774	0.05%	0.006%
94	11.858	3337	3349	3369	rVV	759364	1251354	77.50%	9.475%
95	13.765	3938	3942	3943	rBV2	2364	1824	0.11%	0.014%


Sum of corrected areas: 13207404

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU031619\
Data File : VU030100.D
Acq On : 15 Mar 2019 10:59
Operator : JC/SP
Sample : K1859-07
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

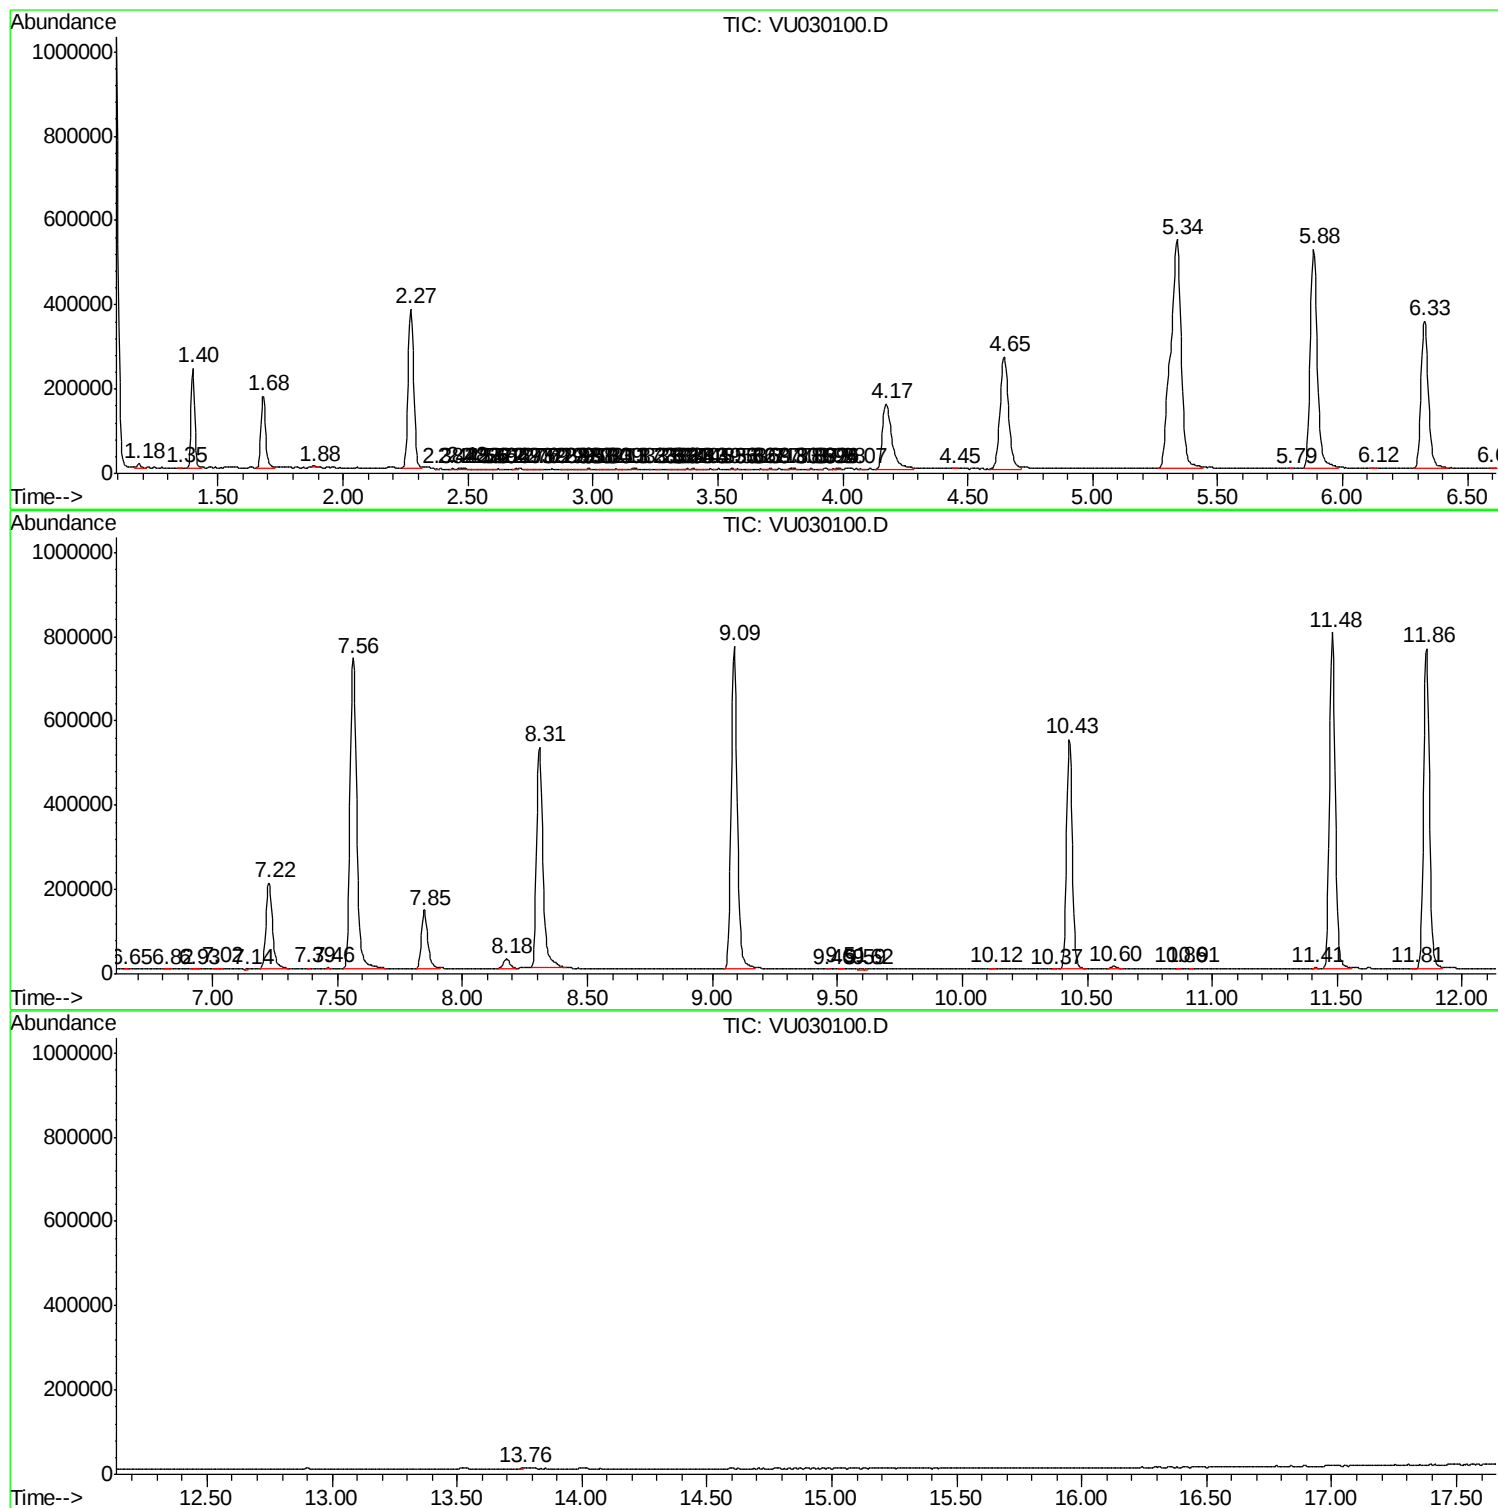

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031619\
Data File : VU030100.D
Acq On : 15 Mar 2019 10:59
Operator : JC/SP
Sample : K1859-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031619\
Data File : VU030100.D
Acq On : 15 Mar 2019 10:59
Operator : JC/SP
Sample : K1859-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc