

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031619\
 Data File : VU030105.D
 Acq On : 15 Mar 2019 12:54
 Operator : JC/SP
 Sample : K1936-20 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1B5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	35	rVB2	10790	9447	0.58%	0.068%
2	1.399	89	96	109	rBV	172223	174691	10.81%	1.256%
3	1.678	175	183	196	rBV	144553	185347	11.47%	1.333%
4	2.270	356	367	380	rBV	315307	479540	29.67%	3.449%
5	2.440	414	420	422	rBV3	1706	1767	0.11%	0.013%
6	2.624	472	477	480	rBV	1643	1836	0.11%	0.013%
7	2.672	487	492	495	rVB	1672	1244	0.08%	0.009%
8	2.698	495	500	506	rBV2	2449	2755	0.17%	0.020%
9	2.784	523	527	532	rVB	1675	1461	0.09%	0.011%
10	3.215	657	661	665	rBV2	1023	935	0.06%	0.007%
11	3.447	731	733	739	rVB	1375	1171	0.07%	0.008%
12	3.524	751	757	760	rBV	1245	1102	0.07%	0.008%
13	3.730	814	821	825	rBV	1944	2251	0.14%	0.016%
14	3.855	856	860	865	rBV	1029	1039	0.06%	0.007%
15	3.997	901	904	910	rVV	1015	1056	0.07%	0.008%
16	4.106	935	938	944	rVB	993	822	0.05%	0.006%
17	4.173	947	959	991	rBV	173654	489507	30.28%	3.521%
18	4.418	1033	1035	1041	rVB	1209	1048	0.06%	0.008%
19	4.524	1064	1068	1071	rVB	1541	1152	0.07%	0.008%
20	4.572	1078	1083	1087	rBV	1176	1308	0.08%	0.009%
21	4.646	1087	1106	1130	rBV	269047	647112	40.03%	4.654%
22	4.968	1203	1206	1210	rBV	1640	1430	0.09%	0.010%
23	5.048	1228	1231	1237	rBV2	1115	1308	0.08%	0.009%
24	5.103	1245	1248	1250	rBV2	1273	870	0.05%	0.006%
25	5.119	1251	1253	1258	rVB	1910	1256	0.08%	0.009%
26	5.144	1258	1261	1265	rBV	1124	1050	0.06%	0.008%
27	5.244	1288	1292	1295	rVB	1267	893	0.06%	0.006%
28	5.337	1295	1321	1348	rBV2	541040	1616482	100.00%	11.627%
29	5.479	1362	1365	1368	rVB	1223	842	0.05%	0.006%
30	5.591	1397	1400	1407	rBV	883	973	0.06%	0.007%
31	5.633	1407	1413	1415	rBV3	1144	1117	0.07%	0.008%
32	5.810	1465	1468	1471	rBV	1027	908	0.06%	0.007%
33	5.884	1478	1491	1523	rBV	534132	1084900	67.11%	7.803%
34	6.087	1550	1554	1560	rVB3	1252	1721	0.11%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031619\
 Data File : VU030105.D
 Acq On : 15 Mar 2019 12:54
 Operator : JC/SP
 Sample : K1936-20 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1B5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

35	6.189	1576	1586	1592	rBV4	6932	12467	0.77%	0.090%
36	6.328	1616	1629	1662	rVV	359568	734913	45.46%	5.286%
37	6.521	1686	1689	1694	rBV	1370	1288	0.08%	0.009%
38	6.588	1708	1710	1716	rVB3	1484	1187	0.07%	0.009%
39	6.707	1739	1747	1751	rBV2	1464	1741	0.11%	0.013%
40	6.900	1802	1807	1813	rVB4	1306	1557	0.10%	0.011%
41	6.935	1813	1818	1824	rVB2	1264	1619	0.10%	0.012%
42	6.971	1824	1829	1831	rBV	1104	830	0.05%	0.006%
43	7.000	1833	1838	1839	rBV3	1134	915	0.06%	0.007%
44	7.058	1850	1856	1859	rVB	1214	1031	0.06%	0.007%
45	7.225	1896	1908	1942	rVV	208604	388893	24.06%	2.797%
46	7.373	1951	1954	1958	rBV2	1346	970	0.06%	0.007%
47	7.431	1967	1972	1975	rBV4	1705	1859	0.12%	0.013%
48	7.476	1979	1986	1991	rVB3	2422	3171	0.20%	0.023%
49	7.562	2000	2013	2044	rBV	720945	1316053	81.41%	9.466%
50	7.849	2091	2102	2117	rBV	139496	245367	15.18%	1.765%
51	8.006	2148	2151	2156	rVB2	1326	1010	0.06%	0.007%
52	8.141	2189	2193	2194	rBV	1242	842	0.05%	0.006%
53	8.177	2194	2204	2210	rVV2	29076	53111	3.29%	0.382%
54	8.225	2210	2219	2235	rVV	221652	396537	24.53%	2.852%
55	8.308	2235	2245	2281	rVB	585710	1029145	63.67%	7.402%
56	8.710	2366	2370	2373	rVB	1012	893	0.06%	0.006%
57	8.771	2382	2389	2390	rBV2	1414	1225	0.08%	0.009%
58	9.038	2469	2472	2474	rBV	1180	819	0.05%	0.006%
59	9.086	2474	2487	2520	rBV	783223	1350787	83.56%	9.716%
60	9.308	2553	2556	2560	rVB	1384	989	0.06%	0.007%
61	9.334	2560	2564	2568	rBV	1957	1723	0.11%	0.012%
62	9.382	2571	2579	2588	rVB2	2610	3925	0.24%	0.028%
63	9.421	2588	2591	2597	rVB	1679	1497	0.09%	0.011%
64	9.456	2597	2602	2603	rBV	1238	1093	0.07%	0.008%
65	9.578	2635	2640	2644	rBV2	1330	1574	0.10%	0.011%
66	9.729	2684	2687	2693	rVB	1811	1673	0.10%	0.012%
67	9.758	2693	2696	2697	rBV	1383	809	0.05%	0.006%
68	9.961	2754	2759	2762	rBV2	1506	1219	0.08%	0.009%
69	9.984	2762	2766	2773	rBV	739	879	0.05%	0.006%
70	10.135	2806	2813	2816	rBV2	1442	1887	0.12%	0.014%
71	10.212	2832	2837	2841	rBV2	1749	1820	0.11%	0.013%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031619\
 Data File : VU030105.D
 Acq On : 15 Mar 2019 12:54
 Operator : JC/SP
 Sample : K1936-20 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1B5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

72	10.238	2841	2845	2847	rBV	1577	1138	0.07%	0.008%
73	10.279	2852	2858	2862	rVB2	1214	1213	0.08%	0.009%
74	10.305	2862	2866	2869	rBV	1584	1364	0.08%	0.010%
75	10.427	2891	2904	2924	rBV	593247	956647	59.18%	6.881%
76	10.511	2927	2930	2934	rVV	2461	2070	0.13%	0.015%
77	10.559	2942	2945	2950	rVV3	1315	1546	0.10%	0.011%
78	10.604	2950	2959	2972	rVB3	17906	32588	2.02%	0.234%
79	10.897	3047	3050	3055	rVB	1406	1151	0.07%	0.008%
80	10.958	3060	3069	3074	rBV2	1748	2824	0.17%	0.020%
81	11.054	3096	3099	3105	rVB3	1007	1012	0.06%	0.007%
82	11.315	3177	3180	3184	rBV2	1140	1040	0.06%	0.007%
83	11.408	3205	3209	3210	rBV	1346	981	0.06%	0.007%
84	11.482	3220	3232	3249	rBV	808065	1290609	79.84%	9.283%
85	11.726	3305	3308	3310	rBV	1246	832	0.05%	0.006%
86	11.858	3336	3349	3367	rBV	784377	1299356	80.38%	9.346%
87	12.167	3442	3445	3448	rBV	1277	932	0.06%	0.007%
88	12.405	3513	3519	3522	rBV	1491	1821	0.11%	0.013%
89	12.627	3585	3588	3592	rBV	1531	1092	0.07%	0.008%
90	12.890	3667	3670	3673	rBV3	1209	952	0.06%	0.007%
91	12.948	3685	3688	3695	rVB	1673	1674	0.10%	0.012%
92	12.980	3695	3698	3700	rBV2	1124	806	0.05%	0.006%
93	13.019	3707	3710	3711	rBV	1491	899	0.06%	0.006%
94	13.173	3754	3758	3763	rBV2	2031	2044	0.13%	0.015%
95	13.739	3931	3934	3936	rBV	1532	1026	0.06%	0.007%
96	13.835	3961	3964	3967	rVB	1982	1102	0.07%	0.008%
97	13.938	3993	3996	4001	rBV3	1347	1080	0.07%	0.008%
98	13.977	4006	4008	4013	rVB	1955	1388	0.09%	0.010%
99	14.170	4065	4068	4070	rBV	1225	868	0.05%	0.006%
100	14.276	4094	4101	4108	rBV3	3670	5406	0.33%	0.039%


Sum of corrected areas: 13903120

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU031619\
Data File : VU030105.D
Acq On : 15 Mar 2019 12:54
Operator : JC/SP
Sample : K1936-20 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1B5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

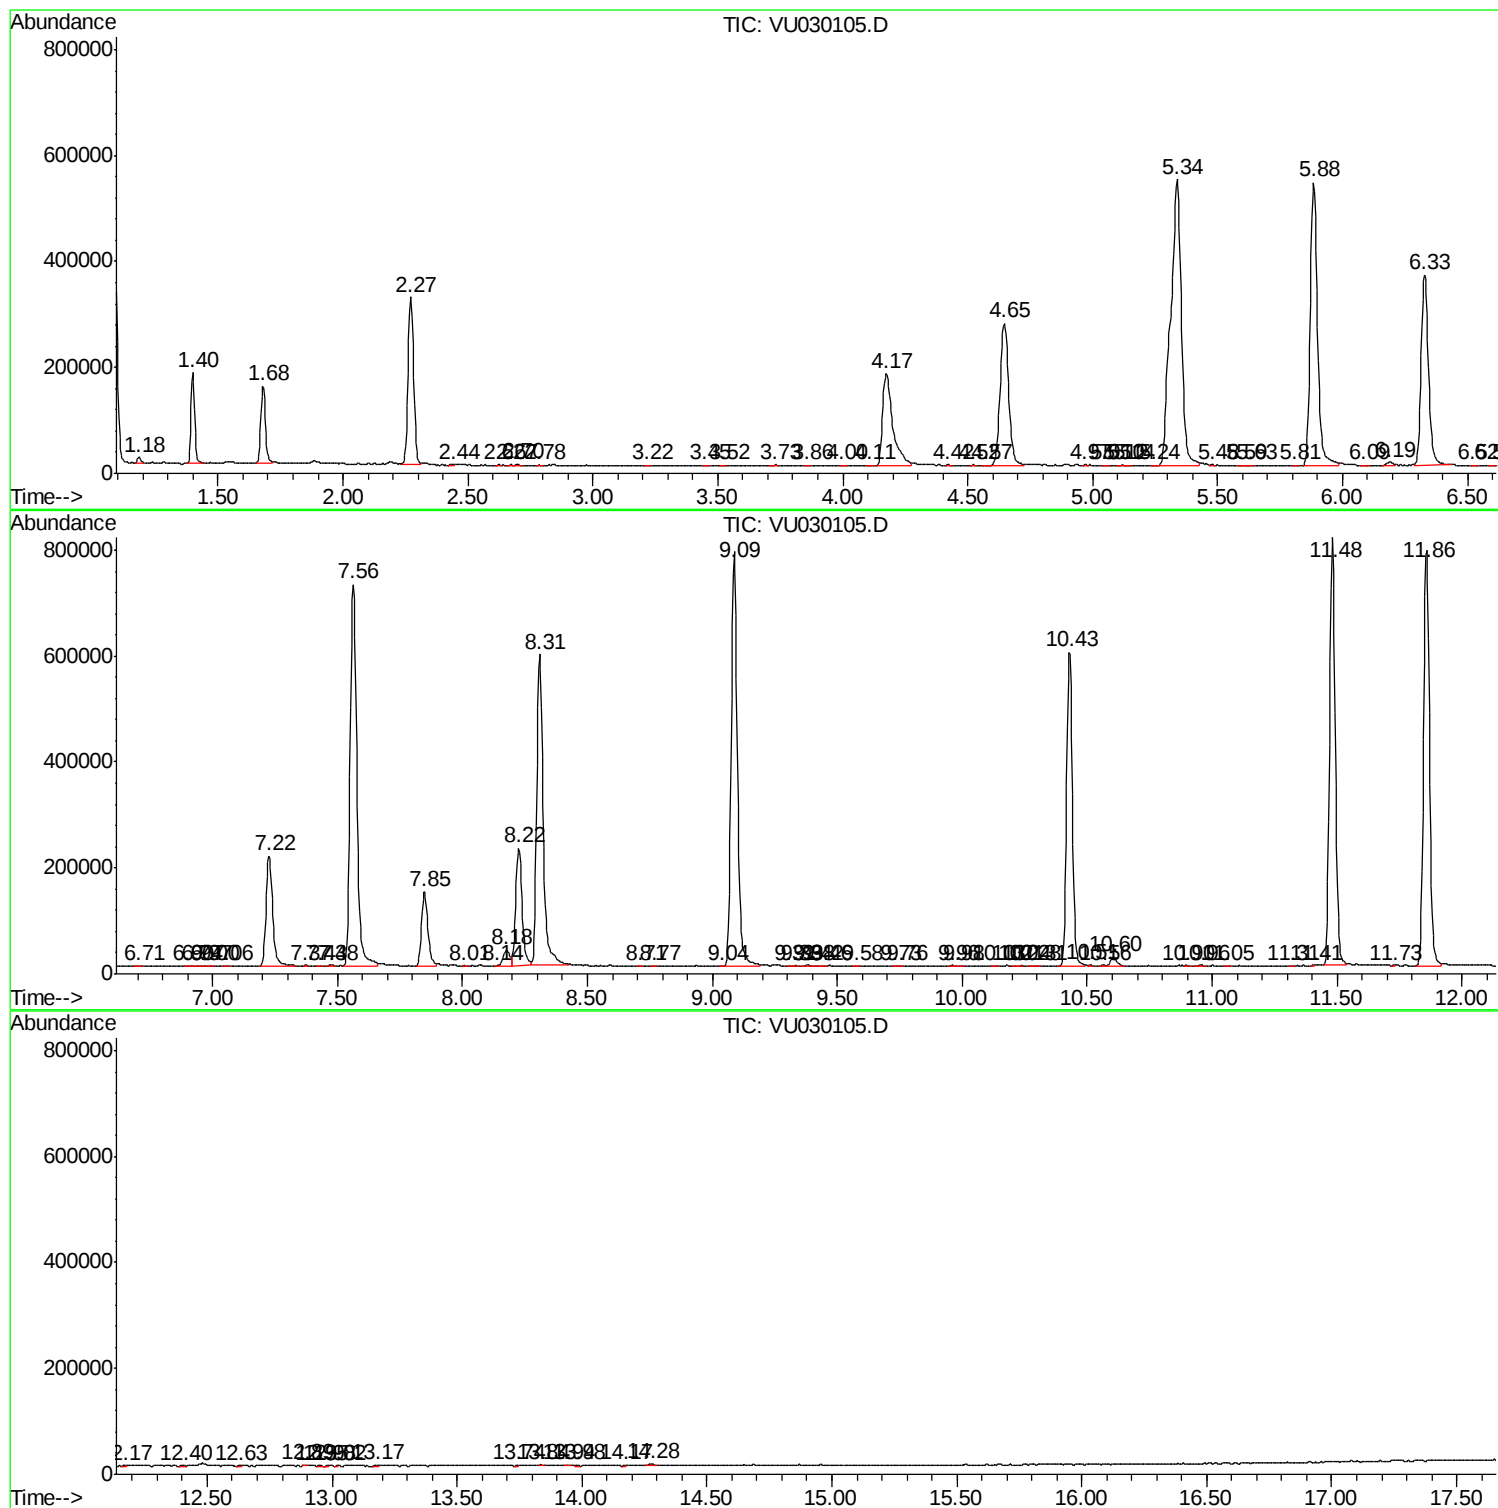

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031619\
Data File : VU030105.D
Acq On : 15 Mar 2019 12:54
Operator : JC/SP
Sample : K1936-20 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1B5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031619\
Data File : VU030105.D
Acq On : 15 Mar 2019 12:54
Operator : JC/SP
Sample : K1936-20 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1B5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc