

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031619\
 Data File : VU030106.D
 Acq On : 15 Mar 2019 13:17
 Operator : JC/SP
 Sample : K1936-21 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1C8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	36	rBV2	11701	11955	0.74%	0.088%
2	1.399	89	96	106	rBV	178177	175335	10.85%	1.297%
3	1.678	175	183	198	rBV	145286	186882	11.57%	1.382%
4	2.270	357	367	380	rBV	314492	474381	29.37%	3.508%
5	2.415	408	412	416	rBV2	1231	1328	0.08%	0.010%
6	2.672	488	492	493	rBV2	1360	875	0.05%	0.006%
7	2.701	495	501	515	rVB3	7522	11816	0.73%	0.087%
8	3.366	704	708	710	rBV	1211	923	0.06%	0.007%
9	3.585	773	776	780	rVB	1738	1139	0.07%	0.008%
10	4.093	930	934	937	rVB2	1457	1148	0.07%	0.008%
11	4.173	947	959	990	rBV	170340	447182	27.68%	3.307%
12	4.646	1085	1106	1128	rBV	270174	645755	39.98%	4.776%
13	5.337	1297	1321	1359	rBV2	538308	1615253	100.00%	11.946%
14	5.591	1397	1400	1406	rBV	1120	1241	0.08%	0.009%
15	5.788	1458	1461	1466	rVB2	1467	1299	0.08%	0.010%
16	5.884	1477	1491	1515	rBV	540722	1086718	67.28%	8.037%
17	6.109	1556	1561	1564	rBV2	1021	1087	0.07%	0.008%
18	6.151	1569	1574	1576	rBV3	1368	1564	0.10%	0.012%
19	6.183	1576	1584	1588	rBV4	2620	3507	0.22%	0.026%
20	6.328	1615	1629	1651	rBV	357373	725632	44.92%	5.366%
21	6.521	1685	1689	1694	rVB	1792	1483	0.09%	0.011%
22	6.546	1694	1697	1700	rBV2	1129	1010	0.06%	0.007%
23	6.624	1716	1721	1724	rBV	1339	1414	0.09%	0.010%
24	6.681	1734	1739	1743	rVB3	971	856	0.05%	0.006%
25	6.714	1746	1749	1755	rVB2	1057	1109	0.07%	0.008%
26	6.746	1755	1759	1762	rBV	1066	1004	0.06%	0.007%
27	6.865	1792	1796	1800	rBV4	1003	1015	0.06%	0.008%
28	7.051	1850	1854	1857	rBV	1166	1133	0.07%	0.008%
29	7.083	1861	1864	1868	rBV	1440	1224	0.08%	0.009%
30	7.138	1879	1881	1888	rVB3	1074	1118	0.07%	0.008%
31	7.173	1888	1892	1895	rBV	1282	1024	0.06%	0.008%
32	7.225	1895	1908	1931	rBV	200016	369120	22.85%	2.730%
33	7.389	1956	1959	1966	rVB2	897	1077	0.07%	0.008%
34	7.424	1966	1970	1974	rVB2	1457	1083	0.07%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031619\
 Data File : VU030106.D
 Acq On : 15 Mar 2019 13:17
 Operator : JC/SP
 Sample : K1936-21 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1C8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

35	7.463	1974	1982	1983	rBV3	1423	1787	0.11%	0.013%
36	7.562	1998	2013	2033	rBV	720324	1285543	79.59%	9.507%
37	7.849	2091	2102	2125	rBV	142026	250170	15.49%	1.850%
38	8.025	2154	2157	2160	rBV2	1358	1001	0.06%	0.007%
39	8.106	2177	2182	2185	rBV	891	966	0.06%	0.007%
40	8.177	2193	2204	2210	rVV	24838	42592	2.64%	0.315%
41	8.225	2210	2219	2234	rVV2	107177	190114	11.77%	1.406%
42	8.308	2234	2245	2276	rVV	560956	1002156	62.04%	7.411%
43	8.623	2341	2343	2348	rVB	1608	1321	0.08%	0.010%
44	8.662	2348	2355	2360	rBV2	1916	2946	0.18%	0.022%
45	8.710	2366	2370	2376	rBV2	1158	1373	0.09%	0.010%
46	8.858	2413	2416	2420	rVB	1132	898	0.06%	0.007%
47	8.964	2446	2449	2454	rVB	919	863	0.05%	0.006%
48	9.025	2465	2468	2474	rVB	1243	1376	0.09%	0.010%
49	9.086	2474	2487	2509	rBV	789206	1351545	83.67%	9.995%
50	9.289	2546	2550	2553	rBV	1278	907	0.06%	0.007%
51	9.366	2569	2574	2577	rBV2	1253	1356	0.08%	0.010%
52	9.469	2603	2606	2609	rVV	1273	869	0.05%	0.006%
53	9.688	2669	2674	2677	rVB	1312	1212	0.08%	0.009%
54	9.755	2693	2695	2699	rBV3	945	922	0.06%	0.007%
55	9.848	2721	2724	2728	rVB	1263	1067	0.07%	0.008%
56	9.919	2740	2746	2750	rVB	1016	957	0.06%	0.007%
57	10.019	2774	2777	2782	rBV	1546	1277	0.08%	0.009%
58	10.051	2782	2787	2790	rBV2	937	900	0.06%	0.007%
59	10.103	2799	2803	2806	rBV2	1629	1583	0.10%	0.012%
60	10.131	2810	2812	2816	rVV2	1282	955	0.06%	0.007%
61	10.157	2816	2820	2822	rVV	936	973	0.06%	0.007%
62	10.225	2835	2841	2845	rBV	2175	2274	0.14%	0.017%
63	10.279	2854	2858	2861	rBV	1785	1391	0.09%	0.010%
64	10.299	2861	2864	2868	rVV	1589	1418	0.09%	0.010%
65	10.321	2868	2871	2875	rVB	1656	1344	0.08%	0.010%
66	10.385	2887	2891	2892	rBV2	1304	858	0.05%	0.006%
67	10.427	2892	2904	2925	rVV	572778	939040	58.14%	6.945%
68	10.607	2952	2960	2970	rVB3	8816	15525	0.96%	0.115%
69	10.820	3018	3026	3033	rVB2	1207	1507	0.09%	0.011%
70	10.861	3033	3039	3045	rBV2	1531	1914	0.12%	0.014%
71	10.893	3045	3049	3059	rVB2	1445	2172	0.13%	0.016%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031619\
 Data File : VU030106.D
 Acq On : 15 Mar 2019 13:17
 Operator : JC/SP
 Sample : K1936-21 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1C8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

72	11.057	3096	3100	3103	rBV	1479	1307	0.08%	0.010%
73	11.138	3122	3125	3130	rVB2	1022	1005	0.06%	0.007%
74	11.231	3148	3154	3159	rBV	724	1177	0.07%	0.009%
75	11.392	3201	3204	3207	rBV	1024	846	0.05%	0.006%
76	11.421	3209	3213	3217	rVB3	1871	1605	0.10%	0.012%
77	11.482	3220	3232	3254	rBV	814396	1303104	80.67%	9.637%
78	11.858	3334	3349	3374	rBV	776876	1286238	79.63%	9.512%
79	12.119	3427	3430	3434	rVB	1331	939	0.06%	0.007%
80	12.427	3523	3526	3530	rBV	1038	840	0.05%	0.006%
81	12.479	3537	3542	3548	rVB2	4564	5112	0.32%	0.038%
82	12.610	3579	3583	3585	rBV	1251	1129	0.07%	0.008%
83	12.704	3606	3612	3615	rBV2	932	1059	0.07%	0.008%
84	12.752	3624	3627	3634	rVB	1262	1107	0.07%	0.008%
85	12.909	3673	3676	3682	rVB	1420	1247	0.08%	0.009%
86	12.980	3694	3698	3705	rVB2	1770	1768	0.11%	0.013%
87	13.032	3711	3714	3719	rBV2	994	1024	0.06%	0.008%
88	13.067	3719	3725	3729	rBV	1430	1382	0.09%	0.010%
89	13.102	3730	3736	3740	rBV2	1364	1804	0.11%	0.013%
90	13.305	3795	3799	3804	rBV2	1833	2292	0.14%	0.017%
91	13.434	3836	3839	3843	rVB	1686	1102	0.07%	0.008%
92	13.604	3889	3892	3894	rBV	1207	870	0.05%	0.006%
93	13.662	3907	3910	3914	rBV	1010	949	0.06%	0.007%
94	13.729	3929	3931	3939	rVB2	1473	1403	0.09%	0.010%
95	14.070	4032	4037	4041	rVB	1965	2124	0.13%	0.016%
96	14.096	4041	4045	4047	rBV2	1370	1334	0.08%	0.010%
97	14.392	4133	4137	4140	rVB	1173	1015	0.06%	0.008%
98	14.816	4266	4269	4274	rBV	1465	1007	0.06%	0.007%
99	14.845	4275	4278	4284	rVV	1130	1281	0.08%	0.009%
100	14.922	4298	4302	4306	rBV	1953	1886	0.12%	0.014%


Sum of corrected areas: 13521718

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU031619\
Data File : VU030106.D
Acq On : 15 Mar 2019 13:17
Operator : JC/SP
Sample : K1936-21 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1C8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

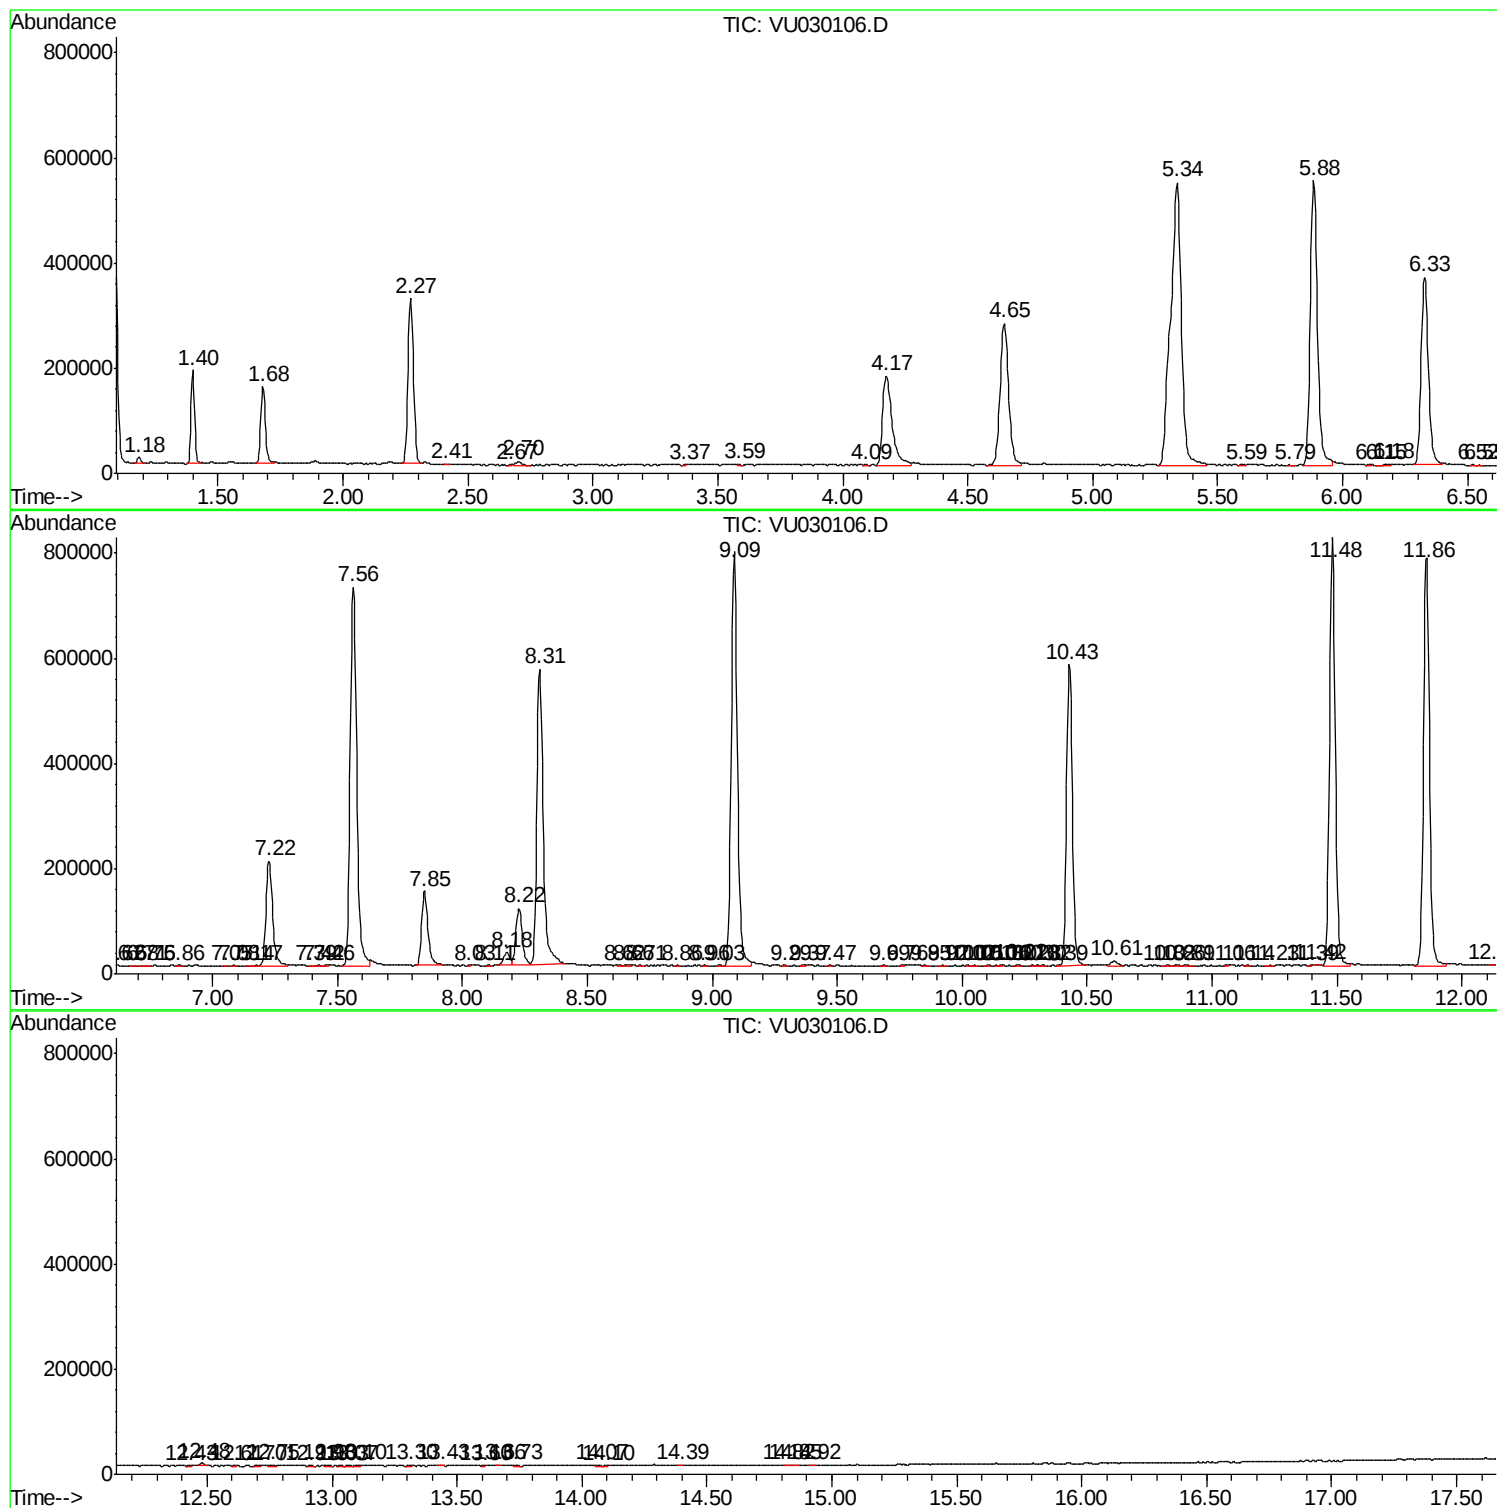

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031619\
Data File : VU030106.D
Acq On : 15 Mar 2019 13:17
Operator : JC/SP
Sample : K1936-21 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1C8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031619\
Data File : VU030106.D
Acq On : 15 Mar 2019 13:17
Operator : JC/SP
Sample : K1936-21 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1C8

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc