

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031619\
 Data File : VU030110.D
 Acq On : 15 Mar 2019 14:50
 Operator : JC/SP
 Sample : K1949-02 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1B6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	34	rVB	12747	9958	0.41%	0.061%
2	1.399	89	96	109	rBV	245871	250957	10.27%	1.542%
3	1.678	175	183	196	rBV	180495	228192	9.34%	1.402%
4	1.820	224	227	233	rBV5	2385	2709	0.11%	0.017%
5	2.270	356	367	380	rBV	401953	615569	25.19%	3.783%
6	2.537	444	450	453	rBV	1223	1372	0.06%	0.008%
7	2.585	462	465	468	rBV	1611	1076	0.04%	0.007%
8	2.701	488	501	514	rBV3	14863	25206	1.03%	0.155%
9	2.781	524	526	529	rVB	1521	855	0.03%	0.005%
10	2.804	529	533	535	rBV	1432	1213	0.05%	0.007%
11	2.833	539	542	544	rVV	1533	1254	0.05%	0.008%
12	2.862	548	551	556	rVB2	1040	955	0.04%	0.006%
13	2.894	556	561	563	rBV	811	863	0.04%	0.005%
14	3.003	589	595	599	rVV2	1099	1415	0.06%	0.009%
15	3.096	619	624	627	rBV	981	978	0.04%	0.006%
16	3.215	654	661	663	rBV	1133	1246	0.05%	0.008%
17	3.273	675	679	681	rBV	1126	770	0.03%	0.005%
18	3.286	681	683	688	rVV2	1765	1469	0.06%	0.009%
19	3.309	688	690	696	rVB	1110	806	0.03%	0.005%
20	3.373	706	710	712	rVV2	1127	791	0.03%	0.005%
21	3.389	712	715	718	rVB2	1466	847	0.03%	0.005%
22	3.450	731	734	737	rBV	1334	847	0.03%	0.005%
23	3.498	745	749	756	rVB2	1394	2058	0.08%	0.013%
24	3.540	756	762	765	rBV	1385	1558	0.06%	0.010%
25	3.591	775	778	780	rBV	1583	1119	0.05%	0.007%
26	3.842	852	856	859	rBV2	1335	923	0.04%	0.006%
27	3.919	876	880	886	rBV	2023	1950	0.08%	0.012%
28	3.974	892	897	898	rBV	1077	924	0.04%	0.006%
29	4.016	908	910	916	rBV	1245	1219	0.05%	0.007%
30	4.071	923	927	933	rBV	879	903	0.04%	0.006%
31	4.173	945	959	990	rBV	163312	452260	18.50%	2.780%
32	4.485	1052	1056	1058	rBV	1528	1110	0.05%	0.007%
33	4.534	1068	1071	1072	rBV	1395	806	0.03%	0.005%
34	4.579	1080	1085	1088	rBV2	1198	924	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031619\
 Data File : VU030110.D
 Acq On : 15 Mar 2019 14:50
 Operator : JC/SP
 Sample : K1949-02 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1B6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

35	4.646	1088	1106	1132	rBV	283785	675834	27.65%	4.154%
36	4.797	1150	1153	1161	rVB3	1459	1448	0.06%	0.009%
37	4.884	1177	1180	1184	rVV2	1448	1303	0.05%	0.008%
38	5.189	1271	1275	1278	rBV	1173	846	0.03%	0.005%
39	5.337	1298	1321	1350	rBV2	586394	1717230	70.26%	10.554%
40	5.601	1399	1403	1408	rBV2	1029	1267	0.05%	0.008%
41	5.630	1408	1412	1417	rVV	1104	1326	0.05%	0.008%
42	5.791	1459	1462	1465	rBV	1638	1279	0.05%	0.008%
43	5.820	1468	1471	1477	rBV	1107	951	0.04%	0.006%
44	5.884	1477	1491	1515	rBV	515799	1044138	42.72%	6.417%
45	6.186	1575	1585	1600	rVV2	22812	47284	1.93%	0.291%
46	6.328	1615	1629	1648	rBV	371719	754637	30.88%	4.638%
47	6.575	1703	1706	1711	rVB	1521	1205	0.05%	0.007%
48	6.656	1728	1731	1734	rVB2	1268	866	0.04%	0.005%
49	6.694	1740	1743	1746	rBV	1283	913	0.04%	0.006%
50	6.820	1777	1782	1785	rBV	1360	1346	0.06%	0.008%
51	6.939	1815	1819	1824	rBV	1837	1534	0.06%	0.009%
52	7.051	1852	1854	1859	rVB	1587	1080	0.04%	0.007%
53	7.225	1897	1908	1930	rBV	212424	386089	15.80%	2.373%
54	7.402	1960	1963	1966	rBV	1382	1032	0.04%	0.006%
55	7.562	2001	2013	2050	rBV	774892	1411197	57.74%	8.673%
56	7.849	2091	2102	2116	rBV	145120	256201	10.48%	1.575%
57	8.177	2194	2204	2207	rBV2	23590	34432	1.41%	0.212%
58	8.225	2208	2219	2235	rVV	1414248	2444087	100.00%	15.021%
59	8.308	2236	2245	2280	rVB	557551	1011492	41.39%	6.217%
60	8.694	2362	2365	2368	rBV	1454	1311	0.05%	0.008%
61	8.913	2430	2433	2436	rBV	1709	1287	0.05%	0.008%
62	9.086	2476	2487	2517	rBV	756001	1292199	52.87%	7.942%
63	9.379	2575	2578	2583	rBV3	1539	1388	0.06%	0.009%
64	9.630	2653	2656	2663	rBV2	1270	1475	0.06%	0.009%
65	9.784	2701	2704	2708	rVB2	2068	1375	0.06%	0.008%
66	9.958	2753	2758	2761	rBV3	1036	1102	0.05%	0.007%
67	10.032	2779	2781	2784	rBV	1127	842	0.03%	0.005%
68	10.212	2834	2837	2839	rBV	1288	821	0.03%	0.005%
69	10.427	2893	2904	2923	rBV	573059	920435	37.66%	5.657%
70	10.611	2953	2961	2968	rBV4	9154	14621	0.60%	0.090%
71	10.816	3021	3025	3032	rBV2	1575	2294	0.09%	0.014%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031619\
 Data File : VU030110.D
 Acq On : 15 Mar 2019 14:50
 Operator : JC/SP
 Sample : K1949-02 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1B6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

72	10.848	3032	3035	3038	rBV2	1183	769	0.03%	0.005%
73	10.913	3052	3055	3057	rBV2	1341	804	0.03%	0.005%
74	11.215	3146	3149	3153	rBV	1734	1651	0.07%	0.010%
75	11.482	3219	3232	3258	rBV	793663	1274040	52.13%	7.830%
76	11.858	3337	3349	3373	rBV	789422	1304283	53.36%	8.016%
77	12.209	3455	3458	3461	rBV	1740	1272	0.05%	0.008%
78	12.482	3534	3543	3548	rBV3	4980	7754	0.32%	0.048%
79	12.591	3571	3577	3580	rBV2	1607	1519	0.06%	0.009%
80	12.745	3622	3625	3628	rBV3	1307	1006	0.04%	0.006%
81	12.803	3638	3643	3647	rBV	1392	1570	0.06%	0.010%
82	12.964	3688	3693	3695	rBV	1493	1219	0.05%	0.007%
83	13.086	3728	3731	3734	rBV	1626	1202	0.05%	0.007%
84	13.250	3778	3782	3785	rBV	1388	1254	0.05%	0.008%
85	13.437	3837	3840	3846	rBV	1097	1532	0.06%	0.009%
86	13.617	3891	3896	3899	rBV2	1109	1046	0.04%	0.006%
87	13.639	3899	3903	3907	rVB2	1378	1161	0.05%	0.007%
88	13.659	3907	3909	3912	rBV	1349	769	0.03%	0.005%
89	13.787	3946	3949	3952	rBV	1256	1041	0.04%	0.006%
90	13.877	3973	3977	3979	rBV2	1255	1106	0.05%	0.007%
91	13.958	3999	4002	4006	rBV	1238	865	0.04%	0.005%
92	13.980	4006	4009	4011	rBV2	1330	761	0.03%	0.005%
93	14.469	4158	4161	4167	rBV2	1511	2027	0.08%	0.012%
94	14.578	4192	4195	4199	rVB	1395	919	0.04%	0.006%
95	14.697	4229	4232	4238	rBV2	1224	1307	0.05%	0.008%
96	14.768	4248	4254	4256	rBV	1467	1583	0.06%	0.010%
97	14.832	4271	4274	4278	rVB2	2050	1558	0.06%	0.010%
98	14.996	4323	4325	4329	rVB	1763	1011	0.04%	0.006%
99	15.241	4398	4401	4404	rBV2	1326	933	0.04%	0.006%
100	15.562	4498	4501	4506	rBV2	1500	1557	0.06%	0.010%


Sum of corrected areas: 16270788

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU031619\
Data File : VU030110.D
Acq On : 15 Mar 2019 14:50
Operator : JC/SP
Sample : K1949-02 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1B6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

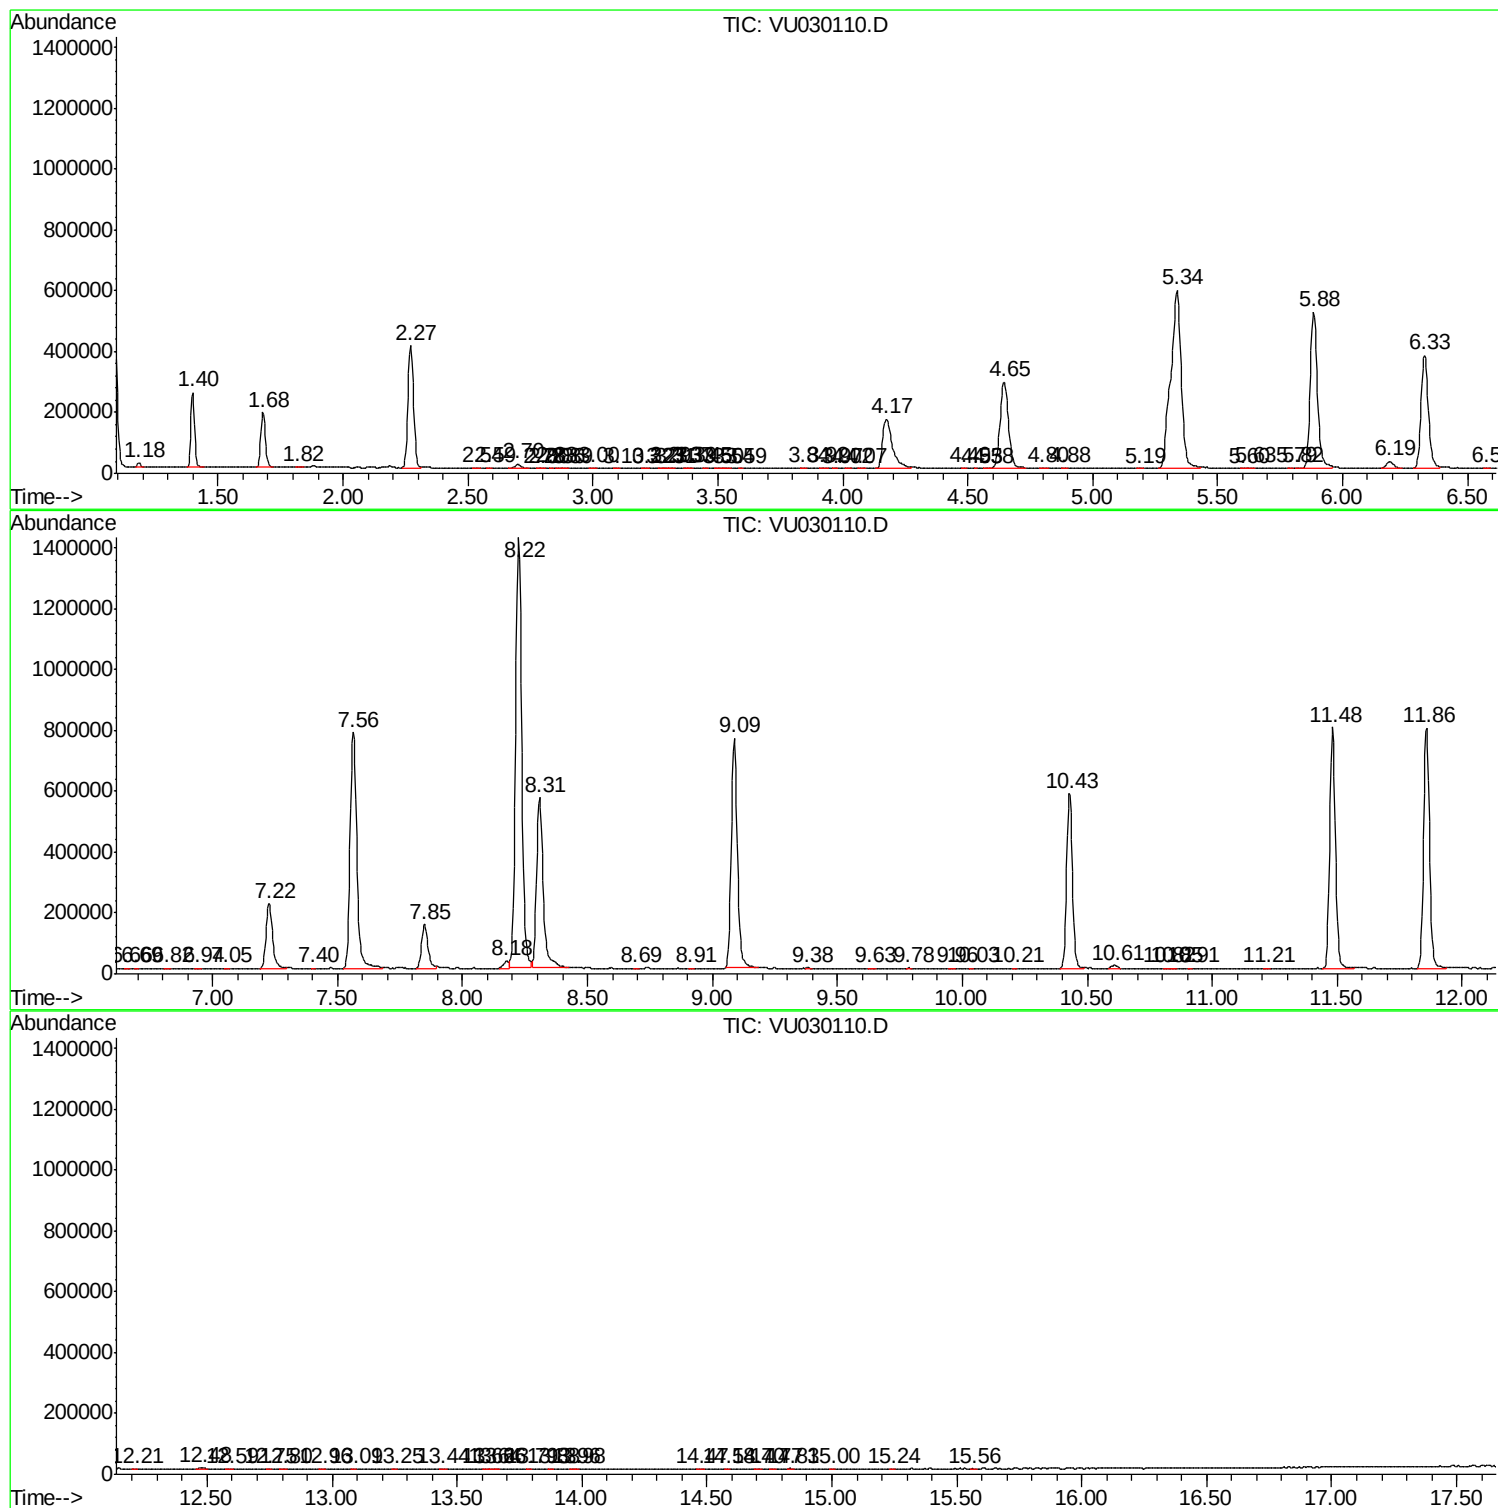

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031619\
Data File : VU030110.D
Acq On : 15 Mar 2019 14:50
Operator : JC/SP
Sample : K1949-02 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1B6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031619\
Data File : VU030110.D
Acq On : 15 Mar 2019 14:50
Operator : JC/SP
Sample : K1949-02 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1B6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc