


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU031619\
 Data File : VU030097.D
 Acq On : 15 Mar 2019 08:19
 Operator : JC/SP
 Sample : BFB34
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB34

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis
 Last Update : Mon Mar 18 12:44:57 2019

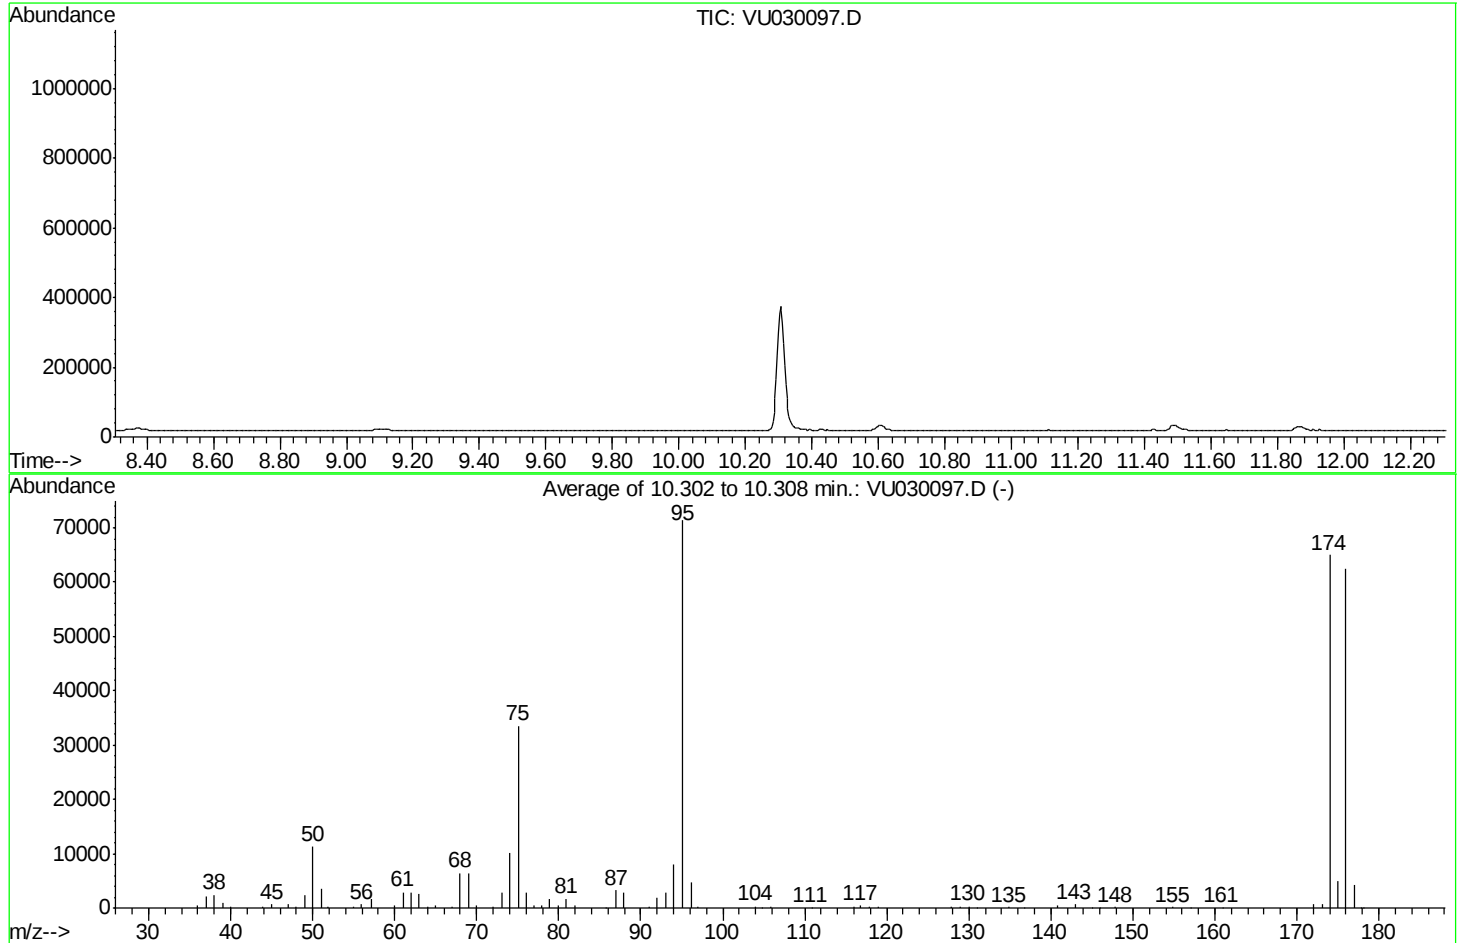

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	11281	PASS
75	95	30	80	47.0	33568	PASS
95	95	100	100	100.0	71381	PASS
96	95	5	9	6.7	4749	PASS
173	174	0.00	2	1.2	797	PASS
174	95	50	120	91.0	64957	PASS
175	174	5	9	7.5	4864	PASS
176	174	95	101	96.0	62384	PASS
177	176	5	9	6.8	4267	PASS

Scan 2854 (10.266 min): VU030097.D
BFB34

m/z	Abundance
39.10	111.0
40.00	18360.0
43.90	418.0
207.00	157.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34

m/z	Abundance
35.90	420.0
37.00	2292.0
38.00	2400.0
39.10	1106.0
40.00	18768.0
44.00	557.0
45.00	679.0
47.00	830.0
48.00	325.0
49.00	2393.0
50.00	11262.0
51.10	3511.0
51.90	171.0
54.90	197.0
55.90	642.0
57.10	1527.0
59.90	411.0
61.00	2747.0
62.00	2748.0
63.00	2506.0
64.00	270.0
65.00	512.0
66.90	129.0
68.00	6452.0
69.00	6447.0
70.00	550.0
72.00	359.0
73.00	2821.0
74.00	10017.0
75.10	32936.0
76.00	2924.0
76.90	410.0
77.80	418.0
78.90	1728.0
79.90	420.0
80.90	1728.0
82.00	325.0
87.00	3369.0
87.90	3024.0
90.90	268.0
92.00	1734.0
93.00	2894.0
94.00	7625.0
95.10	69200.0
96.10	4603.0
97.00	160.0
104.00	302.0
104.70	113.0
105.80	268.0
116.00	230.0
116.90	448.0
117.90	274.0
119.00	314.0
128.00	209.0
128.90	211.0
130.00	328.0
130.90	120.0
134.90	144.0
140.80	516.0
142.90	548.0
147.90	182.0
154.90	175.0
160.90	110.0
172.00	673.0
173.10	710.0
174.00	61544.0
175.00	4923.0
176.00	59176.0
177.00	4234.0
177.80	145.0
207.00	142.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34

m/z	Abundance
36.00	399.0
37.00	2244.0
38.00	2556.0
39.00	1117.0
40.00	18576.0
44.00	587.0
45.00	662.0
47.00	822.0
48.00	331.0
49.00	2327.0
50.00	11524.0
51.00	3608.0
51.90	140.0
54.90	231.0
56.00	714.0
57.10	1734.0
60.00	463.0
61.00	3005.0
62.00	2761.0
63.00	2555.0
63.90	278.0
65.00	447.0
67.00	150.0
68.00	6702.0
69.00	6540.0
70.00	552.0
72.10	309.0
73.00	3045.0
74.00	10451.0
75.00	34744.0
76.10	2984.0
76.90	365.0
77.80	422.0
78.90	1757.0
79.90	473.0
80.90	1763.0
82.00	389.0
85.70	125.0
87.00	3306.0
87.90	3043.0
90.90	308.0
92.00	1870.0
93.00	2929.0
94.00	8171.0
95.10	73568.0
96.10	4933.0
97.00	189.0
104.00	293.0
104.70	102.0
105.80	269.0
110.80	100.0
116.00	224.0
116.90	398.0
117.90	363.0
119.00	361.0
127.80	162.0
128.00	163.0
128.90	188.0
130.00	308.0
130.90	118.0
134.90	174.0
136.70	123.0
140.90	596.0
142.90	641.0
146.00	115.0
147.90	210.0
154.90	194.0
172.00	643.0
173.10	813.0
174.00	66968.0
175.00	5042.0
176.00	64224.0
177.00	4452.0
177.90	121.0
207.00	136.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34

m/z	Abundance
36.00	393.0
37.00	2186.0
38.00	2432.0
39.00	995.0
40.00	18552.0
44.00	590.0
45.00	614.0
47.10	849.0
48.00	310.0
49.00	2082.0
50.00	11058.0
51.00	3386.0
51.90	139.0
54.90	221.0
56.00	659.0
57.10	1701.0
60.00	491.0
61.00	2958.0
62.00	2660.0
63.00	2425.0
63.90	225.0
65.00	392.0
67.00	149.0
68.00	6213.0
69.00	6313.0
70.00	507.0
72.10	292.0
73.00	2982.0
74.00	10058.0
75.00	33024.0
76.10	2890.0
76.90	337.0
77.90	384.0
78.90	1697.0
79.90	493.0
80.90	1621.0
82.00	444.0
85.80	149.0
87.00	3061.0
88.00	2636.0
91.00	308.0
92.00	1875.0
93.00	2791.0
94.00	8047.0
95.10	71376.0
96.10	4711.0
97.00	173.0
104.00	265.0
105.80	274.0
115.90	202.0
116.80	355.0
117.80	365.0
119.00	375.0
127.80	164.0
129.00	115.0
130.00	269.0
134.90	144.0
136.80	125.0
140.90	578.0
143.00	677.0
145.00	104.0
146.00	137.0
147.90	196.0
154.90	192.0
157.00	122.0
172.00	571.0
173.10	868.0
174.00	66360.0
175.00	4627.0
176.00	63752.0
177.00	4117.0
178.10	101.0
207.00	120.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34