

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031620\
 Data File : VU037303.D
 Acq On : 16 Mar 2020 19:29
 Operator : JC/MD
 Sample : L1923-18
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Quant Time: Mar 17 02:36:23 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Mar 17 01:33:31 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	123734	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	124341	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	51624	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	29671	4.60	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.00%
7) Chloroethane-d5	1.93	69	29418	5.11	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.20%
11) 1,1-Dichloroethene-d2	2.59	63	47462	3.35	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.00%
20) 2-Butanone-d5	4.68	46	102994	52.88	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.76%
24) Chloroform-d	5.11	84	73497	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.80%
26) 1,2-Dichloroethane-d4	5.74	65	44894	5.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.40%
32) Benzene-d6	5.76	84	135231	5.13	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.60%
36) 1,2-Dichloropropane-d6	6.73	67	44020	5.09	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.80%
41) Toluene-d8	7.93	98	120635	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.00%
43) trans-1,3-Dichloropropene-	8.20	79	17933	4.66	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.20%
46) 2-Hexanone-d5	8.66	63	83473	48.65	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.30%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	36370	4.90	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.00%
64) 1,2-Dichlorobenzene-d4	12.21	152	44112	5.23	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.60%


Target Compounds					Ovalue
16) Methylene chloride	3.08	84	1162	0.122 ug/L	95




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031620\
Data File : VU037303.D
Acq On : 16 Mar 2020 19:29
Operator : JC/MD
Sample : L1923-18
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Time: Mar 17 02:36:23 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Mar 17 01:33:31 2020
Response via : Initial Calibration

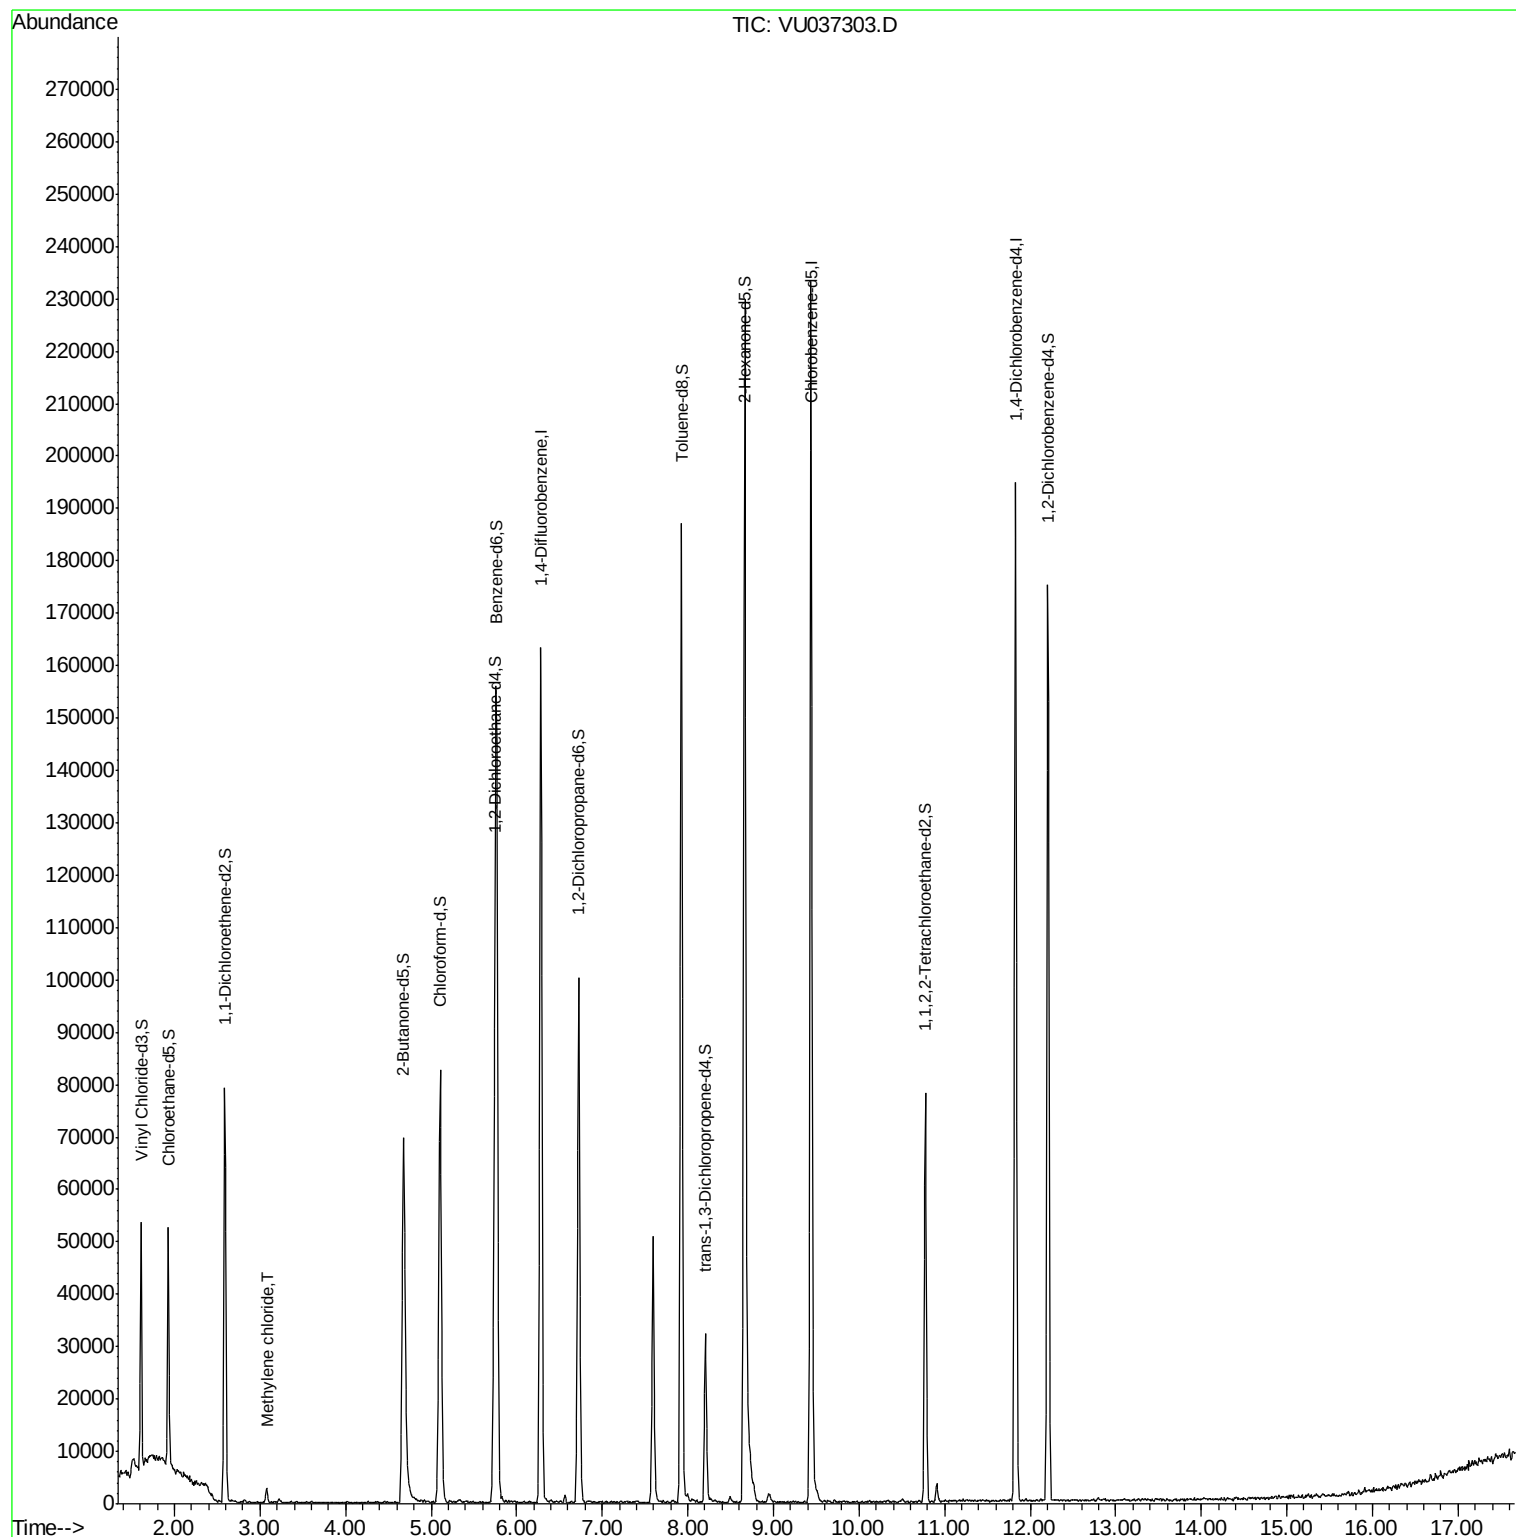

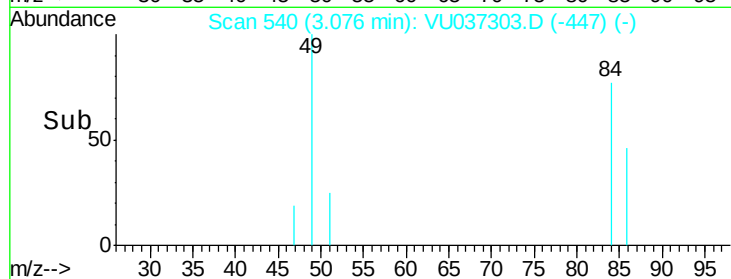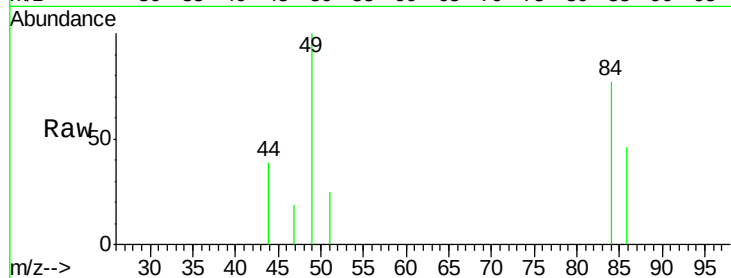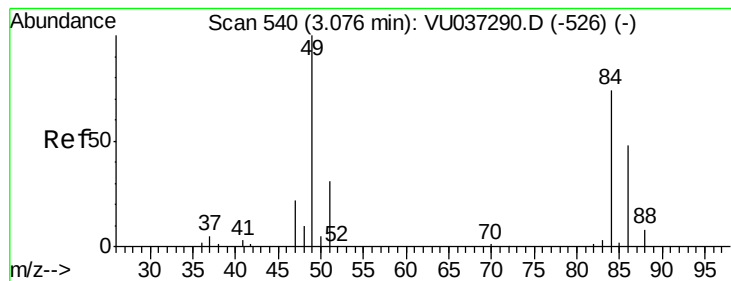

#16

Methylene chloride

Concen: 0.122 ug/L

RT: 3.08 min Scan# 540

Delta R.T. 0.00 min

Lab File: VU037303.D

Acq: 16 Mar 2020 19:29

Instrument :

MSVOA_U

ClientSampleId :

VHBLK01

Tot Ion: 84 Resp: 1162

Ion Ratio Lower Upper

84 100

86 60.2 45.2 84.0

49 129.6 94.4 175.4

