


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031620\
 Data File : VU037285.D
 Acq On : 16 Mar 2020 09:07
 Operator : JC/MD
 Sample : BFB05
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB05

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031620WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Mar 17 04:15:02 2020

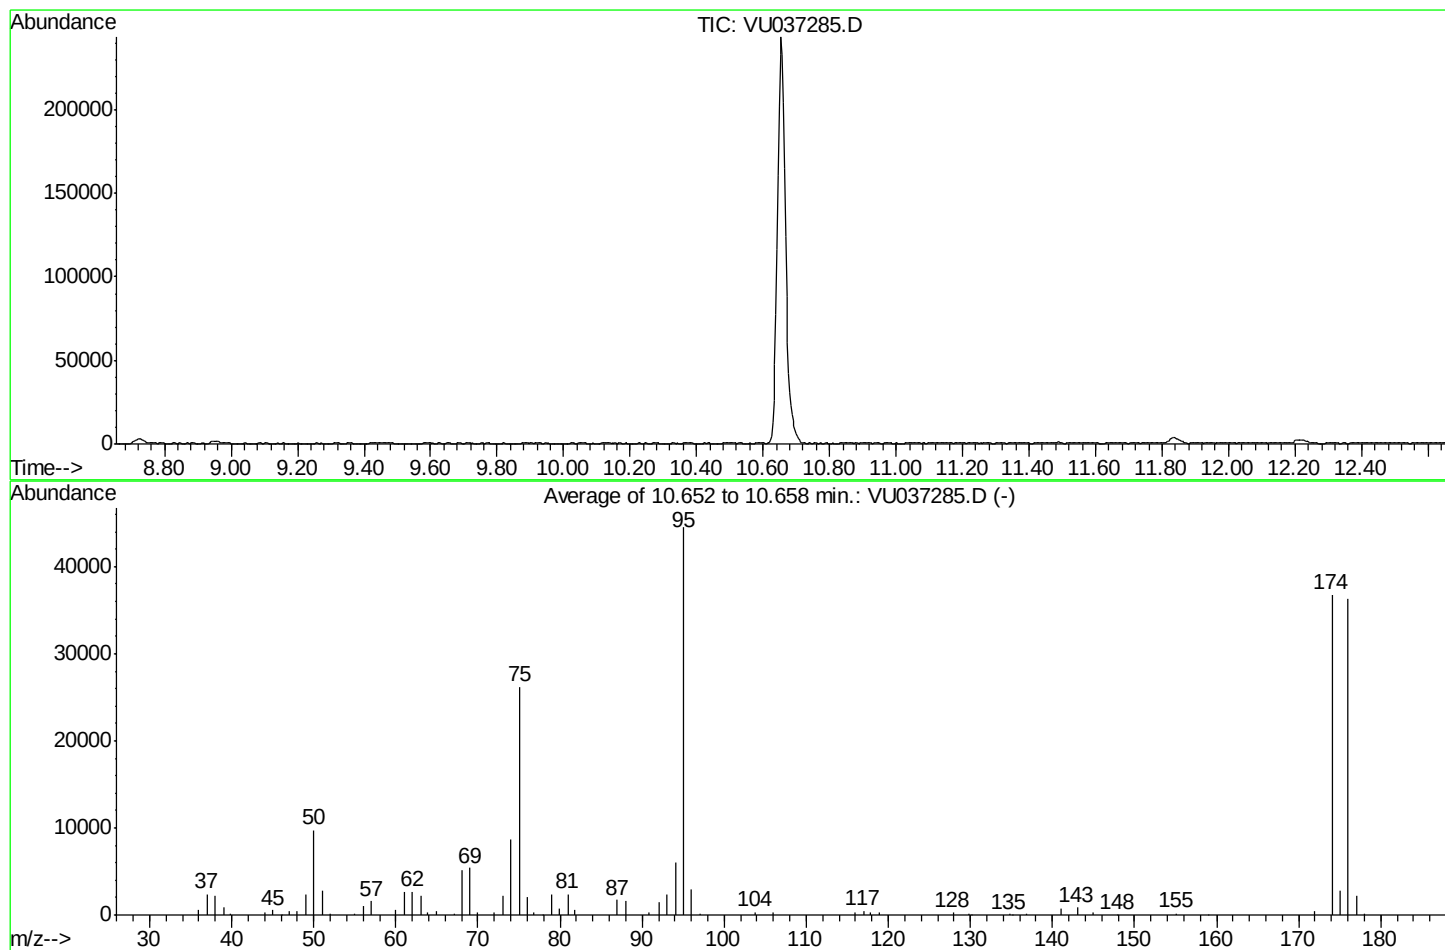

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	9710	PASS
75	95	30	80	58.9	26237	PASS
95	95	100	100	100.0	44512	PASS
96	95	5	9	6.5	2915	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.6	36770	PASS
175	174	5	9	7.5	2766	PASS
176	174	95	101	98.9	36368	PASS
177	176	5	9	6.2	2240	PASS

m/z	Abundance
44.00	351.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

m/z	Abundance
35.90	491.0
37.00	2377.0
38.00	2376.0
39.00	928.0
44.00	593.0
45.00	537.0
47.10	455.0
47.90	400.0
49.00	2384.0
50.00	9678.0
51.00	2745.0
51.90	151.0
54.90	233.0
56.00	994.0
57.00	1510.0
59.90	661.0
61.00	2444.0
62.00	2686.0
63.00	2275.0
63.90	360.0
65.00	424.0
67.10	215.0
68.00	5087.0
69.00	5350.0
70.00	339.0
71.90	260.0
73.00	2043.0
74.00	8747.0
75.10	25696.0
76.00	2098.0
76.80	295.0
77.90	143.0
78.90	2241.0
79.90	669.0
80.90	2490.0
81.90	566.0
87.00	1738.0
88.10	1423.0
90.90	317.0
92.00	1487.0
93.00	2282.0
94.10	5858.0
95.10	44248.0
96.10	2890.0
97.10	114.0
103.90	358.0
105.90	264.0
116.00	293.0
117.00	445.0
117.90	311.0
118.90	347.0
127.90	198.0
129.80	225.0
134.70	147.0
135.20	112.0
136.90	130.0
141.00	600.0
143.00	877.0
145.10	226.0
155.10	196.0
172.00	510.0
174.10	35928.0
175.10	2716.0
176.10	34920.0
177.00	2217.0
178.00	111.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

m/z	Abundance
36.00	613.0
37.00	2470.0
38.00	2342.0
39.00	879.0
39.80	116.0
44.00	664.0
45.00	619.0
47.00	472.0
47.90	440.0
49.00	2369.0
50.00	10001.0
51.00	2972.0
52.00	108.0
54.90	238.0
56.00	1047.0
57.00	1673.0
59.90	667.0
61.00	2691.0
62.00	2710.0
63.00	2260.0
63.90	311.0
64.90	471.0
67.10	207.0
68.00	5226.0
69.00	5624.0
70.00	384.0
71.90	275.0
73.00	2201.0
74.00	8933.0
75.10	27080.0
76.00	2138.0
76.80	336.0
78.90	2394.0
79.90	701.0
80.90	2423.0
81.90	565.0
87.00	1744.0
88.00	1580.0
90.90	282.0
92.00	1483.0
93.00	2413.0
94.10	6132.0
95.10	45936.0
96.00	2979.0
97.10	136.0
103.90	338.0
105.90	319.0
116.00	331.0
117.00	482.0
117.90	297.0
119.00	378.0
127.90	230.0
129.90	218.0
134.80	139.0
136.90	140.0
141.00	675.0
143.00	916.0
145.00	251.0
147.90	117.0
155.10	223.0
159.00	105.0
172.00	500.0
174.10	37808.0
175.10	2872.0
176.10	37504.0
177.00	2264.0
178.00	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

m/z	Abundance
36.00	663.0
37.00	2412.0
38.00	2089.0
39.00	735.0
39.80	148.0
44.00	712.0
45.00	586.0
46.00	105.0
47.00	452.0
47.90	370.0
49.10	2107.0
50.00	9452.0
51.00	2892.0
55.00	188.0
56.00	1030.0
57.00	1663.0
60.00	588.0
61.00	2765.0
62.00	2568.0
63.00	2088.0
63.90	265.0
65.00	412.0
67.10	178.0
68.00	4988.0
69.00	5286.0
70.00	389.0
72.00	285.0
73.10	2256.0
74.00	8420.0
75.10	25936.0
76.00	1935.0
76.80	270.0
78.90	2306.0
80.00	688.0
81.00	2212.0
81.80	475.0
87.00	1714.0
88.00	1653.0
90.80	254.0
92.00	1395.0
93.00	2275.0
94.10	5962.0
95.10	43352.0
96.00	2877.0
97.10	135.0
103.80	271.0
105.90	323.0
116.00	278.0
117.00	487.0
117.80	256.0
119.00	387.0
127.90	259.0
130.10	197.0
134.90	120.0
136.90	114.0
141.00	731.0
143.00	805.0
144.90	251.0
148.00	113.0
155.10	210.0
172.00	496.0
174.10	36576.0
175.10	2710.0
176.00	36680.0
177.10	2239.0
178.00	106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05