

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053220.D
 Acq On : 16 Mar 2023 12:47
 Operator : JC/MD
 Sample : 01929-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFB4

Quant Time: Mar 17 02:40:52 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 17 02:34:44 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	156813	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	150504	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.806	152	74263	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	61067	42.212	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	84.420%		
7) Chloroethane-d5	1.912	69	51379	43.906	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	87.820%		
11) 1,1-Dichloroethene-d2	2.565	63	82621	32.968	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	65.940%		
21) 2-Butanone-d5	4.620	46	63113	94.061	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	94.060%		
24) Chloroform-d	5.057	84	104517	43.863	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.720%		
26) 1,2-Dichloroethane-d4	5.694	65	68105	46.023	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.040%		
32) Benzene-d6	5.723	84	224177	45.922	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.840%		
36) 1,2-Dichloropropane-d6	6.684	67	73022	46.348	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	92.700%		
41) Toluene-d8	7.893	98	199384	43.869	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	87.740%		
43) trans-1,3-Dichloroprop...	8.173	79	34035	43.784	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	87.560%		
47) 2-Hexanone-d5	8.629	63	50048	101.606	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	101.610%		
56) 1,1,2,2-Tetrachloroeth...	10.751	84	94444	46.274	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	92.540%		
66) 1,2-Dichlorobenzene-d4	12.189	152	65798	45.758	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.520%		
Target Compounds						Qvalue
37) 1,2-Dichloropropane	6.684	63	7603	5.223	ug/L #	90
60) 1,2,3-Trichloropropane	11.806	75	10989	7.447	ug/L #	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053220.D
Acq On : 16 Mar 2023 12:47
Operator : JC/MD
Sample : 01929-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFB4

Quant Time: Mar 17 02:40:52 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 17 02:34:44 2023
Response via : Initial Calibration

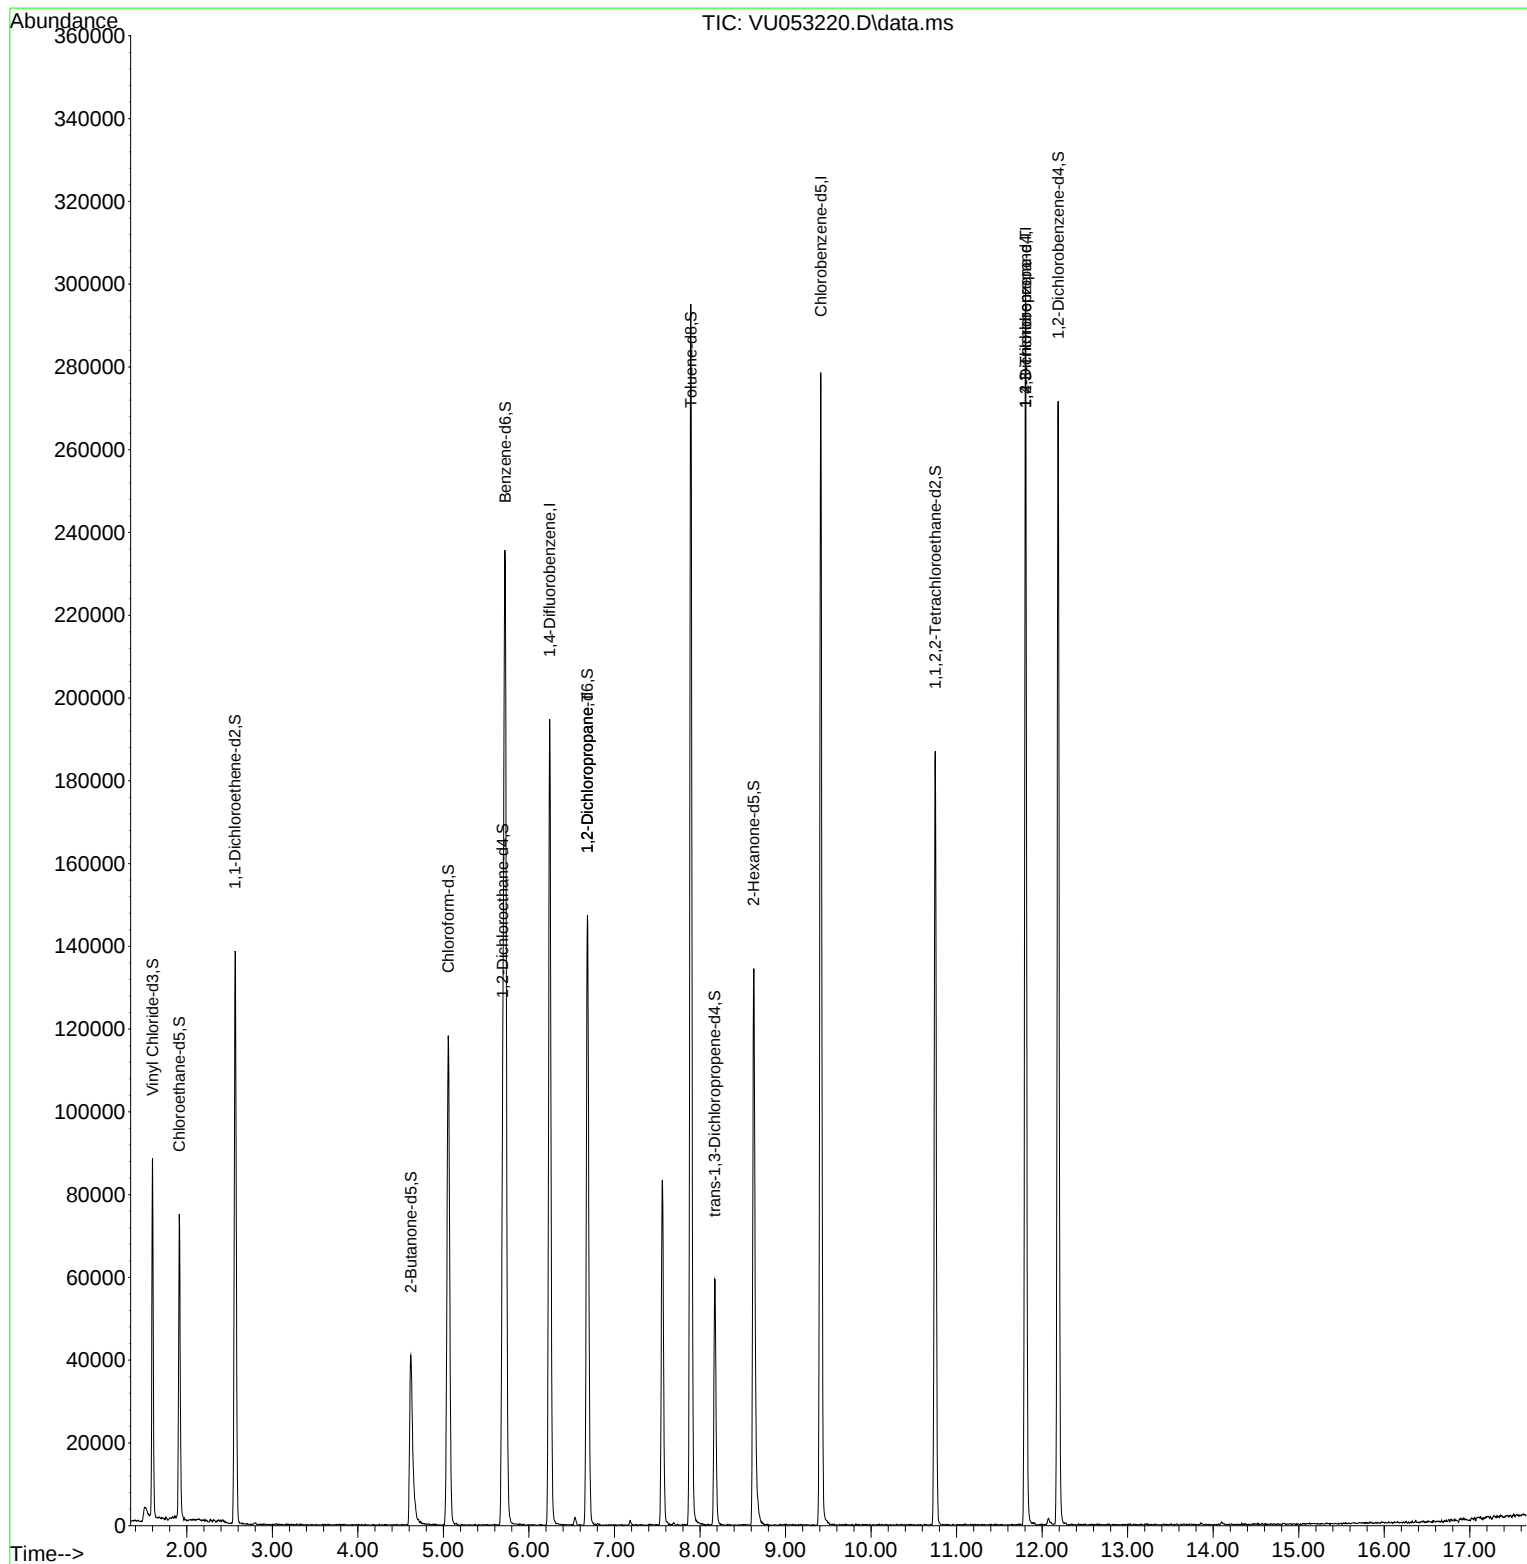

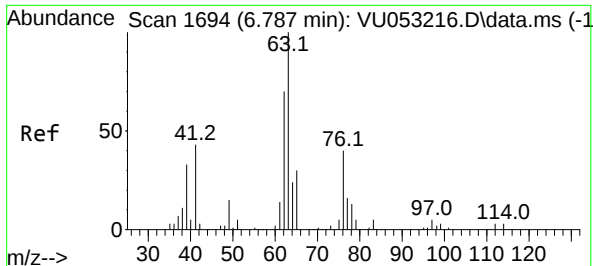

#37

1,2-Dichloropropane

Concen: 5.223 ug/L

RT: 6.684 min Scan# 1

Delta R.T. -0.103 min

Lab File: VU053220.D

Acq: 16 Mar 2023 12:47

Instrument :

MSVOA_U

ClientSampleId :





EYFB4

Tgt Ion: 63 Resp: 7603

Ion Ratio Lower Upper

63 100

112 0.0 2.6 3.8#

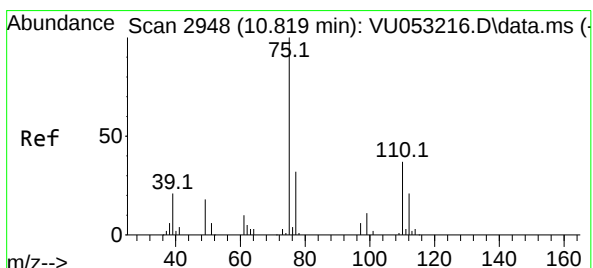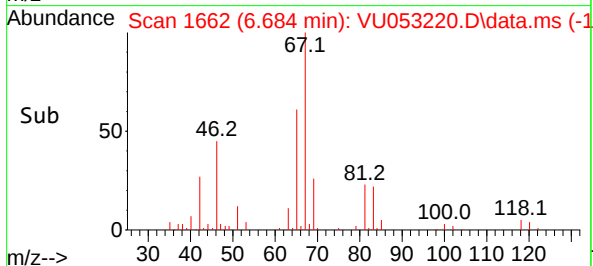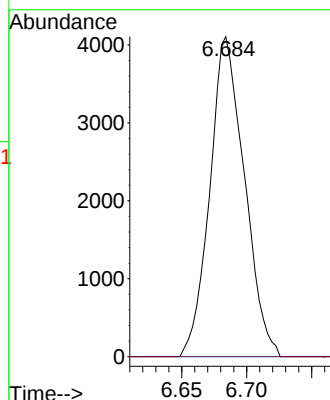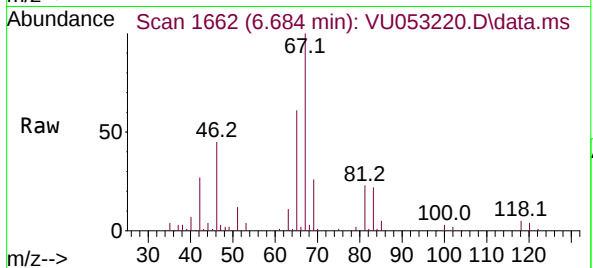

#60

1,2,3-Trichloropropane

Concen: 7.447 ug/L

RT: 11.806 min Scan# 3255

Delta R.T. 0.987 min

Lab File: VU053220.D

Acq: 16 Mar 2023 12:47

Tgt Ion: 75 Resp: 10989

Ion Ratio Lower Upper

75 100

77 30.9 26.6 40.0

110 1.5 28.6 42.8#

