

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053244.D
 Acq On : 16 Mar 2023 22:35
 Operator : JC/MD
 Sample : 01930-15 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFC1

Quant Time: Mar 17 04:31:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 17 04:28:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.244	114	142329	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	134236	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.806	152	65681	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	49770	37.904	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	75.800%
7) Chloroethane-d5	1.909	69	43677	41.123	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	82.240%
11) 1,1-Dichloroethene-d2	2.562	63	68144	29.958	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	59.920%#
21) 2-Butanone-d5	4.610	46	64696	106.232	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	106.230%
24) Chloroform-d	5.057	84	91364	42.245	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.500%
26) 1,2-Dichloroethane-d4	5.694	65	60693	45.188	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.380%
32) Benzene-d6	5.719	84	193915	44.537	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.080%
36) 1,2-Dichloropropane-d6	6.684	67	65480	46.597	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	93.200%
41) Toluene-d8	7.893	98	172634	42.587	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.180%
43) trans-1,3-Dichloroprop...	8.173	79	29395	42.397	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.800%
47) 2-Hexanone-d5	8.626	63	46824	106.581	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	106.580%
56) 1,1,2,2-Tetrachloroeth...	10.751	84	85903	47.190	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.380%
66) 1,2-Dichlorobenzene-d4	12.189	152	56376	44.329	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.660%
Target Compounds						
37) 1,2-Dichloropropane	6.687	63	6778	5.220	ug/L	Qvalue # 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053244.D
Acq On : 16 Mar 2023 22:35
Operator : JC/MD
Sample : 01930-15 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFC1

Quant Time: Mar 17 04:31:45 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 17 04:28:43 2023
Response via : Initial Calibration

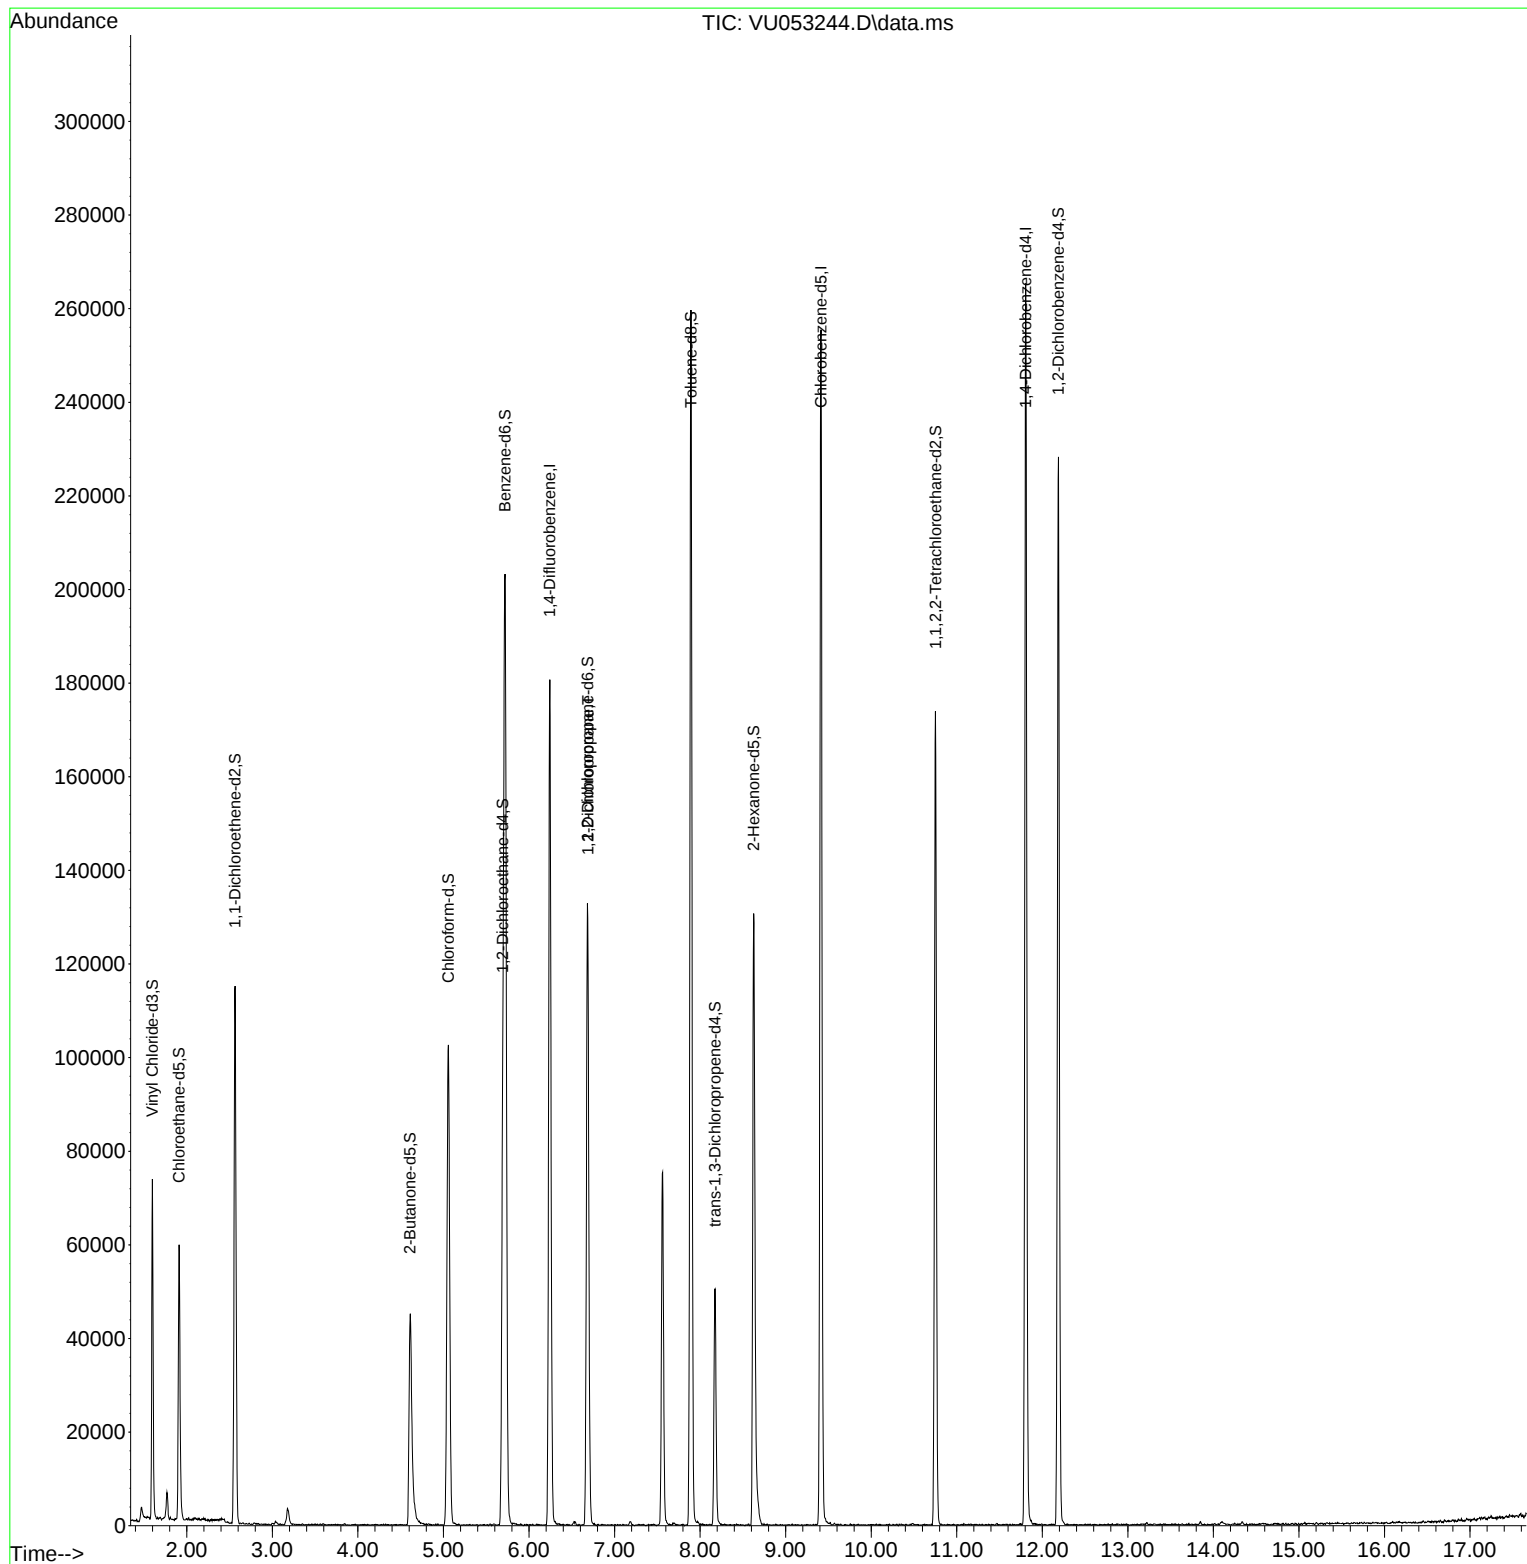

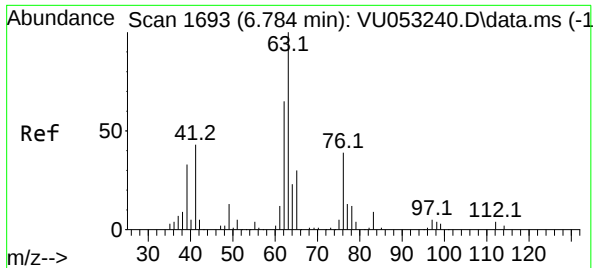

#37
 1,2-Dichloropropane
 Concen: 5.220 ug/L
 RT: 6.687 min Scan# 1
 Delta R.T. -0.096 min
 Lab File: VU053244.D
 Acq: 16 Mar 2023 22:35

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFC1

Tgt Ion: 63 Resp: 6778
 Ion Ratio Lower Upper
 63 100
 112 0.0 2.6 3.8#

