




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053219.D
Acq On : 16 Mar 2023 12:02
Operator : JC/MD
Sample : 01929-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFF2

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 03/17/2023
Supervised By :Mahesh Dadoda 03/20/2023

Quant Time: Mar 17 02:40:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 17 02:34:44 2023
Response via : Initial Calibration

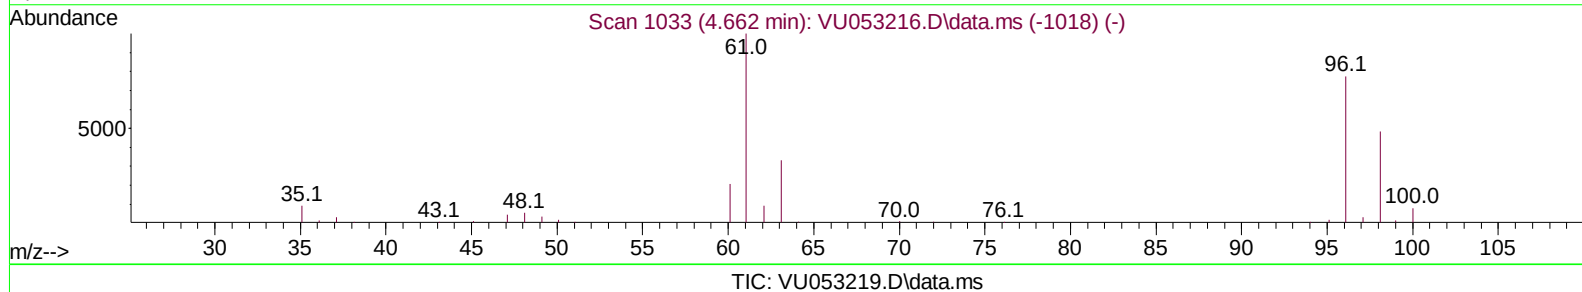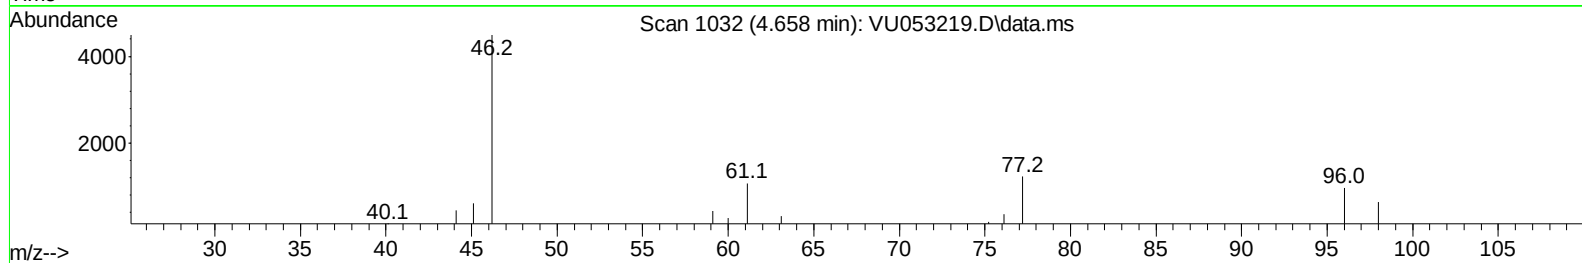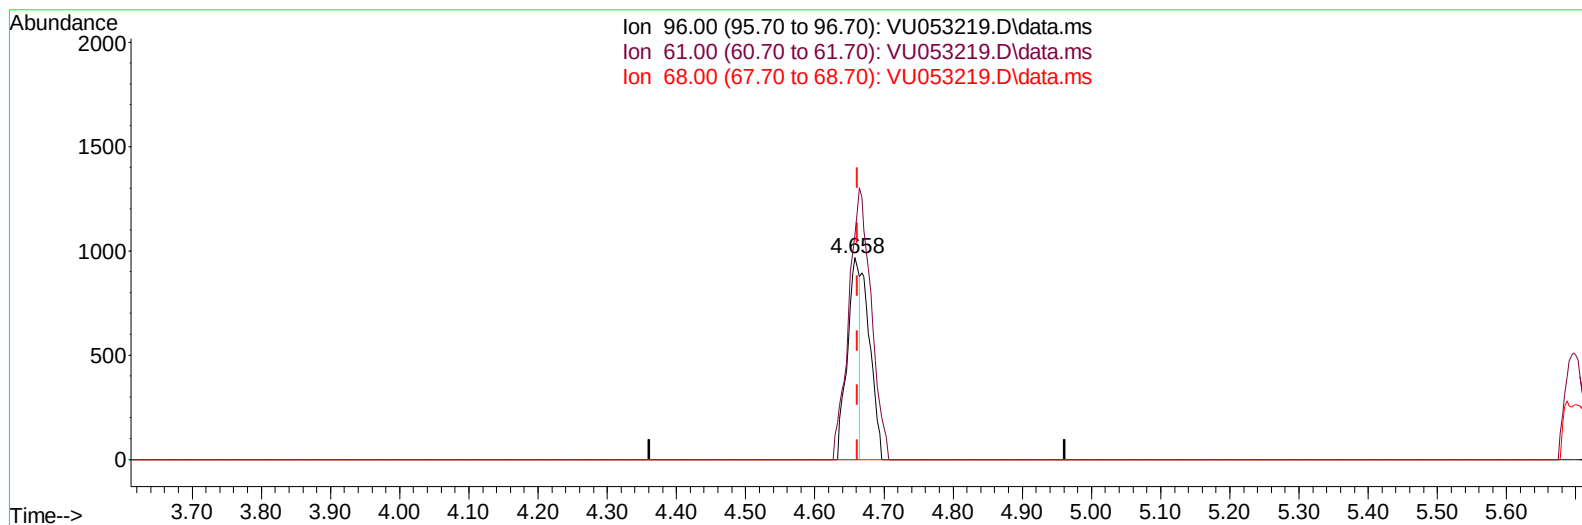

(20) cis-1,2-Dichloroethene (T)

4.658min (-0.003) 1.71 ug/L

response 1204

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	132.10	111.07
68.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053219.D
 Acq On : 16 Mar 2023 12:02
 Operator : JC/MD
 Sample : 01929-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFF2

Manual IntegrationsAPPROVED

Quant Time: Mar 17 02:40:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 17 02:34:44 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/17/2023
 Supervised By :Mahesh Dadoda 03/20/2023

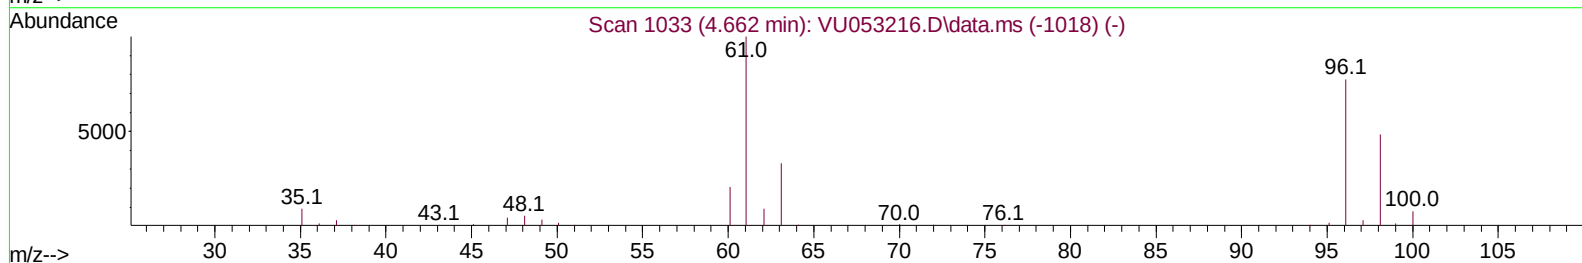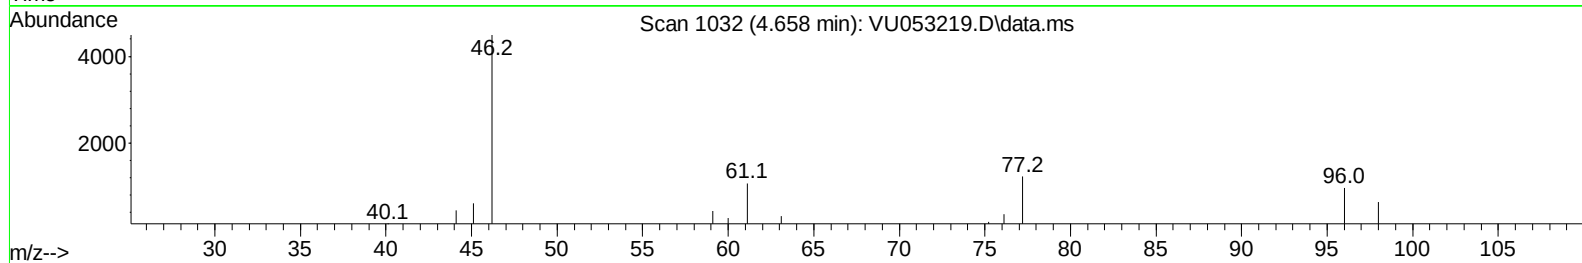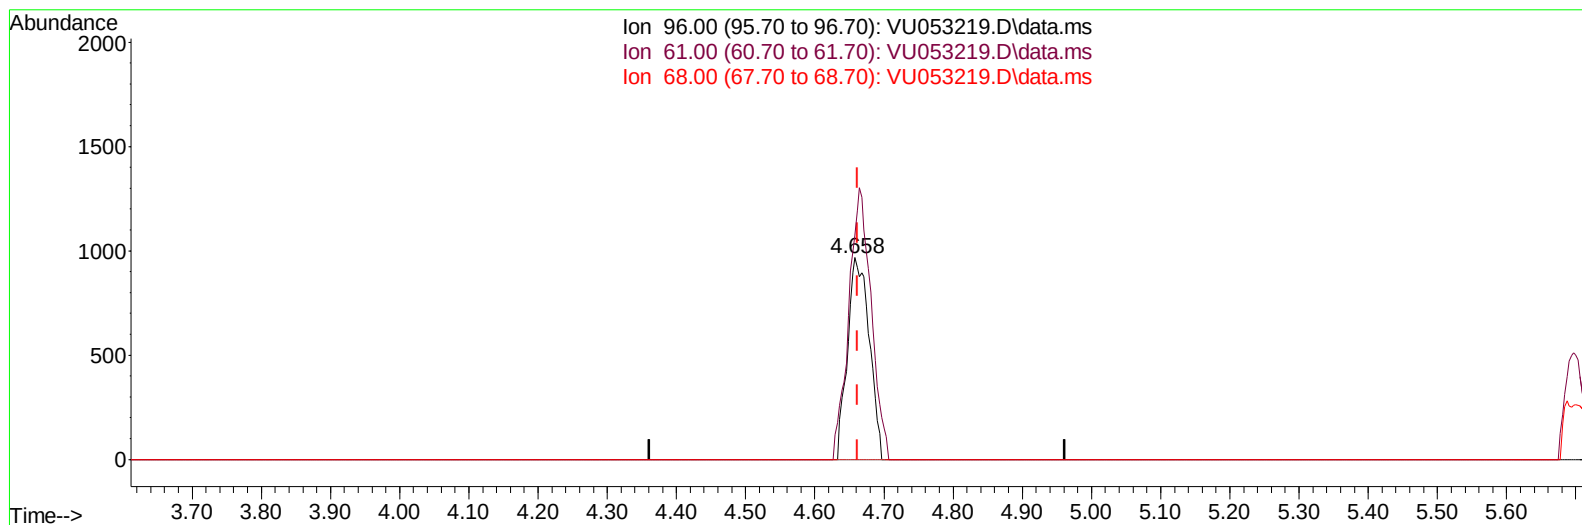

TIC: VU053219.D\data.ms

(20) cis-1,2-Dichloroethene (T)

4.658min (-0.003) 2.99 ug/L m

response 2105

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	132.10	111.07
68.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053219.D
 Acq On : 16 Mar 2023 12:02
 Operator : JC/MD
 Sample : 01929-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFF2

Manual IntegrationsAPPROVED

Quant Time: Mar 17 02:40:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 17 02:34:44 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/17/2023
 Supervised By :Mahesh Dadoda 03/20/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.247	114		80414	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117		75002	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.806	152		37491	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.600	65		47181	63.598	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery	=	127.200%	
7) Chloroethane-d5	1.916	69		39598	65.988	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130		Recovery	=	131.980%#	
11) 1,1-Dichloroethene-d2	2.568	63		63418	49.347	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	98.700%	
21) 2-Butanone-d5	4.620	46		57155	166.110	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130		Recovery	=	166.110%#	
24) Chloroform-d	5.057	84		81787	66.935	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	133.860%#	
26) 1,2-Dichloroethane-d4	5.697	65		54899	72.345	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	144.700%#	
32) Benzene-d6	5.723	84		172295	70.824	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	141.640%#	
36) 1,2-Dichloropropane-d6	6.684	67		57533	73.277	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery	=	146.560%#	
41) Toluene-d8	7.893	98		154198	68.080	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	136.160%#	
43) trans-1,3-Dichloroprop...	8.176	79		27398	70.726	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	141.460%#	
47) 2-Hexanone-d5	8.629	63		44745	182.286	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130		Recovery	=	182.290%#	
56) 1,1,2,2-Tetrachloroeth...	10.751	84		78328	77.011	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery	=	154.020%#	
66) 1,2-Dichlorobenzene-d4	12.188	152		51367	70.760	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	141.520%#	
Target Compounds							
13) Acetone	2.633	43		2430	6.201	ug/L	87
20) cis-1,2-Dichloroethene	4.658	96		2105m	2.991	ug/L	
34) Trichloroethene	6.539	95		1219	1.798	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053219.D
Acq On : 16 Mar 2023 12:02
Operator : JC/MD
Sample : 01929-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFF2

Manual IntegrationsAPPROVED

Quant Time: Mar 17 02:40:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 17 02:34:44 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 03/17/2023
Supervised By :Mahesh Dadoda 03/20/2023

