

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053230.D
 Acq On : 16 Mar 2023 16:42
 Operator : JC/MD
 Sample : 01930-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFF4

Quant Time: Mar 17 02:43:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 17 02:34:44 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	102551	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	94811	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	45799	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	40497	42.805	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	85.600%
7) Chloroethane-d5	1.909	69	32463	42.420	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	84.840%
11) 1,1-Dichloroethene-d2	2.565	63	53606	32.708	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.420%
21) 2-Butanone-d5	4.613	46	56262	128.218	ug/L	-0.01
Spiked Amount	100.000	Range	40 - 130	Recovery	=	128.220%
24) Chloroform-d	5.057	84	67521	43.331	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.660%
26) 1,2-Dichloroethane-d4	5.697	65	43966	45.431	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.860%
32) Benzene-d6	5.722	84	140092	45.555	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.120%
36) 1,2-Dichloropropane-d6	6.684	67	47414	47.772	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.540%
41) Toluene-d8	7.893	98	126984	44.351	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.700%
43) trans-1,3-Dichloroprop...	8.172	79	21384	43.668	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.340%
47) 2-Hexanone-d5	8.626	63	40428	130.288	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	130.290%#
56) 1,1,2,2-Tetrachloroeth...	10.751	84	66087	51.400	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	102.800%
66) 1,2-Dichlorobenzene-d4	12.188	152	39500	44.542	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.080%
Target Compounds						
13) Acetone	2.620	43	2435	4.872	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053230.D
Acq On : 16 Mar 2023 16:42
Operator : JC/MD
Sample : 01930-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFF4

Quant Time: Mar 17 02:43:04 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 17 02:34:44 2023
Response via : Initial Calibration

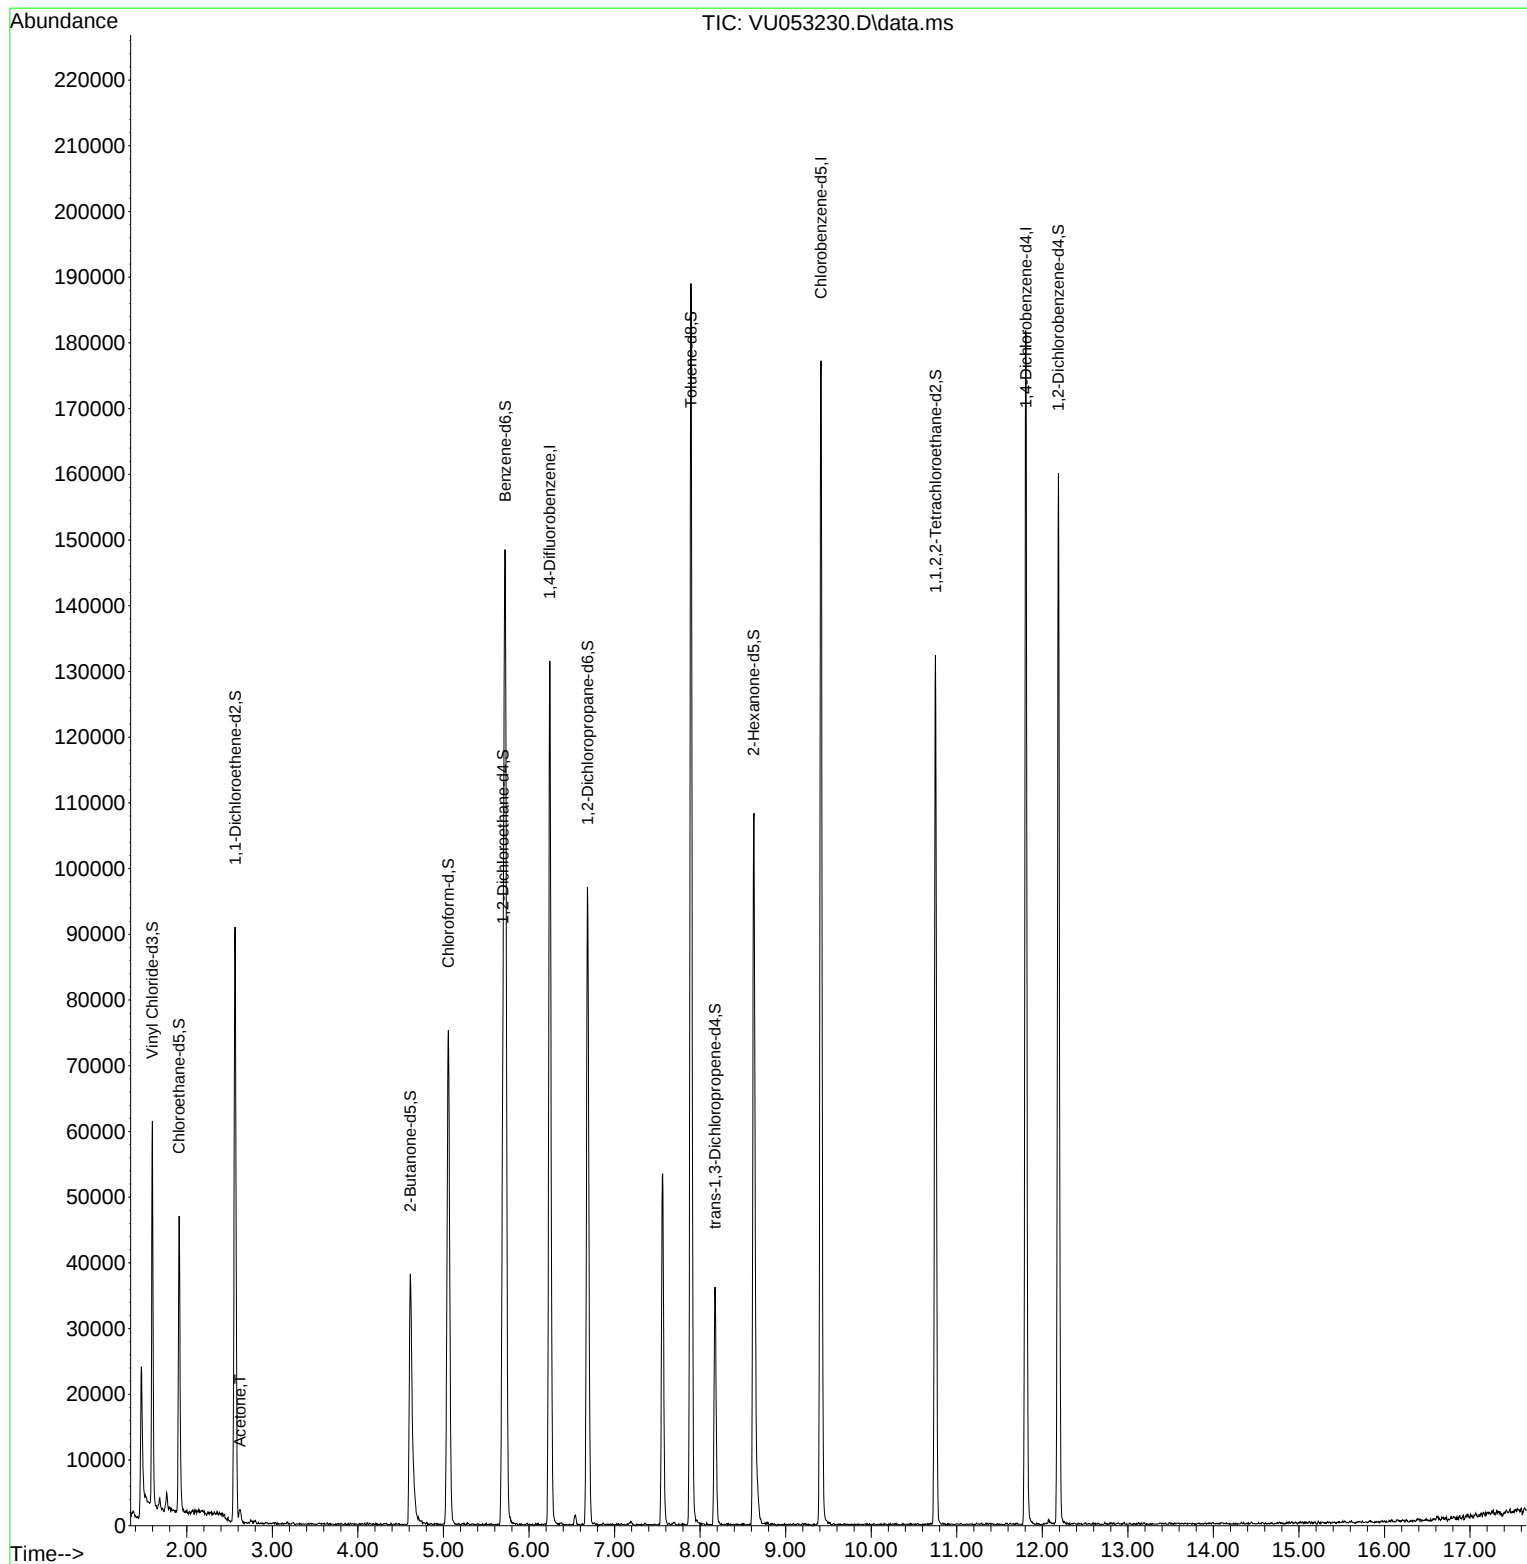

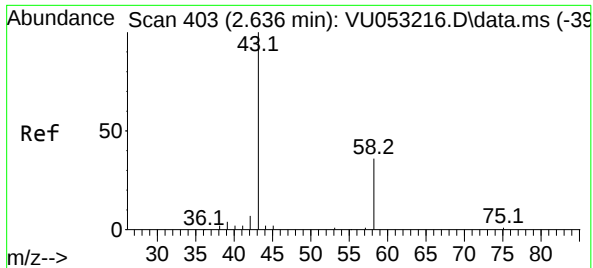

#13
 Acetone
 Concen: 4.872 ug/L
 RT: 2.620 min Scan# 398
 Delta R.T. -0.016 min
 Lab File: VU053230.D
 Acq: 16 Mar 2023 16:42

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFF4

Tgt Ion: 43 Resp: 2435
 Ion Ratio Lower Upper
 43 100
 58 36.7 0.0 75.0

