

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053217.D
 Acq On : 16 Mar 2023 11:07
 Operator : JC/MD
 Sample : VU0316WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK050

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053217.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	93	rBV	88752	101029	15.63%	2.115%
2	1.912	171	178	196	rVB	76709	105494	16.32%	2.209%
3	2.568	370	382	400	rVB	142815	230573	35.67%	4.828%
4	2.716	425	428	431	rBV	198	115	0.02%	0.002%
5	3.038	523	528	530	rBV3	723	653	0.10%	0.014%
6	3.099	544	547	550	rBV	202	126	0.02%	0.003%
7	3.150	560	563	565	rBV	249	149	0.02%	0.003%
8	3.359	626	628	637	rVB3	375	337	0.05%	0.007%
9	3.552	683	688	694	rBV2	285	294	0.05%	0.006%
10	3.581	694	697	701	rVB2	251	223	0.03%	0.005%
11	3.719	738	740	742	rBV	146	65	0.01%	0.001%
12	4.356	937	938	941	rVB	132	50	0.01%	0.001%
13	4.385	943	947	951	rVB2	284	273	0.04%	0.006%
14	4.404	951	953	955	rBV	162	97	0.02%	0.002%
15	4.620	1009	1020	1050	rBV	43703	115998	17.95%	2.429%
16	4.858	1091	1094	1098	rVV	188	115	0.02%	0.002%
17	4.883	1100	1102	1107	rVB	373	218	0.03%	0.005%
18	4.957	1121	1125	1126	rBV	182	117	0.02%	0.002%
19	5.057	1138	1156	1176	rBV	119963	264229	40.88%	5.533%
20	5.353	1246	1248	1249	rBV	133	51	0.01%	0.001%
21	5.414	1264	1267	1268	rBV	169	75	0.01%	0.002%
22	5.555	1306	1311	1313	rBV	240	231	0.04%	0.005%
23	5.575	1316	1317	1319	rVB	176	67	0.01%	0.001%
24	5.719	1342	1362	1388	rBV2	237519	646357	100.00%	13.534%
25	5.832	1395	1397	1401	rBV2	415	387	0.06%	0.008%
26	5.928	1426	1427	1429	rBV2	110	60	0.01%	0.001%
27	5.941	1429	1431	1436	rVB2	402	298	0.05%	0.006%
28	5.967	1437	1439	1441	rBV	329	215	0.03%	0.005%
29	6.083	1471	1475	1477	rVB2	166	104	0.02%	0.002%
30	6.153	1495	1497	1501	rVB2	159	90	0.01%	0.002%
31	6.173	1501	1503	1504	rBV2	142	63	0.01%	0.001%
32	6.243	1511	1525	1550	rBV	185003	351784	54.43%	7.366%
33	6.407	1574	1576	1578	rBV	285	103	0.02%	0.002%
34	6.420	1578	1580	1582	rVV	197	116	0.02%	0.002%
35	6.436	1583	1585	1588	rVB	193	66	0.01%	0.001%
36	6.484	1596	1600	1601	rBV	243	171	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053217.D
 Acq On : 16 Mar 2023 11:07
 Operator : JC/MD
 Sample : VU0316WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK050

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.533	1607	1615	1628	rBV8	2671	5205	0.81%	0.109%
38	6.620	1640	1642	1645	rVB	320	180	0.03%	0.004%
39	6.684	1646	1662	1681	rBV	151467	295444	45.71%	6.186%
40	6.780	1690	1692	1693	rBV	265	93	0.01%	0.002%
41	6.893	1723	1727	1728	rBV	149	110	0.02%	0.002%
42	7.044	1772	1774	1776	rBV	169	99	0.02%	0.002%
43	7.079	1782	1785	1786	rBV	200	128	0.02%	0.003%
44	7.108	1791	1794	1797	rBV	192	192	0.03%	0.004%
45	7.182	1811	1817	1822	rBV2	704	857	0.13%	0.018%
46	7.337	1863	1865	1867	rVB	158	81	0.01%	0.002%
47	7.497	1912	1915	1917	rBV2	182	117	0.02%	0.002%
48	7.510	1917	1919	1922	rVB	172	62	0.01%	0.001%
49	7.562	1922	1935	1957	rBV	87047	155260	24.02%	3.251%
50	7.687	1970	1974	1977	rBV3	518	396	0.06%	0.008%
51	7.793	2001	2007	2009	rBV	491	472	0.07%	0.010%
52	7.893	2025	2038	2066	rBV	299358	515704	79.79%	10.798%
53	8.044	2083	2085	2088	rVB	171	75	0.01%	0.002%
54	8.070	2091	2093	2096	rVB	172	77	0.01%	0.002%
55	8.176	2111	2126	2145	rBV	58538	100318	15.52%	2.101%
56	8.266	2152	2154	2155	rBV	198	75	0.01%	0.002%
57	8.362	2182	2184	2187	rBV2	169	97	0.02%	0.002%
58	8.407	2193	2198	2203	rBV2	276	271	0.04%	0.006%
59	8.452	2210	2212	2219	rBV2	196	160	0.02%	0.003%
60	8.591	2252	2255	2256	rBV	194	105	0.02%	0.002%
61	8.629	2256	2267	2299	rVB2	136404	259252	40.11%	5.429%
62	8.742	2299	2302	2303	rBV	270	133	0.02%	0.003%
63	8.870	2341	2342	2345	rBV	135	59	0.01%	0.001%
64	8.963	2366	2371	2376	rVB	181	191	0.03%	0.004%
65	9.008	2383	2385	2387	rBV	126	51	0.01%	0.001%
66	9.201	2442	2445	2447	rBV	150	96	0.01%	0.002%
67	9.330	2482	2485	2487	rBV	195	155	0.02%	0.003%
68	9.414	2499	2511	2531	rBV	264026	437038	67.62%	9.151%
69	9.565	2553	2558	2567	rBV3	746	1009	0.16%	0.021%
70	9.632	2577	2579	2583	rBV2	190	142	0.02%	0.003%
71	9.687	2591	2596	2604	rBV3	543	697	0.11%	0.015%
72	9.851	2644	2647	2649	rBV	164	142	0.02%	0.003%
73	9.899	2659	2662	2663	rBV	287	161	0.02%	0.003%
74	9.947	2674	2677	2679	rBV	213	177	0.03%	0.004%
75	10.098	2717	2724	2725	rBV3	496	479	0.07%	0.010%
76	10.108	2725	2727	2729	rVV	597	273	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053217.D
 Acq On : 16 Mar 2023 11:07
 Operator : JC/MD
 Sample : VU0316WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK050

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.327	2792	2795	2797	rBV2	281	176	0.03%	0.004%
78	10.481	2837	2843	2847	rBV2	585	720	0.11%	0.015%
79	10.751	2915	2927	2944	rBV	187915	298683	46.21%	6.254%
80	10.835	2951	2953	2957	rBV2	296	195	0.03%	0.004%
81	10.886	2967	2969	2973	rVB	270	145	0.02%	0.003%
82	11.089	3025	3032	3040	rVB2	690	1131	0.17%	0.024%
83	11.179	3058	3060	3062	rBV	162	51	0.01%	0.001%
84	11.430	3136	3138	3140	rVB	150	61	0.01%	0.001%
85	11.452	3142	3145	3146	rVV	304	167	0.03%	0.003%
86	11.465	3146	3149	3162	rVB3	1062	1303	0.20%	0.027%
87	11.748	3231	3237	3241	rBV4	638	761	0.12%	0.016%
88	11.806	3244	3255	3274	rBV	271574	435258	67.34%	9.114%
89	12.188	3362	3374	3397	rBV	264669	425553	65.84%	8.911%
90	12.523	3476	3478	3481	rBV	215	122	0.02%	0.003%
91	12.561	3488	3490	3493	rVB2	250	140	0.02%	0.003%
92	12.671	3522	3524	3529	rBV	198	160	0.02%	0.003%
93	13.227	3691	3697	3702	rVB2	776	937	0.14%	0.020%
94	13.613	3814	3817	3819	rBV	194	108	0.02%	0.002%
95	13.661	3830	3832	3835	rBV2	200	112	0.02%	0.002%
96	13.815	3878	3880	3882	rBV	172	101	0.02%	0.002%
97	13.841	3882	3888	3897	rVV4	1942	2842	0.44%	0.060%
98	14.089	3958	3965	3982	rVB2	4687	7128	1.10%	0.149%
99	14.327	4034	4039	4051	rVB7	2459	3661	0.57%	0.077%
100	14.500	4090	4093	4096	rBV	252	175	0.03%	0.004%


Sum of corrected areas: 4775716

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053217.D
Acq On : 16 Mar 2023 11:07
Operator : JC/MD
Sample : VU0316WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK050

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

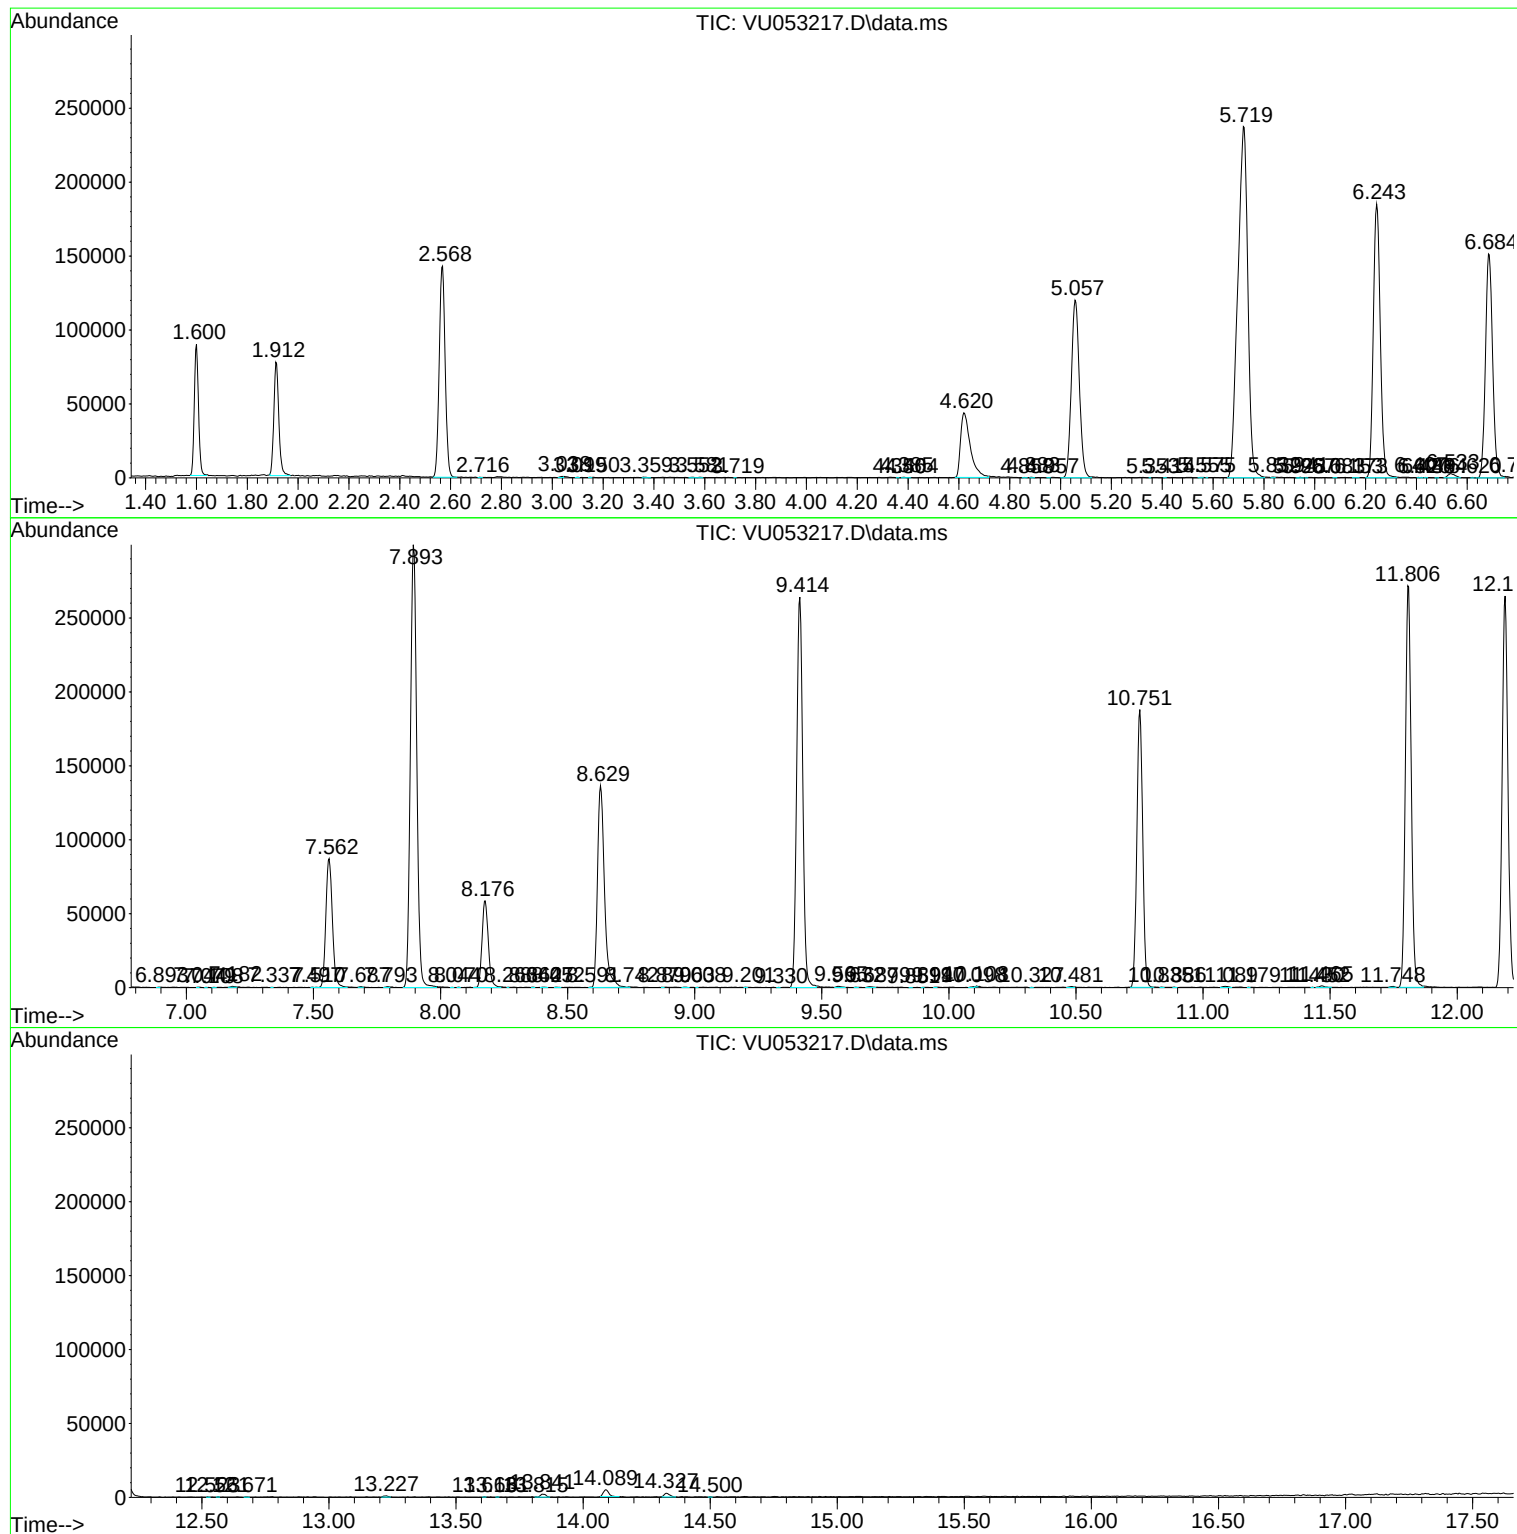

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053217.D
Acq On : 16 Mar 2023 11:07
Operator : JC/MD
Sample : VU0316WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK050

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053217.D
Acq On : 16 Mar 2023 11:07
Operator : JC/MD
Sample : VU0316WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK050

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc