

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053218.D
 Acq On : 16 Mar 2023 11:39
 Operator : JC/MD
 Sample : 01929-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053218.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	94	rVB2	139823	175440	29.36%	4.343%
2	1.912	171	178	197	rVB	69985	95656	16.01%	2.368%
3	2.568	370	382	395	rBV	134909	219289	36.70%	5.429%
4	2.780	446	448	449	rBV	368	150	0.03%	0.004%
5	3.067	534	537	542	rBV	212	155	0.03%	0.004%
6	3.584	694	698	700	rBV3	511	430	0.07%	0.011%
7	3.655	717	720	721	rBV	196	112	0.02%	0.003%
8	3.796	762	764	766	rVB	226	112	0.02%	0.003%
9	3.867	783	786	790	rBV2	265	219	0.04%	0.005%
10	3.938	804	808	811	rBV2	261	185	0.03%	0.005%
11	4.530	990	992	994	rBV2	161	96	0.02%	0.002%
12	4.623	1008	1021	1028	rBV	41760	95180	15.93%	2.356%
13	4.906	1107	1109	1112	rVB	225	122	0.02%	0.003%
14	5.060	1141	1157	1178	rBV	110032	242445	40.57%	6.002%
15	5.173	1189	1192	1195	rBV2	153	85	0.01%	0.002%
16	5.269	1220	1222	1226	rVB	227	124	0.02%	0.003%
17	5.343	1242	1245	1248	rBV	206	190	0.03%	0.005%
18	5.391	1253	1260	1263	rBV2	248	295	0.05%	0.007%
19	5.510	1293	1297	1302	rVB2	203	184	0.03%	0.005%
20	5.722	1341	1363	1386	rBV2	217798	597567	100.00%	14.793%
21	5.941	1428	1431	1436	rBV	291	278	0.05%	0.007%
22	5.989	1444	1446	1447	rBV	217	91	0.02%	0.002%
23	6.031	1453	1459	1461	rBV2	199	175	0.03%	0.004%
24	6.070	1468	1471	1478	rBB	241	302	0.05%	0.007%
25	6.095	1478	1479	1480	rBV	219	70	0.01%	0.002%
26	6.134	1488	1491	1493	rBV	223	147	0.02%	0.004%
27	6.247	1514	1526	1548	rBV	87571	165035	27.62%	4.086%
28	6.343	1554	1556	1562	rBV2	319	274	0.05%	0.007%
29	6.388	1568	1570	1573	rBV	133	98	0.02%	0.002%
30	6.446	1585	1588	1591	rBV	162	172	0.03%	0.004%
31	6.504	1601	1606	1607	rBV	161	167	0.03%	0.004%
32	6.539	1608	1617	1629	rVV3	7304	13148	2.20%	0.325%
33	6.626	1642	1644	1646	rBV	141	79	0.01%	0.002%
34	6.687	1649	1663	1685	rVB	138239	269697	45.13%	6.676%
35	6.828	1702	1707	1709	rBV	148	112	0.02%	0.003%
36	7.037	1770	1772	1776	rBV	289	254	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053218.D
 Acq On : 16 Mar 2023 11:39
 Operator : JC/MD
 Sample : 01929-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	7.131	1798	1801	1805	rBV2	222	186	0.03%	0.005%
38	7.179	1813	1816	1822	rBV4	654	712	0.12%	0.018%
39	7.263	1840	1842	1845	rVB	170	74	0.01%	0.002%
40	7.285	1847	1849	1851	rBV2	277	156	0.03%	0.004%
41	7.562	1923	1935	1956	rBV	80931	142849	23.91%	3.536%
42	7.684	1968	1973	1974	rBV2	271	220	0.04%	0.005%
43	7.735	1986	1989	1991	rVB2	188	99	0.02%	0.002%
44	7.816	2011	2014	2017	rVB	177	82	0.01%	0.002%
45	7.838	2019	2021	2024	rVB	197	90	0.02%	0.002%
46	7.896	2024	2039	2056	rBV	275806	483441	80.90%	11.968%
47	8.176	2115	2126	2153	rBV	54789	94240	15.77%	2.333%
48	8.343	2176	2178	2182	rBV	247	187	0.03%	0.005%
49	8.468	2215	2217	2220	rVB	147	78	0.01%	0.002%
50	8.629	2256	2267	2299	rBV2	138421	265947	44.50%	6.584%
51	8.893	2346	2349	2352	rBV	266	260	0.04%	0.006%
52	8.941	2359	2364	2369	rVB2	230	205	0.03%	0.005%
53	8.989	2377	2379	2382	rBV	193	109	0.02%	0.003%
54	9.037	2392	2394	2397	rBV	214	91	0.02%	0.002%
55	9.172	2433	2436	2439	rBV2	151	90	0.02%	0.002%
56	9.205	2442	2446	2449	rBV2	184	175	0.03%	0.004%
57	9.259	2460	2463	2467	rBV	228	199	0.03%	0.005%
58	9.414	2498	2511	2528	rBV	128317	211666	35.42%	5.240%
59	9.523	2543	2545	2548	rVB	292	136	0.02%	0.003%
60	9.594	2565	2567	2568	rVB	231	88	0.01%	0.002%
61	9.616	2568	2574	2578	rBV	181	297	0.05%	0.007%
62	9.687	2594	2596	2599	rBV	195	157	0.03%	0.004%
63	9.722	2604	2607	2611	rBV2	289	266	0.04%	0.007%
64	9.886	2655	2658	2664	rBV2	282	333	0.06%	0.008%
65	10.002	2691	2694	2697	rBV	193	100	0.02%	0.002%
66	10.082	2717	2719	2722	rVB	201	89	0.01%	0.002%
67	10.102	2722	2725	2731	rVB2	217	210	0.04%	0.005%
68	10.227	2762	2764	2767	rBV	159	90	0.02%	0.002%
69	10.269	2773	2777	2782	rBV2	191	182	0.03%	0.005%
70	10.330	2793	2796	2799	rBV	203	152	0.03%	0.004%
71	10.475	2839	2841	2845	rBV2	316	252	0.04%	0.006%
72	10.639	2888	2892	2895	rBV2	290	199	0.03%	0.005%
73	10.751	2914	2927	2949	rBV	182820	295624	49.47%	7.318%
74	10.883	2966	2968	2970	rBV	130	94	0.02%	0.002%
75	11.012	3005	3008	3010	rBV	167	121	0.02%	0.003%
76	11.272	3086	3089	3092	rVB2	163	89	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053218.D
 Acq On : 16 Mar 2023 11:39
 Operator : JC/MD
 Sample : 01929-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	11.301	3095	3098	3102	rBV	229	232	0.04%	0.006%
78	11.468	3147	3150	3156	rBV2	487	431	0.07%	0.011%
79	11.494	3156	3158	3162	rVB	182	81	0.01%	0.002%
80	11.574	3181	3183	3188	rBV	185	122	0.02%	0.003%
81	11.751	3233	3238	3241	rVB3	464	421	0.07%	0.010%
82	11.809	3241	3256	3278	rBV	135346	223695	37.43%	5.538%
83	12.012	3316	3319	3322	rBV	163	118	0.02%	0.003%
84	12.037	3325	3327	3328	rBV	161	87	0.01%	0.002%
85	12.066	3329	3336	3348	rBV5	4547	9736	1.63%	0.241%
86	12.188	3363	3374	3395	rVB	255340	417258	69.83%	10.329%
87	12.262	3395	3397	3398	rBV	264	109	0.02%	0.003%
88	12.565	3487	3491	3493	rBV	170	140	0.02%	0.003%
89	12.729	3540	3542	3545	rVB	240	95	0.02%	0.002%
90	12.767	3550	3554	3556	rBV2	327	273	0.05%	0.007%
91	13.092	3652	3655	3657	rBV	181	115	0.02%	0.003%
92	13.220	3692	3695	3706	rBV3	460	557	0.09%	0.014%
93	13.291	3714	3717	3721	rBV	344	205	0.03%	0.005%
94	13.494	3776	3780	3784	rVB	328	261	0.04%	0.006%
95	13.847	3884	3890	3896	rVB4	1122	1407	0.24%	0.035%
96	14.092	3959	3966	3973	rBV3	2338	3380	0.57%	0.084%
97	14.330	4034	4040	4050	rVB5	1575	2139	0.36%	0.053%
98	14.497	4087	4092	4099	rBV2	409	401	0.07%	0.010%
99	14.603	4123	4125	4128	rBV	308	151	0.03%	0.004%
100	14.790	4179	4183	4187	rBV3	305	318	0.05%	0.008%




Sum of corrected areas: 4039502

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053218.D
Acq On : 16 Mar 2023 11:39
Operator : JC/MD
Sample : 01929-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

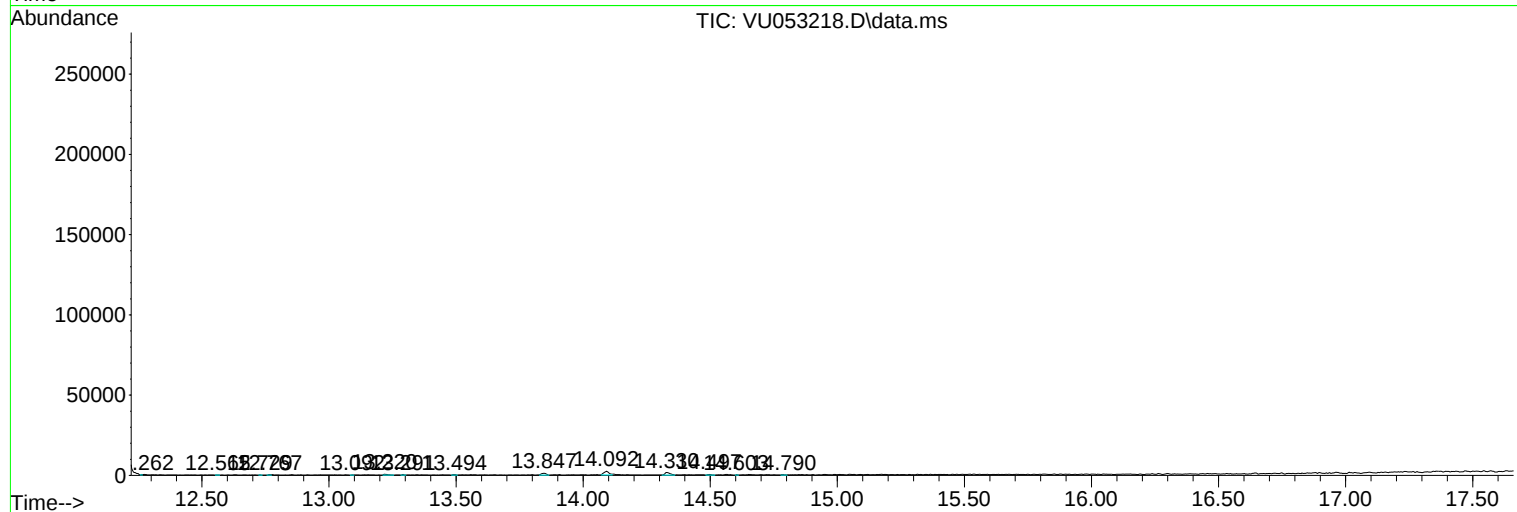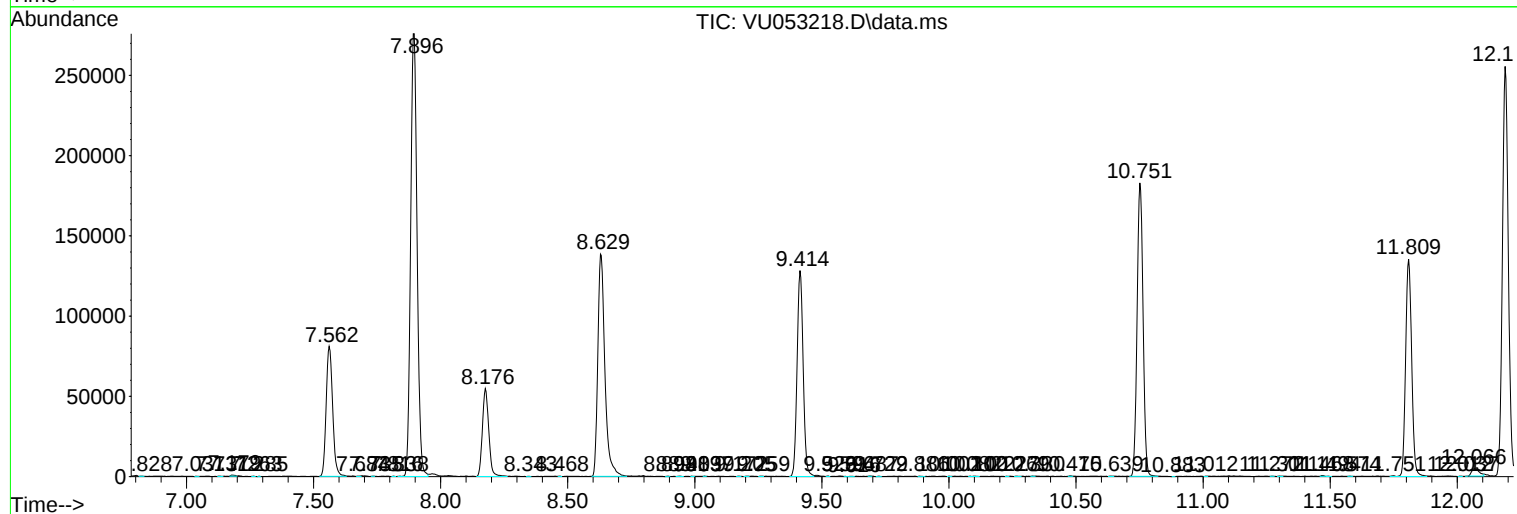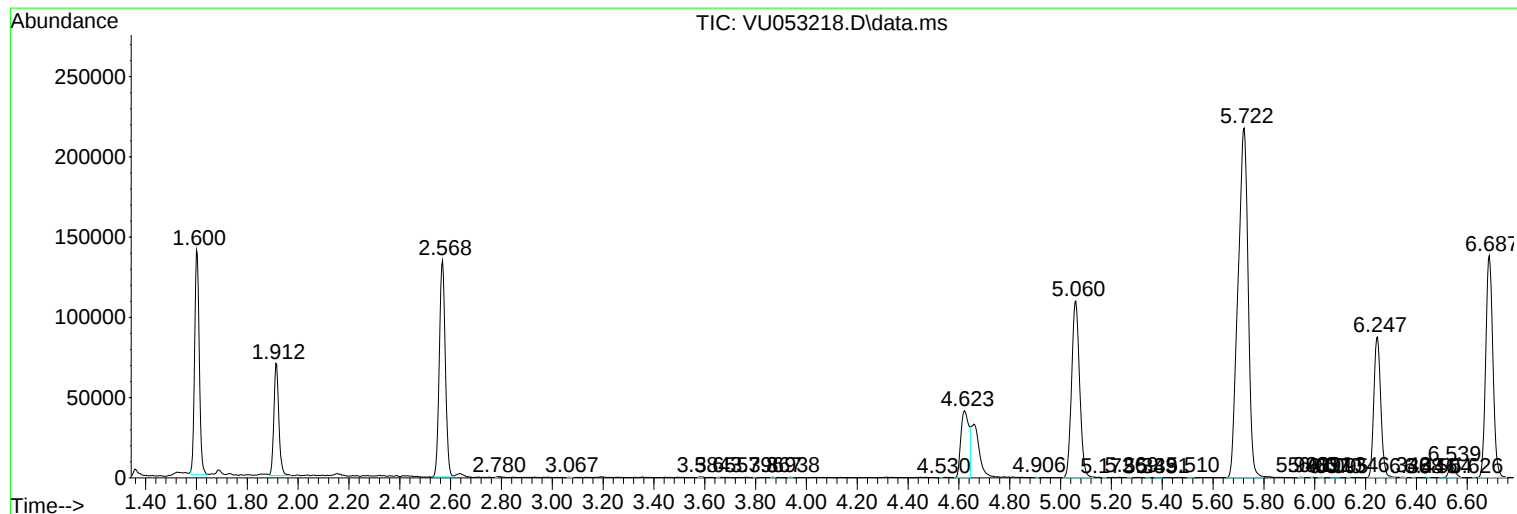

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053218.D
Acq On : 16 Mar 2023 11:39
Operator : JC/MD
Sample : 01929-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053218.D
Acq On : 16 Mar 2023 11:39
Operator : JC/MD
Sample : 01929-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------