

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053222.D
 Acq On : 16 Mar 2023 13:33
 Operator : JC/MD
 Sample : 01930-01 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053222.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.598	73	80	96	rVB	90871	101969	15.65%	2.169%
2	1.909	169	177	194	rVB	72390	97497	14.97%	2.074%
3	2.565	369	381	396	rBV	141084	227789	34.97%	4.846%
4	3.041	523	529	533	rBV4	1028	1328	0.20%	0.028%
5	3.234	586	589	591	rBV	277	175	0.03%	0.004%
6	3.260	595	597	598	rBV	151	46	0.01%	0.001%
7	3.588	696	699	706	rVB	295	296	0.05%	0.006%
8	4.176	879	882	884	rBV	214	95	0.01%	0.002%
9	4.205	888	891	894	rBV	244	132	0.02%	0.003%
10	4.295	916	919	923	rVB2	226	155	0.02%	0.003%
11	4.318	923	926	931	rVB	187	101	0.02%	0.002%
12	4.405	950	953	958	rVB	244	171	0.03%	0.004%
13	4.430	958	961	964	rBV	174	132	0.02%	0.003%
14	4.524	987	990	995	rBV	237	200	0.03%	0.004%
15	4.617	1007	1019	1050	rBV	46117	118543	18.20%	2.522%
16	4.845	1087	1090	1092	rBV	147	86	0.01%	0.002%
17	4.858	1092	1094	1099	rVB	266	172	0.03%	0.004%
18	5.057	1139	1156	1175	rBV	121233	261724	40.18%	5.568%
19	5.192	1195	1198	1200	rBV	197	164	0.03%	0.003%
20	5.241	1212	1213	1221	rVB	200	124	0.02%	0.003%
21	5.421	1266	1269	1272	rVV2	223	145	0.02%	0.003%
22	5.437	1272	1274	1278	rVB	150	54	0.01%	0.001%
23	5.485	1286	1289	1292	rBV	247	170	0.03%	0.004%
24	5.720	1341	1362	1384	rBV2	241674	651421	100.00%	13.859%
25	5.880	1410	1412	1414	rVB	224	108	0.02%	0.002%
26	5.938	1428	1430	1432	rVB	118	25	0.00%	0.001%
27	5.993	1445	1447	1448	rBV	136	59	0.01%	0.001%
28	6.244	1511	1525	1545	rBV	163876	306410	47.04%	6.519%
29	6.414	1576	1578	1579	rBV	209	63	0.01%	0.001%
30	6.469	1593	1595	1599	rBV	194	116	0.02%	0.002%
31	6.536	1611	1616	1620	rBV6	1344	1638	0.25%	0.035%
32	6.620	1640	1642	1647	rBV	181	142	0.02%	0.003%
33	6.684	1648	1662	1684	rVV	154144	298531	45.83%	6.351%
34	7.048	1771	1775	1776	rBV	148	87	0.01%	0.002%
35	7.089	1786	1788	1791	rBV2	154	98	0.02%	0.002%
36	7.128	1797	1800	1805	rVB	215	204	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053222.D
 Acq On : 16 Mar 2023 13:33
 Operator : JC/MD
 Sample : 01930-01 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	7.154	1805	1808	1810	rBV	191	132	0.02%	0.003%
38	7.260	1839	1841	1844	rBB	168	107	0.02%	0.002%
39	7.308	1847	1856	1860	rBV	271	442	0.07%	0.009%
40	7.401	1881	1885	1888	rBV	234	241	0.04%	0.005%
41	7.482	1907	1910	1912	rBV	137	88	0.01%	0.002%
42	7.559	1923	1934	1954	rBV	89920	154753	23.76%	3.292%
43	7.678	1967	1971	1972	rBV2	260	211	0.03%	0.004%
44	7.694	1972	1976	1982	rVB3	826	811	0.12%	0.017%
45	7.781	2000	2003	2007	rBV	134	118	0.02%	0.003%
46	7.829	2016	2018	2019	rBV	136	35	0.01%	0.001%
47	7.893	2024	2038	2058	rBV	301503	517805	79.49%	11.016%
48	8.041	2082	2084	2086	rBV2	186	82	0.01%	0.002%
49	8.105	2101	2104	2108	rVB	194	145	0.02%	0.003%
50	8.173	2114	2125	2143	rBV	59118	99601	15.29%	2.119%
51	8.256	2149	2151	2157	rVB	147	72	0.01%	0.002%
52	8.279	2157	2158	2159	rBV	133	44	0.01%	0.001%
53	8.363	2182	2184	2190	rVB2	219	181	0.03%	0.004%
54	8.395	2192	2194	2197	rVB2	206	125	0.02%	0.003%
55	8.575	2248	2250	2252	rBV	243	163	0.03%	0.003%
56	8.629	2256	2267	2295	rVV2	141504	264212	40.56%	5.621%
57	8.793	2316	2318	2321	rBV2	151	87	0.01%	0.002%
58	8.826	2326	2328	2330	rBV	136	36	0.01%	0.001%
59	8.999	2380	2382	2385	rBV	267	149	0.02%	0.003%
60	9.019	2385	2388	2392	rVV	207	202	0.03%	0.004%
61	9.109	2414	2416	2420	rVB2	144	97	0.01%	0.002%
62	9.166	2432	2434	2437	rBV	152	45	0.01%	0.001%
63	9.285	2469	2471	2472	rBV	143	62	0.01%	0.001%
64	9.353	2489	2492	2493	rBV	121	52	0.01%	0.001%
65	9.411	2498	2510	2533	rBV	238180	390359	59.92%	8.305%
66	9.568	2557	2559	2560	rBV	131	31	0.00%	0.001%
67	9.578	2560	2562	2564	rVB	167	46	0.01%	0.001%
68	9.694	2596	2598	2599	rBV	232	74	0.01%	0.002%
69	9.797	2626	2630	2633	rBB	247	196	0.03%	0.004%
70	9.832	2634	2641	2644	rBV	339	352	0.05%	0.007%
71	9.899	2660	2662	2663	rBV	149	45	0.01%	0.001%
72	10.256	2769	2773	2774	rBV	175	107	0.02%	0.002%
73	10.305	2787	2788	2790	rBV	119	47	0.01%	0.001%
74	10.375	2807	2810	2817	rVB	199	129	0.02%	0.003%
75	10.465	2835	2838	2843	rBV	211	168	0.03%	0.004%
76	10.562	2866	2868	2871	rBV	198	88	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053222.D
 Acq On : 16 Mar 2023 13:33
 Operator : JC/MD
 Sample : 01930-01 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.617	2884	2885	2886	rBV	117	30	0.00%	0.001%
78	10.752	2915	2927	2944	rBV	194448	307815	47.25%	6.549%
79	10.871	2962	2964	2967	rVB2	159	91	0.01%	0.002%
80	10.912	2975	2977	2980	rVB	191	60	0.01%	0.001%
81	11.044	3015	3018	3020	rBV	176	113	0.02%	0.002%
82	11.089	3029	3032	3036	rVB	193	128	0.02%	0.003%
83	11.260	3083	3085	3089	rVB	210	101	0.02%	0.002%
84	11.279	3089	3091	3093	rBV	156	52	0.01%	0.001%
85	11.530	3166	3169	3171	rBV	213	97	0.01%	0.002%
86	11.636	3200	3202	3207	rBV	190	136	0.02%	0.003%
87	11.806	3244	3255	3281	rBV	282141	446384	68.52%	9.497%
88	11.951	3298	3300	3302	rBV	301	99	0.02%	0.002%
89	12.076	3337	3339	3343	rBV	295	151	0.02%	0.003%
90	12.189	3361	3374	3394	rBV	272378	440860	67.68%	9.379%
91	12.279	3400	3402	3406	rVB2	373	175	0.03%	0.004%
92	12.546	3481	3485	3491	rBV2	225	272	0.04%	0.006%
93	12.710	3533	3536	3538	rBV	199	93	0.01%	0.002%
94	12.748	3545	3548	3549	rBV	207	117	0.02%	0.002%
95	12.835	3572	3575	3580	rVB	229	150	0.02%	0.003%
96	12.896	3588	3594	3597	rBV2	222	284	0.04%	0.006%
97	12.948	3607	3610	3612	rBV2	217	139	0.02%	0.003%
98	13.851	3888	3891	3896	rBV2	322	215	0.03%	0.005%
99	14.102	3963	3969	3974	rBV2	526	725	0.11%	0.015%
100	15.070	4268	4270	4274	rBV	330	261	0.04%	0.006%


Sum of corrected areas: 4700458

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053222.D
Acq On : 16 Mar 2023 13:33
Operator : JC/MD
Sample : 01930-01 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

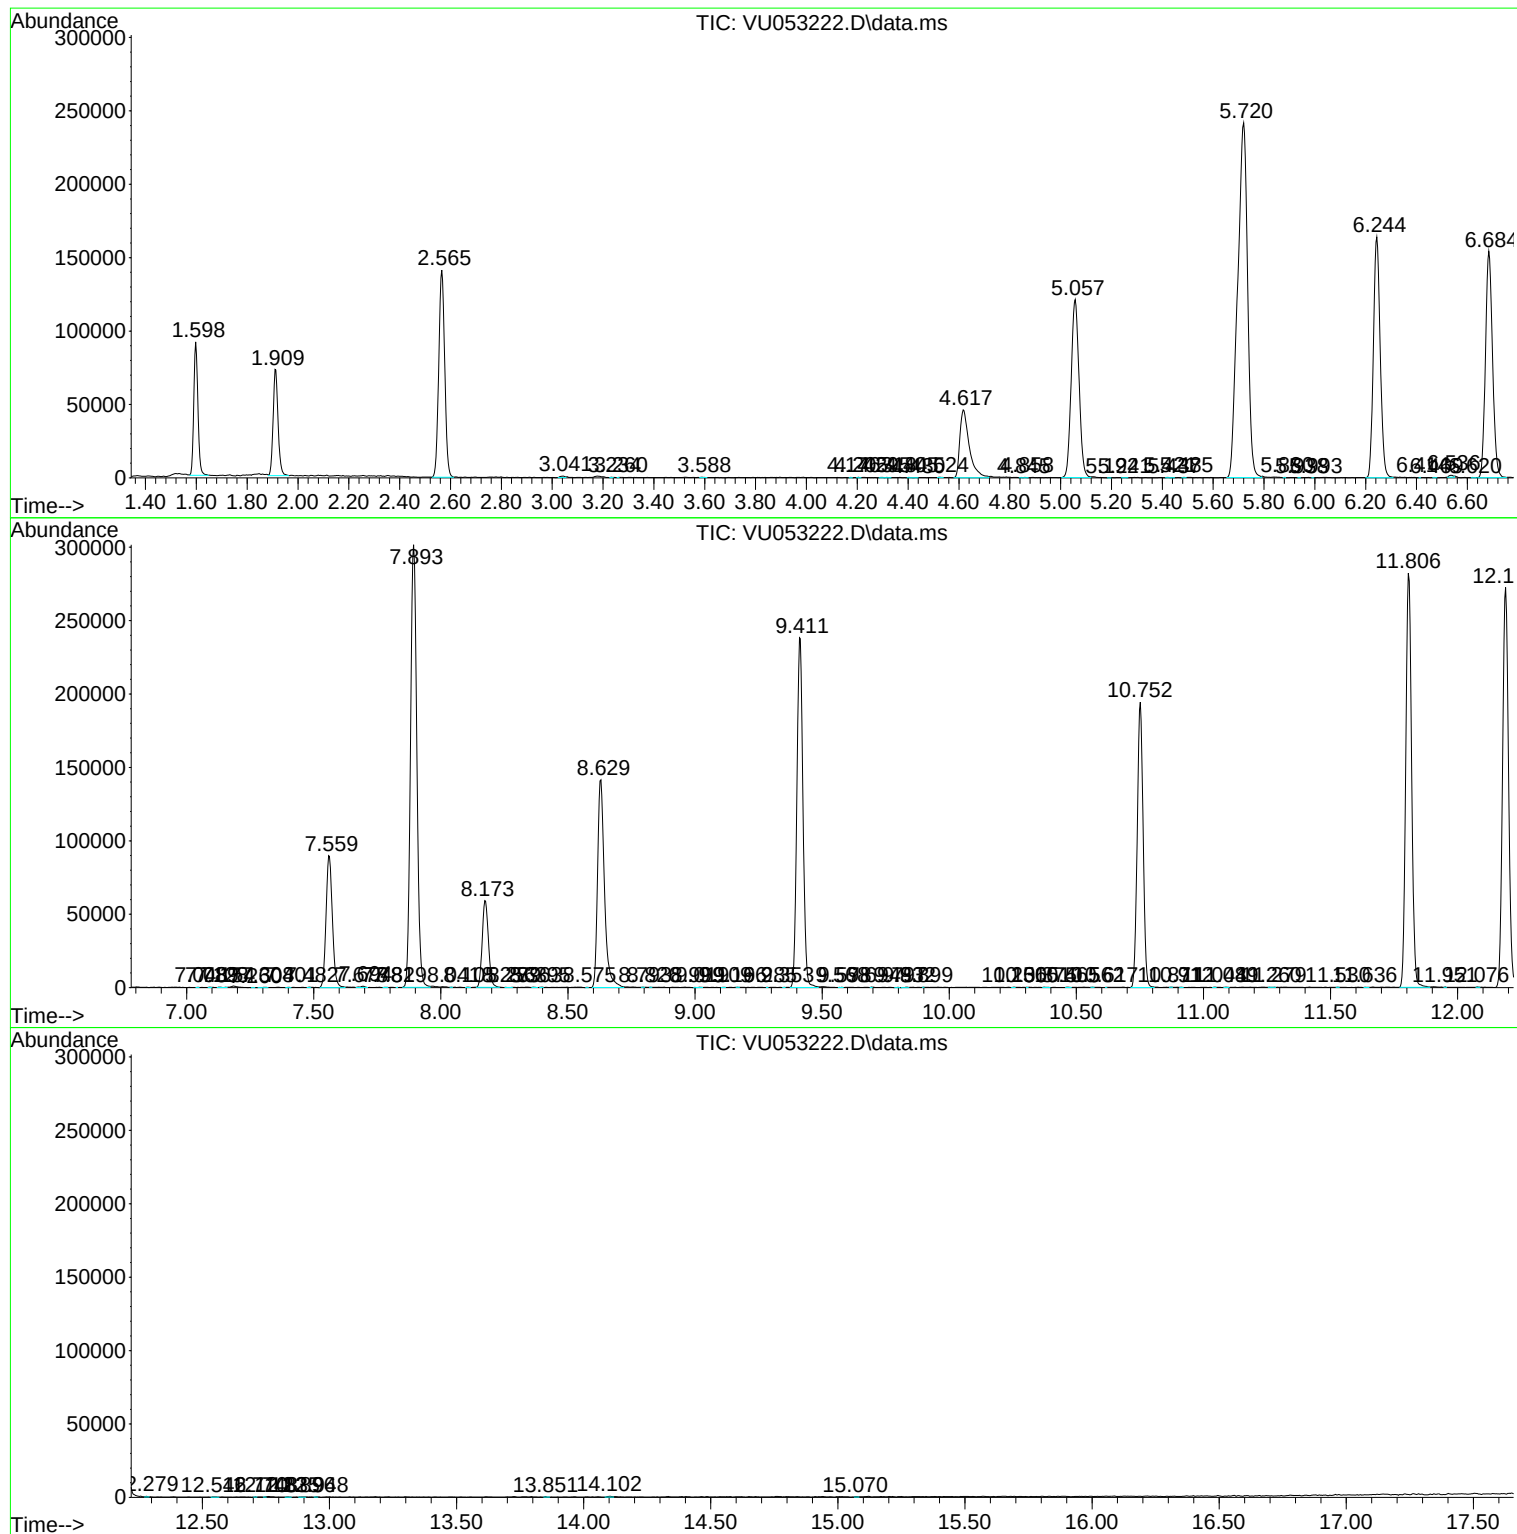

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053222.D
Acq On : 16 Mar 2023 13:33
Operator : JC/MD
Sample : 01930-01 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053222.D
Acq On : 16 Mar 2023 13:33
Operator : JC/MD
Sample : 01930-01 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------