

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053226.D
 Acq On : 16 Mar 2023 15:08
 Operator : JC/MD
 Sample : 01930-05 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053226.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rVB	83754	95314	15.43%	2.116%
2	1.909	170	177	195	rVB	66384	90309	14.62%	2.005%
3	2.565	369	381	396	rVB	133431	216127	34.99%	4.799%
4	3.041	523	529	535	rBV2	634	817	0.13%	0.018%
5	3.613	704	707	711	rBV2	248	210	0.03%	0.005%
6	3.951	808	812	820	rVB2	250	279	0.05%	0.006%
7	4.031	832	837	841	rVV2	230	279	0.05%	0.006%
8	4.221	888	896	899	rBV2	291	457	0.07%	0.010%
9	4.256	904	907	910	rBV2	252	183	0.03%	0.004%
10	4.295	916	919	923	rBV2	207	160	0.03%	0.004%
11	4.349	933	936	939	rVB	211	112	0.02%	0.002%
12	4.411	951	955	957	rBV	175	143	0.02%	0.003%
13	4.475	970	975	977	rBV2	244	213	0.03%	0.005%
14	4.517	985	988	990	rBV	214	152	0.02%	0.003%
15	4.613	1007	1018	1048	rBV2	45309	114801	18.58%	2.549%
16	4.922	1111	1114	1118	rBV	150	84	0.01%	0.002%
17	5.057	1140	1156	1180	rBV2	114396	248281	40.19%	5.513%
18	5.256	1216	1218	1219	rBV2	150	63	0.01%	0.001%
19	5.378	1254	1256	1258	rVB	191	81	0.01%	0.002%
20	5.394	1258	1261	1262	rBV	133	71	0.01%	0.002%
21	5.452	1276	1279	1282	rVB	207	145	0.02%	0.003%
22	5.478	1285	1287	1291	rVB	163	65	0.01%	0.001%
23	5.607	1323	1327	1330	rBV2	193	140	0.02%	0.003%
24	5.719	1341	1362	1386	rBV2	228924	617740	100.00%	13.716%
25	5.915	1420	1423	1427	rVB2	347	250	0.04%	0.006%
26	5.957	1433	1436	1439	rVB2	213	147	0.02%	0.003%
27	6.031	1457	1459	1462	rVB2	177	91	0.01%	0.002%
28	6.047	1462	1464	1466	rVB	162	60	0.01%	0.001%
29	6.070	1469	1471	1473	rVB	198	81	0.01%	0.002%
30	6.083	1473	1475	1480	rBV	225	160	0.03%	0.004%
31	6.137	1490	1492	1494	rBV	139	58	0.01%	0.001%
32	6.243	1512	1525	1544	rBV	166278	311977	50.50%	6.927%
33	6.385	1567	1569	1572	rBV2	276	179	0.03%	0.004%
34	6.623	1640	1643	1646	rBV	231	132	0.02%	0.003%
35	6.684	1649	1662	1682	rBV	145918	280179	45.36%	6.221%
36	6.806	1693	1700	1705	rBV2	516	649	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053226.D
 Acq On : 16 Mar 2023 15:08
 Operator : JC/MD
 Sample : 01930-05 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.838	1705	1710	1714	rBV	193	236	0.04%	0.005%
38	6.915	1731	1734	1738	rBV	254	192	0.03%	0.004%
39	6.957	1744	1747	1749	rBV2	116	85	0.01%	0.002%
40	7.044	1771	1774	1776	rBV2	204	131	0.02%	0.003%
41	7.218	1826	1828	1833	rBV2	205	161	0.03%	0.004%
42	7.256	1837	1840	1841	rBV2	165	71	0.01%	0.002%
43	7.439	1895	1897	1899	rBV	153	78	0.01%	0.002%
44	7.562	1923	1935	1952	rBV	81463	146026	23.64%	3.242%
45	7.642	1957	1960	1961	rBV	196	97	0.02%	0.002%
46	7.777	1998	2002	2004	rBV2	172	123	0.02%	0.003%
47	7.796	2007	2008	2012	rVB	187	72	0.01%	0.002%
48	7.816	2012	2014	2018	rBV	185	106	0.02%	0.002%
49	7.845	2020	2023	2024	rBV	161	72	0.01%	0.002%
50	7.893	2025	2038	2064	rBV	282229	489161	79.19%	10.861%
51	8.176	2115	2126	2140	rBV	57801	96583	15.63%	2.144%
52	8.317	2167	2170	2174	rBV2	199	199	0.03%	0.004%
53	8.378	2187	2189	2191	rBV	156	86	0.01%	0.002%
54	8.488	2220	2223	2225	rBV2	242	186	0.03%	0.004%
55	8.517	2230	2232	2235	rBV	154	64	0.01%	0.001%
56	8.555	2241	2244	2246	rBV	168	103	0.02%	0.002%
57	8.629	2256	2267	2291	rBV2	139064	252342	40.85%	5.603%
58	8.893	2345	2349	2351	rBV	160	131	0.02%	0.003%
59	9.076	2401	2406	2407	rBV	180	174	0.03%	0.004%
60	9.092	2409	2411	2413	rVB	198	99	0.02%	0.002%
61	9.185	2437	2440	2444	rBV2	173	123	0.02%	0.003%
62	9.414	2498	2511	2529	rBV	232603	386943	62.64%	8.591%
63	9.558	2554	2556	2559	rVB	222	104	0.02%	0.002%
64	9.578	2559	2562	2564	rBV	175	82	0.01%	0.002%
65	9.658	2585	2587	2589	rBV	203	112	0.02%	0.002%
66	9.700	2596	2600	2602	rBV2	305	201	0.03%	0.004%
67	9.716	2602	2605	2610	rBV2	215	183	0.03%	0.004%
68	9.758	2615	2618	2621	rVV2	157	104	0.02%	0.002%
69	9.822	2636	2638	2640	rBV	180	118	0.02%	0.003%
70	9.857	2646	2649	2652	rBV2	173	113	0.02%	0.003%
71	9.931	2669	2672	2677	rVB	228	140	0.02%	0.003%
72	10.008	2692	2696	2701	rBV2	325	417	0.07%	0.009%
73	10.076	2714	2717	2718	rBV	137	78	0.01%	0.002%
74	10.751	2914	2927	2941	rBV	186300	293223	47.47%	6.510%
75	11.018	3008	3010	3013	rBV	211	172	0.03%	0.004%
76	11.137	3043	3047	3050	rBV	279	270	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053226.D
 Acq On : 16 Mar 2023 15:08
 Operator : JC/MD
 Sample : 01930-05 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	11.208	3067	3069	3072	rBV	155	94	0.02%	0.002%
78	11.253	3081	3083	3087	rVB	273	143	0.02%	0.003%
79	11.275	3087	3090	3092	rBV	159	104	0.02%	0.002%
80	11.359	3114	3116	3119	rBV	145	73	0.01%	0.002%
81	11.455	3144	3146	3147	rBV	171	90	0.01%	0.002%
82	11.674	3210	3214	3216	rBV2	211	122	0.02%	0.003%
83	11.696	3219	3221	3223	rBV	196	101	0.02%	0.002%
84	11.809	3243	3256	3278	rBV	281177	445230	72.07%	9.885%
85	11.967	3303	3305	3307	rBV	161	68	0.01%	0.002%
86	11.983	3307	3310	3313	rBV	164	120	0.02%	0.003%
87	12.188	3362	3374	3394	rBV	253565	406662	65.83%	9.029%
88	12.375	3430	3432	3434	rBV	209	122	0.02%	0.003%
89	12.568	3490	3492	3496	rVB2	240	150	0.02%	0.003%
90	13.140	3667	3670	3673	rBV	259	162	0.03%	0.004%
91	13.272	3708	3711	3715	rBV2	179	141	0.02%	0.003%
92	13.487	3775	3778	3782	rBV	347	209	0.03%	0.005%
93	13.555	3797	3799	3801	rBV	194	80	0.01%	0.002%
94	13.838	3884	3887	3889	rBV2	220	149	0.02%	0.003%
95	14.102	3966	3969	3972	rBV2	304	225	0.04%	0.005%
96	14.224	4005	4007	4009	rBV	193	79	0.01%	0.002%
97	14.301	4029	4031	4034	rBV	299	202	0.03%	0.004%
98	14.384	4054	4057	4060	rVB	302	171	0.03%	0.004%
99	15.008	4249	4251	4252	rBV	181	82	0.01%	0.002%
100	15.436	4381	4384	4385	rBV2	296	171	0.03%	0.004%




Sum of corrected areas: 4503900

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053226.D
Acq On : 16 Mar 2023 15:08
Operator : JC/MD
Sample : 01930-05 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

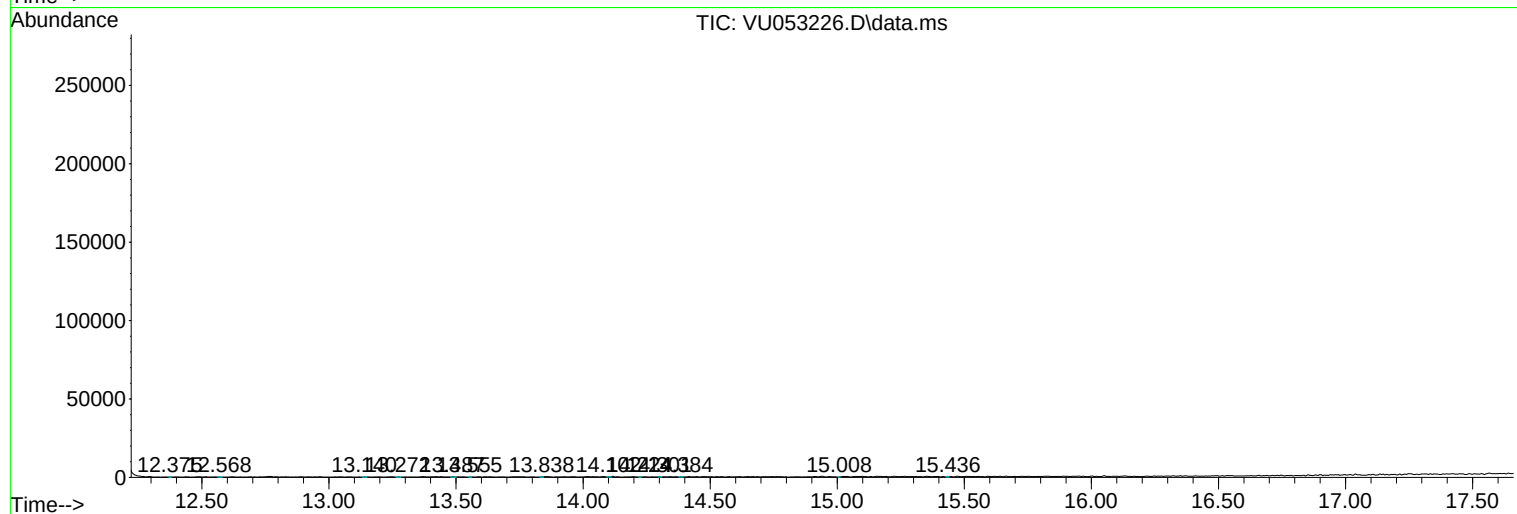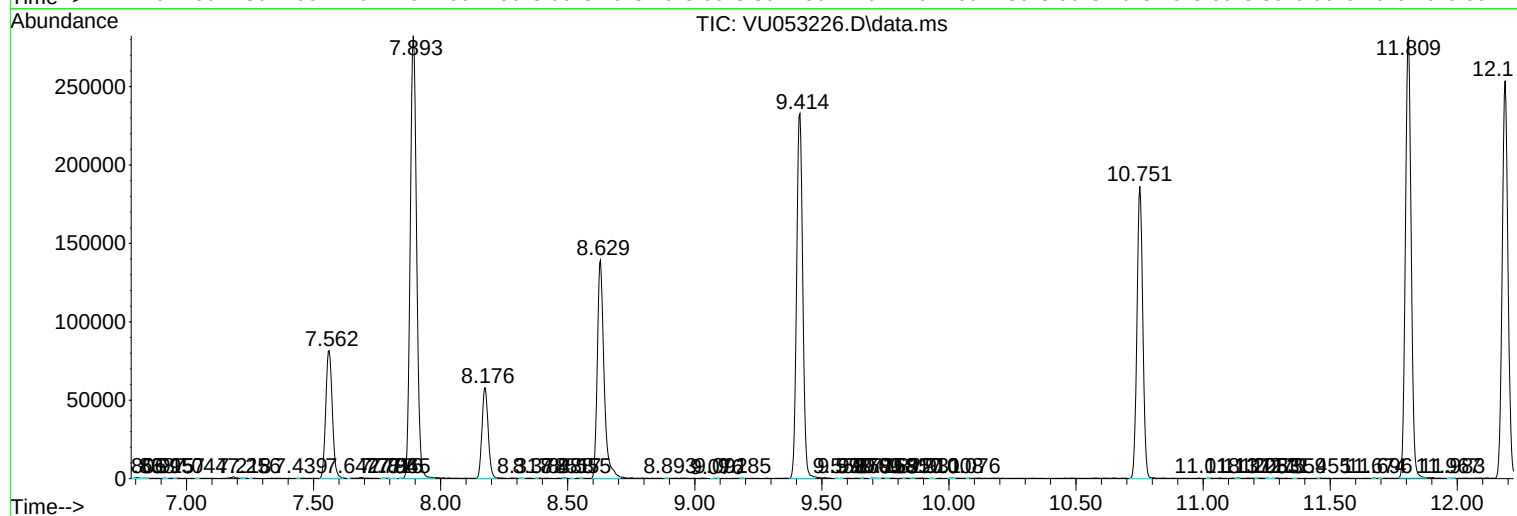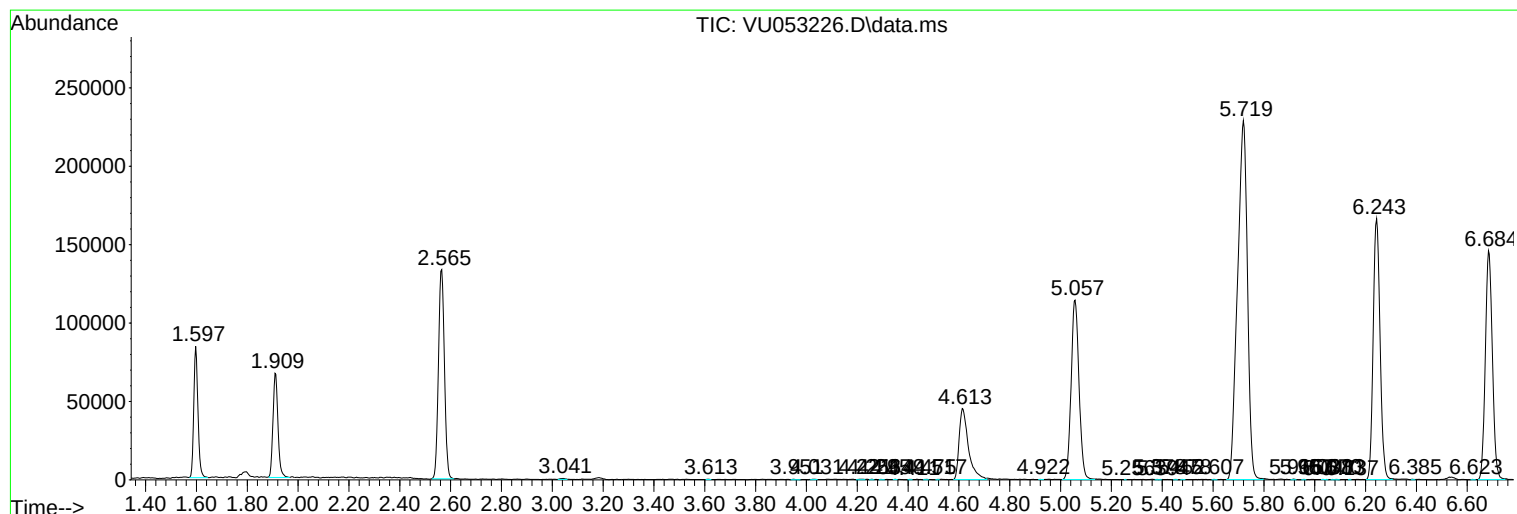

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053226.D
Acq On : 16 Mar 2023 15:08
Operator : JC/MD
Sample : 01930-05 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053226.D
Acq On : 16 Mar 2023 15:08
Operator : JC/MD
Sample : 01930-05 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------