

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053227.D
 Acq On : 16 Mar 2023 15:31
 Operator : JC/MD
 Sample : 01929-20 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053227.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rVB2	103861	126373	20.55%	2.804%
2	1.912	170	178	192	rVB	66379	88288	14.35%	1.959%
3	2.565	369	381	395	rVB	130151	210197	34.17%	4.664%
4	2.845	465	468	474	rBV	254	277	0.05%	0.006%
5	3.620	705	709	712	rBV	216	234	0.04%	0.005%
6	3.729	741	743	747	rBV2	189	151	0.02%	0.003%
7	3.826	766	773	781	rBV2	275	531	0.09%	0.012%
8	3.928	802	805	807	rBV2	152	117	0.02%	0.003%
9	3.989	821	824	826	rBV	290	157	0.03%	0.003%
10	4.141	869	871	873	rBV	185	96	0.02%	0.002%
11	4.227	896	898	900	rBV	189	89	0.01%	0.002%
12	4.430	957	961	963	rBV2	248	188	0.03%	0.004%
13	4.465	970	972	978	rBV	172	87	0.01%	0.002%
14	4.613	1005	1018	1027	rBV2	46771	107296	17.44%	2.381%
15	4.887	1100	1103	1109	rBV3	283	305	0.05%	0.007%
16	4.993	1133	1136	1137	rBV3	160	71	0.01%	0.002%
17	5.057	1140	1156	1181	rVV	114550	247357	40.21%	5.489%
18	5.163	1185	1189	1191	rBV2	230	196	0.03%	0.004%
19	5.449	1276	1278	1281	rBV2	202	114	0.02%	0.003%
20	5.719	1341	1362	1382	rBV2	227133	615090	100.00%	13.649%
21	5.944	1429	1432	1434	rBV	260	197	0.03%	0.004%
22	5.970	1438	1440	1442	rBV	203	98	0.02%	0.002%
23	6.038	1459	1461	1462	rBV	165	92	0.01%	0.002%
24	6.134	1488	1491	1494	rBV	271	210	0.03%	0.005%
25	6.150	1494	1496	1500	rVV2	177	111	0.02%	0.002%
26	6.243	1511	1525	1544	rBV	164023	307234	49.95%	6.817%
27	6.407	1573	1576	1579	rVB	200	106	0.02%	0.002%
28	6.456	1589	1591	1595	rVB	192	79	0.01%	0.002%
29	6.478	1595	1598	1599	rBV	141	101	0.02%	0.002%
30	6.533	1609	1615	1628	rVB10	1719	3399	0.55%	0.075%
31	6.581	1628	1630	1632	rBV	310	196	0.03%	0.004%
32	6.639	1646	1648	1649	rBV2	170	86	0.01%	0.002%
33	6.684	1649	1662	1687	rVV	144854	282055	45.86%	6.259%
34	6.800	1696	1698	1703	rBV2	264	267	0.04%	0.006%
35	6.960	1745	1748	1753	rBV2	210	179	0.03%	0.004%
36	6.996	1753	1759	1768	rVB2	429	697	0.11%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053227.D
 Acq On : 16 Mar 2023 15:31
 Operator : JC/MD
 Sample : 01929-20 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	7.034	1768	1771	1773	rBV	126	111	0.02%	0.002%
38	7.047	1773	1775	1778	rBV	175	103	0.02%	0.002%
39	7.070	1778	1782	1791	rVB	455	576	0.09%	0.013%
40	7.115	1791	1796	1798	rBV	301	298	0.05%	0.007%
41	7.176	1812	1815	1816	rBV	558	286	0.05%	0.006%
42	7.407	1884	1887	1893	rVV2	232	201	0.03%	0.004%
43	7.430	1893	1894	1897	rVB	170	88	0.01%	0.002%
44	7.562	1923	1935	1956	rBV	82303	145129	23.59%	3.220%
45	7.639	1956	1959	1962	rVB3	323	202	0.03%	0.004%
46	7.661	1962	1966	1968	rBV	215	149	0.02%	0.003%
47	7.748	1991	1993	1996	rVB2	286	194	0.03%	0.004%
48	7.771	1996	2000	2002	rBV	190	177	0.03%	0.004%
49	7.800	2007	2009	2011	rBV	176	102	0.02%	0.002%
50	7.829	2014	2018	2023	rBV	238	266	0.04%	0.006%
51	7.893	2025	2038	2060	rBV	283155	483679	78.64%	10.733%
52	8.079	2093	2096	2098	rBV	306	178	0.03%	0.004%
53	8.173	2114	2125	2143	rBV	57135	94954	15.44%	2.107%
54	8.250	2148	2149	2152	rVB	192	74	0.01%	0.002%
55	8.356	2180	2182	2184	rBV	145	77	0.01%	0.002%
56	8.439	2205	2208	2209	rBV	198	130	0.02%	0.003%
57	8.494	2222	2225	2227	rBV2	145	106	0.02%	0.002%
58	8.587	2250	2254	2256	rBV	174	139	0.02%	0.003%
59	8.629	2256	2267	2290	rBV2	136946	252224	41.01%	5.597%
60	9.025	2387	2390	2392	rVB	188	102	0.02%	0.002%
61	9.173	2435	2436	2441	rVB	181	81	0.01%	0.002%
62	9.224	2450	2452	2456	rVB2	186	141	0.02%	0.003%
63	9.333	2483	2486	2490	rVB	222	137	0.02%	0.003%
64	9.414	2499	2511	2530	rBV	238104	389185	63.27%	8.636%
65	9.546	2549	2552	2555	rVB	177	81	0.01%	0.002%
66	9.642	2579	2582	2589	rVB	260	202	0.03%	0.004%
67	9.681	2590	2594	2597	rVB	379	336	0.05%	0.007%
68	9.706	2598	2602	2603	rBV2	357	282	0.05%	0.006%
69	9.845	2643	2645	2647	rVB	196	95	0.02%	0.002%
70	10.041	2704	2706	2713	rVB2	287	283	0.05%	0.006%
71	10.179	2747	2749	2752	rVB	166	71	0.01%	0.002%
72	10.279	2776	2780	2784	rBV	208	187	0.03%	0.004%
73	10.751	2915	2927	2944	rBV	185652	293422	47.70%	6.511%
74	10.835	2949	2953	2954	rBV	188	112	0.02%	0.002%
75	11.230	3074	3076	3078	rBV	210	139	0.02%	0.003%
76	11.288	3092	3094	3096	rBV	191	79	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053227.D
 Acq On : 16 Mar 2023 15:31
 Operator : JC/MD
 Sample : 01929-20 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M

Title : VOC Analysis

77	11.404	3128	3130	3132	rBV2	190	117	0.02%	0.003%
78	11.468	3147	3150	3153	rBV	246	146	0.02%	0.003%
79	11.578	3181	3184	3187	rBV	194	161	0.03%	0.004%
80	11.613	3192	3195	3198	rBV	270	195	0.03%	0.004%
81	11.713	3223	3226	3233	rVB2	244	175	0.03%	0.004%
82	11.761	3238	3241	3243	rBV	227	166	0.03%	0.004%
83	11.806	3243	3255	3274	rBV	273113	436846	71.02%	9.694%
84	12.018	3319	3321	3322	rBV	175	78	0.01%	0.002%
85	12.092	3342	3344	3348	rBV	164	120	0.02%	0.003%
86	12.147	3358	3361	3362	rBV2	214	117	0.02%	0.003%
87	12.189	3362	3374	3398	rVV	254020	409338	66.55%	9.083%
88	12.430	3445	3449	3450	rBV	203	141	0.02%	0.003%
89	12.488	3465	3467	3469	rBV	177	114	0.02%	0.003%
90	12.767	3549	3554	3558	rVB2	357	407	0.07%	0.009%
91	12.793	3558	3562	3563	rBV	281	187	0.03%	0.004%
92	13.140	3667	3670	3673	rBV2	242	188	0.03%	0.004%
93	13.243	3700	3702	3705	rBV	241	133	0.02%	0.003%
94	13.385	3743	3746	3750	rBV2	208	160	0.03%	0.004%
95	13.442	3761	3764	3767	rVB	260	133	0.02%	0.003%
96	13.484	3773	3777	3780	rBV2	235	196	0.03%	0.004%
97	14.404	4060	4063	4067	rBV2	313	230	0.04%	0.005%
98	14.558	4108	4111	4113	rBV	293	170	0.03%	0.004%
99	15.053	4262	4265	4268	rBV	363	196	0.03%	0.004%
100	15.323	4347	4349	4351	rBV2	257	150	0.02%	0.003%




Sum of corrected areas: 4506563

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053227.D
Acq On : 16 Mar 2023 15:31
Operator : JC/MD
Sample : 01929-20 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

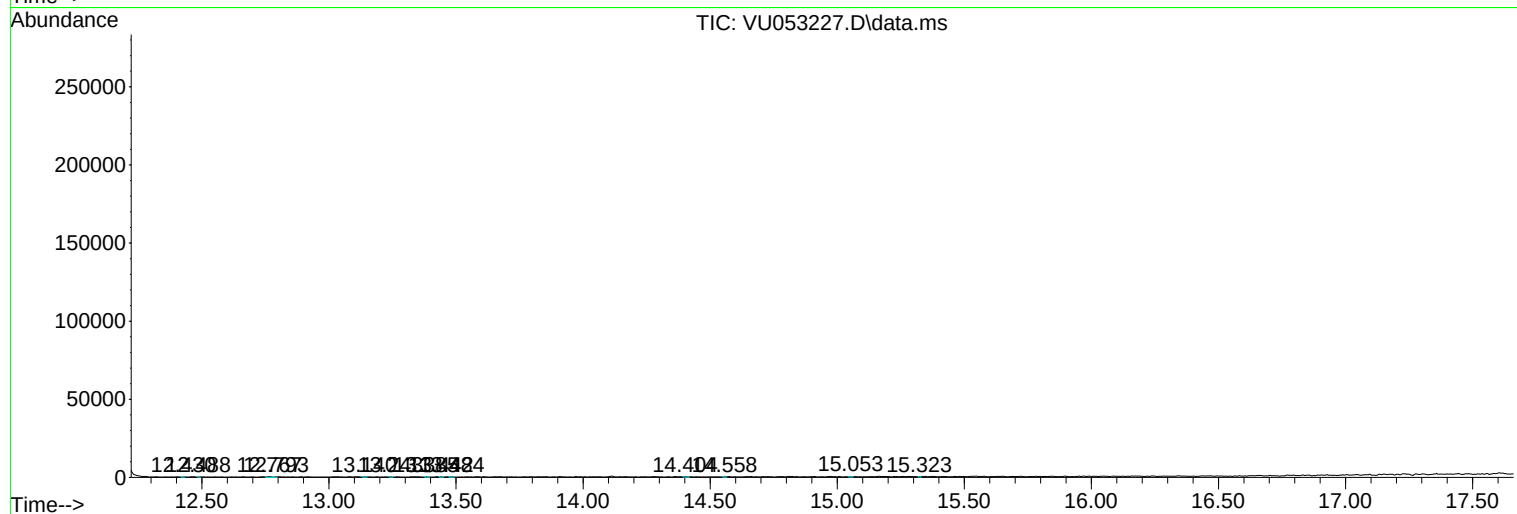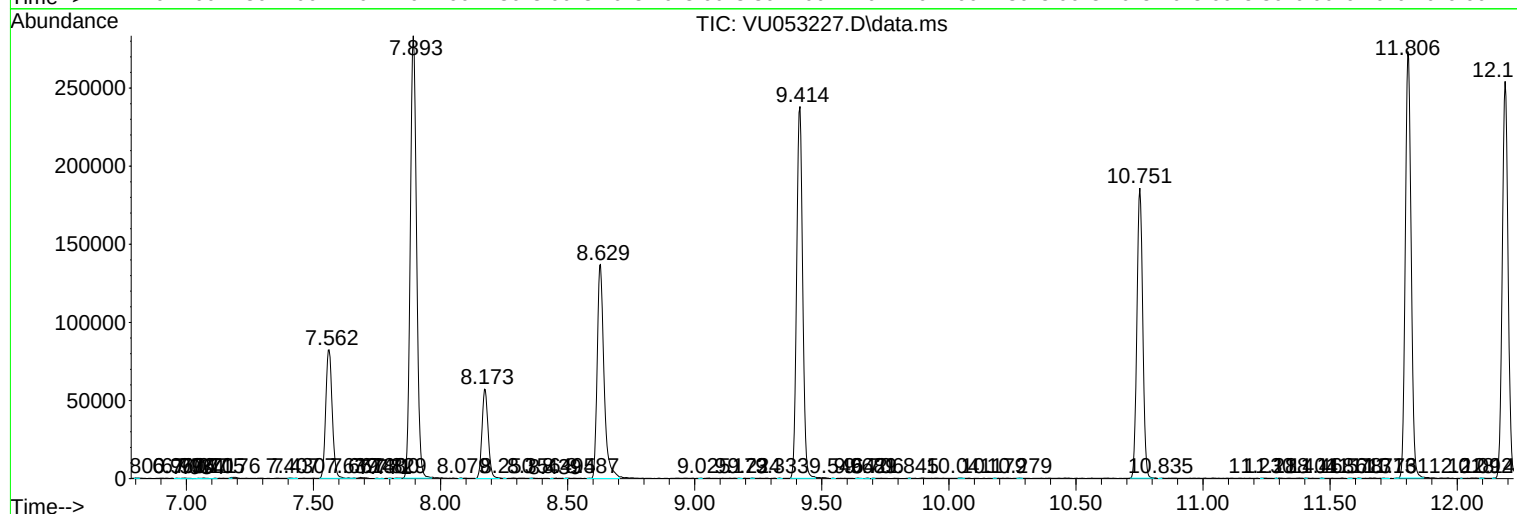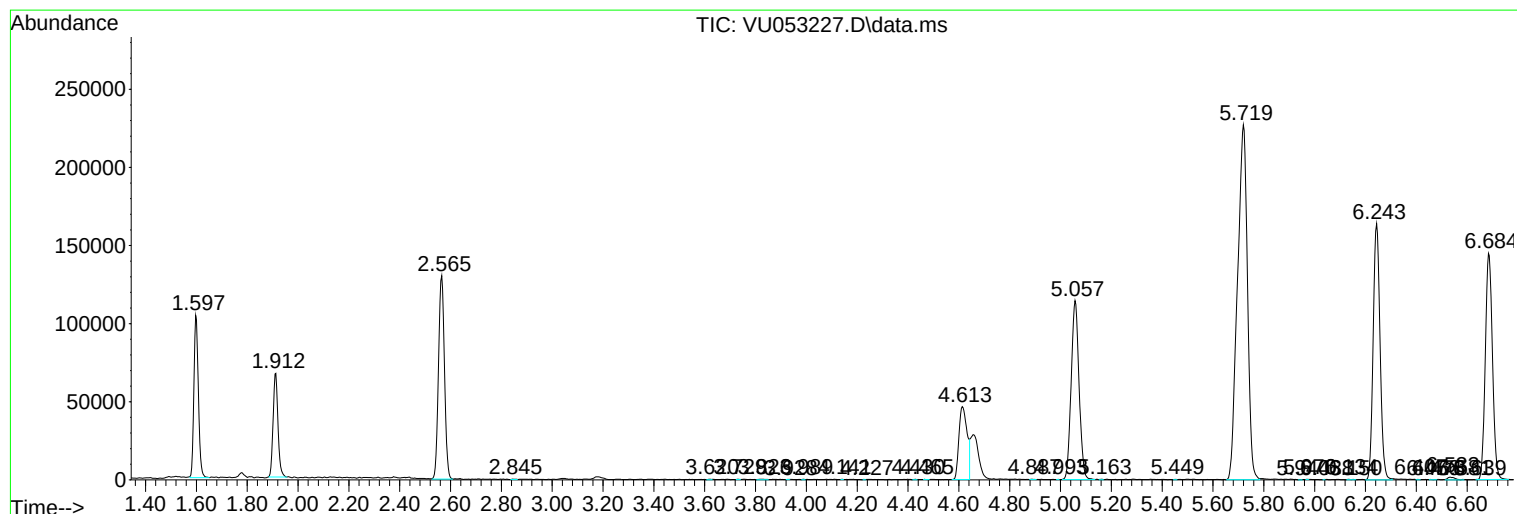

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053227.D
Acq On : 16 Mar 2023 15:31
Operator : JC/MD
Sample : 01929-20 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053227.D
Acq On : 16 Mar 2023 15:31
Operator : JC/MD
Sample : 01929-20 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc