

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053229.D
 Acq On : 16 Mar 2023 16:19
 Operator : JC/MD
 Sample : 01930-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053229.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB2	102639	129372	21.45%	2.804%
2	1.909	170	177	198	rVB	64288	89488	14.83%	1.939%
3	2.565	369	381	396	rBV	125888	202110	33.50%	4.380%
4	3.044	527	530	532	rBV	588	331	0.05%	0.007%
5	3.163	565	567	568	rBV	296	141	0.02%	0.003%
6	3.292	604	607	613	rBV	259	261	0.04%	0.006%
7	3.350	622	625	630	rVB3	551	440	0.07%	0.010%
8	3.703	730	735	738	rBV2	252	250	0.04%	0.005%
9	4.018	830	833	835	rBV	237	141	0.02%	0.003%
10	4.192	885	887	889	rBV	185	76	0.01%	0.002%
11	4.359	935	939	941	rVB	164	114	0.02%	0.002%
12	4.491	978	980	985	rVB	235	135	0.02%	0.003%
13	4.575	1004	1006	1008	rBV2	193	99	0.02%	0.002%
14	4.616	1008	1019	1046	rVV	46732	127607	21.15%	2.766%
15	4.854	1090	1093	1096	rBV2	226	204	0.03%	0.004%
16	4.986	1132	1134	1137	rVB	230	87	0.01%	0.002%
17	5.057	1140	1156	1175	rVV2	111708	246144	40.80%	5.334%
18	5.218	1204	1206	1209	rBV	151	65	0.01%	0.001%
19	5.272	1216	1223	1225	rBV	266	340	0.06%	0.007%
20	5.350	1245	1247	1249	rVB	174	66	0.01%	0.001%
21	5.430	1269	1272	1278	rVB	184	129	0.02%	0.003%
22	5.459	1278	1281	1282	rBV	158	72	0.01%	0.002%
23	5.501	1292	1294	1297	rVB	212	76	0.01%	0.002%
24	5.555	1309	1311	1314	rVB	130	73	0.01%	0.002%
25	5.581	1318	1319	1322	rVB	158	42	0.01%	0.001%
26	5.604	1323	1326	1330	rBV	235	153	0.03%	0.003%
27	5.719	1340	1362	1384	rBV2	223606	603270	100.00%	13.074%
28	5.890	1411	1415	1416	rBV2	215	155	0.03%	0.003%
29	6.031	1456	1459	1461	rVB2	191	112	0.02%	0.002%
30	6.115	1484	1485	1486	rBV2	117	30	0.00%	0.001%
31	6.153	1494	1497	1501	rVB2	199	148	0.02%	0.003%
32	6.243	1512	1525	1548	rBV	197409	370111	61.35%	8.021%
33	6.385	1566	1569	1572	rBV	356	236	0.04%	0.005%
34	6.414	1576	1578	1580	rBV	133	61	0.01%	0.001%
35	6.478	1596	1598	1600	rBV2	219	107	0.02%	0.002%
36	6.533	1608	1615	1616	rBV4	1406	1285	0.21%	0.028%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053229.D
 Acq On : 16 Mar 2023 16:19
 Operator : JC/MD
 Sample : 01930-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.584	1629	1631	1634	rVB	234	142	0.02%	0.003%
38	6.636	1644	1647	1649	rBV2	176	122	0.02%	0.003%
39	6.687	1649	1663	1686	rVV	142458	274639	45.53%	5.952%
40	6.784	1691	1693	1696	rBV	165	122	0.02%	0.003%
41	6.806	1696	1700	1701	rBV	178	126	0.02%	0.003%
42	6.838	1708	1710	1713	rBV	128	38	0.01%	0.001%
43	6.861	1713	1717	1719	rBV	276	223	0.04%	0.005%
44	6.915	1731	1734	1737	rVB2	225	132	0.02%	0.003%
45	6.986	1752	1756	1759	rBV2	245	199	0.03%	0.004%
46	7.041	1772	1773	1775	rVB	148	35	0.01%	0.001%
47	7.157	1807	1809	1811	rBV	141	71	0.01%	0.002%
48	7.192	1811	1820	1826	rVB4	1061	1718	0.28%	0.037%
49	7.443	1896	1898	1899	rBV4	141	58	0.01%	0.001%
50	7.562	1923	1935	1951	rBV2	81309	143674	23.82%	3.114%
51	7.755	1993	1995	1996	rBV2	117	64	0.01%	0.001%
52	7.796	2006	2008	2010	rBV	403	216	0.04%	0.005%
53	7.893	2024	2038	2056	rBV	277635	478357	79.29%	10.367%
54	8.041	2082	2084	2086	rVB	214	82	0.01%	0.002%
55	8.054	2086	2088	2091	rBV2	195	109	0.02%	0.002%
56	8.073	2092	2094	2097	rBV	159	75	0.01%	0.002%
57	8.105	2103	2104	2106	rVB	115	26	0.00%	0.001%
58	8.173	2113	2125	2142	rBV	55716	93193	15.45%	2.020%
59	8.276	2155	2157	2158	rVB	115	27	0.00%	0.001%
60	8.317	2167	2170	2173	rBV	154	102	0.02%	0.002%
61	8.356	2180	2182	2184	rVB	132	31	0.01%	0.001%
62	8.372	2185	2187	2190	rVV	182	85	0.01%	0.002%
63	8.394	2191	2194	2197	rVB	185	96	0.02%	0.002%
64	8.478	2214	2220	2223	rBV	422	427	0.07%	0.009%
65	8.565	2242	2247	2248	rBV	188	174	0.03%	0.004%
66	8.629	2256	2267	2296	rBV2	140425	257474	42.68%	5.580%
67	8.909	2351	2354	2356	rBV	151	101	0.02%	0.002%
68	8.996	2380	2381	2386	rBV	149	98	0.02%	0.002%
69	9.018	2386	2388	2389	rBV	141	39	0.01%	0.001%
70	9.195	2440	2443	2446	rVB2	216	143	0.02%	0.003%
71	9.414	2498	2511	2534	rBV	273692	454857	75.40%	9.858%
72	9.571	2558	2560	2561	rBV	173	70	0.01%	0.002%
73	9.767	2619	2621	2622	rBV	116	46	0.01%	0.001%
74	9.787	2625	2627	2629	rVV	120	33	0.01%	0.001%
75	9.970	2681	2684	2688	rBV	435	210	0.03%	0.005%
76	10.076	2714	2717	2721	rVB	176	97	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053229.D
 Acq On : 16 Mar 2023 16:19
 Operator : JC/MD
 Sample : 01930-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.176	2741	2748	2751	rBV	379	464	0.08%	0.010%
78	10.317	2789	2792	2798	rVB2	285	321	0.05%	0.007%
79	10.626	2885	2888	2889	rBV2	223	107	0.02%	0.002%
80	10.751	2914	2927	2941	rBV	179725	284928	47.23%	6.175%
81	10.947	2985	2988	2991	rVB	253	143	0.02%	0.003%
82	10.970	2992	2995	2998	rBV	269	150	0.02%	0.003%
83	11.140	3042	3048	3054	rBV	344	479	0.08%	0.010%
84	11.410	3128	3132	3134	rBV2	181	152	0.03%	0.003%
85	11.558	3175	3178	3180	rBV	141	79	0.01%	0.002%
86	11.590	3186	3188	3191	rBV2	147	92	0.02%	0.002%
87	11.806	3244	3255	3275	rBV	289189	452413	74.99%	9.805%
88	12.189	3362	3374	3395	rBV	246209	392471	65.06%	8.506%
89	12.465	3457	3460	3464	rBV	165	112	0.02%	0.002%
90	12.536	3480	3482	3485	rBV	161	76	0.01%	0.002%
91	12.635	3510	3513	3516	rBV2	243	183	0.03%	0.004%
92	12.816	3565	3569	3570	rBV	224	163	0.03%	0.004%
93	12.873	3584	3587	3591	rBV2	262	283	0.05%	0.006%
94	13.317	3722	3725	3729	rBV	280	232	0.04%	0.005%
95	13.992	3933	3935	3939	rBV	213	121	0.02%	0.003%
96	14.729	4161	4164	4167	rBV	268	170	0.03%	0.004%




Sum of corrected areas: 4614201

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053229.D
Acq On : 16 Mar 2023 16:19
Operator : JC/MD
Sample : 01930-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

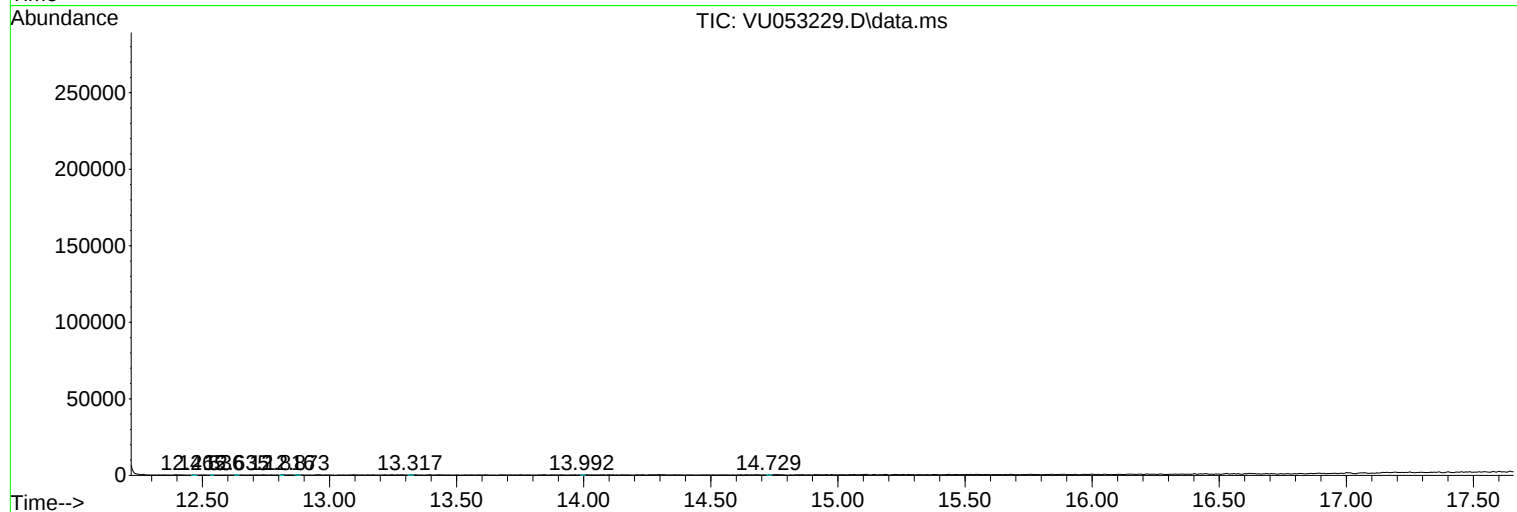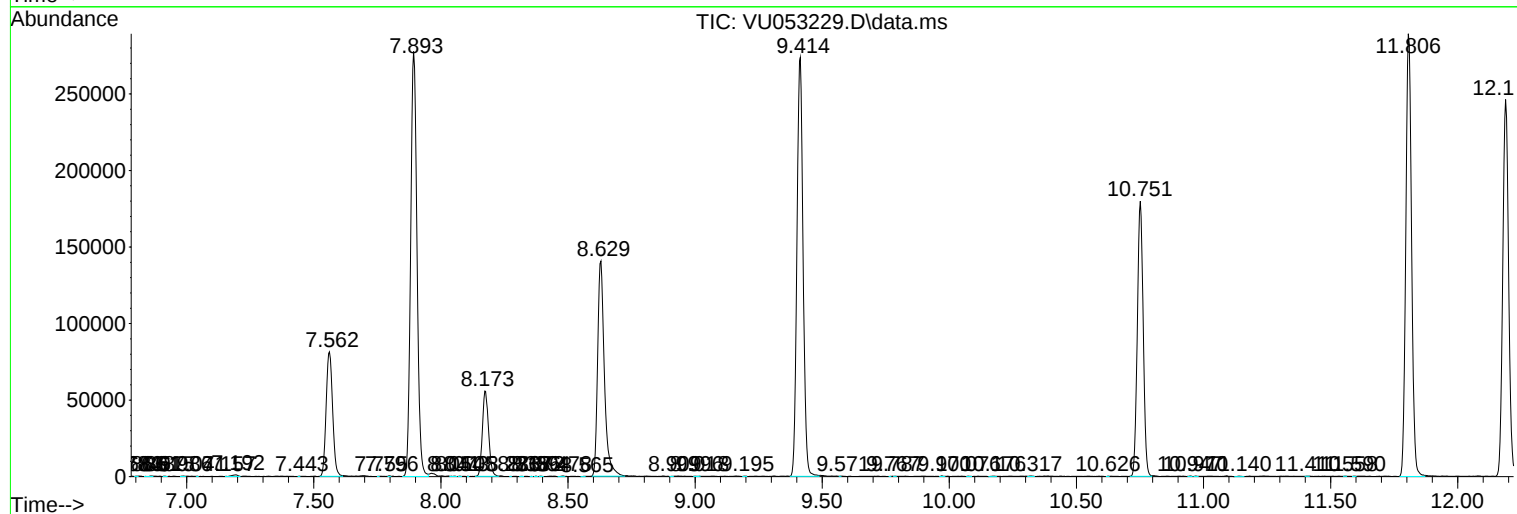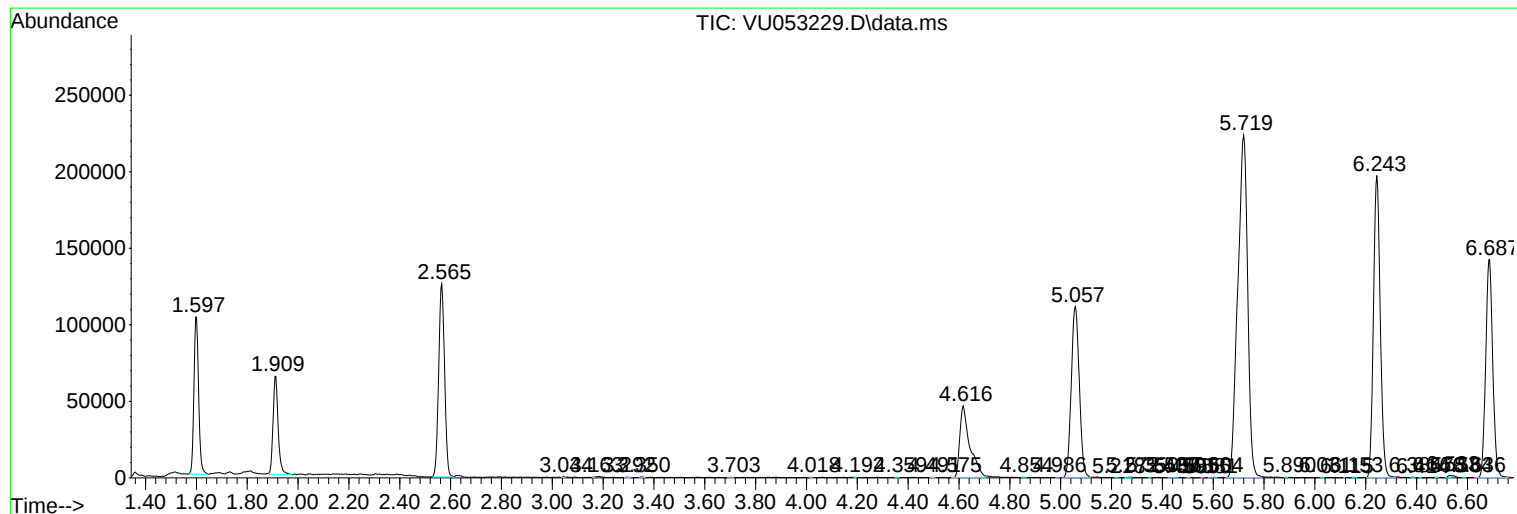

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053229.D
Acq On : 16 Mar 2023 16:19
Operator : JC/MD
Sample : 01930-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053229.D
Acq On : 16 Mar 2023 16:19
Operator : JC/MD
Sample : 01930-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc