

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053233.D
 Acq On : 16 Mar 2023 17:52
 Operator : JC/MD
 Sample : 01930-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053233.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.466	34	39	54	rBV	10637	17112	2.81%	0.377%
2	1.597	73	80	99	rVB2	87162	103121	16.96%	2.271%
3	1.912	170	178	189	rBV	61290	82288	13.53%	1.812%
4	2.565	369	381	394	rBV	123718	198998	32.72%	4.383%
5	3.019	519	522	525	rBV	309	218	0.04%	0.005%
6	3.038	525	528	534	rVB3	361	355	0.06%	0.008%
7	3.867	774	786	800	rVB2	2716	5879	0.97%	0.129%
8	4.031	833	837	840	rBV	187	150	0.02%	0.003%
9	4.102	855	859	867	rVB2	289	340	0.06%	0.007%
10	4.276	908	913	919	rVB	204	203	0.03%	0.004%
11	4.559	998	1001	1003	rBV	144	60	0.01%	0.001%
12	4.613	1006	1018	1048	rBV	46032	117792	19.37%	2.594%
13	4.896	1104	1106	1108	rBV	188	81	0.01%	0.002%
14	5.057	1140	1156	1177	rBV	109924	239770	39.43%	5.281%
15	5.221	1204	1207	1213	rVB	276	217	0.04%	0.005%
16	5.404	1262	1264	1268	rBV2	160	117	0.02%	0.003%
17	5.498	1289	1293	1295	rBV	220	139	0.02%	0.003%
18	5.539	1303	1306	1309	rVB	223	124	0.02%	0.003%
19	5.552	1309	1310	1313	rBV	134	54	0.01%	0.001%
20	5.719	1341	1362	1392	rVB2	217276	608148	100.00%	13.394%
21	5.925	1421	1426	1428	rBV2	159	119	0.02%	0.003%
22	6.015	1452	1454	1455	rBV2	219	87	0.01%	0.002%
23	6.028	1455	1458	1460	rVV	321	210	0.03%	0.005%
24	6.057	1463	1467	1468	rBV	158	126	0.02%	0.003%
25	6.092	1476	1478	1479	rBV	123	28	0.00%	0.001%
26	6.144	1492	1494	1496	rBV	144	58	0.01%	0.001%
27	6.244	1508	1525	1544	rBV	189820	357648	58.81%	7.877%
28	6.388	1568	1570	1571	rBV	126	49	0.01%	0.001%
29	6.462	1591	1593	1599	rVB2	227	180	0.03%	0.004%
30	6.536	1610	1616	1618	rBV2	1318	1358	0.22%	0.030%
31	6.684	1648	1662	1684	rBV	141553	268984	44.23%	5.924%
32	6.797	1695	1697	1703	rBV2	399	311	0.05%	0.007%
33	6.925	1735	1737	1739	rBV	161	77	0.01%	0.002%
34	6.961	1746	1748	1751	rBV	248	184	0.03%	0.004%
35	7.047	1772	1775	1780	rBV	183	112	0.02%	0.002%
36	7.115	1794	1796	1800	rVB	142	42	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053233.D
 Acq On : 16 Mar 2023 17:52
 Operator : JC/MD
 Sample : 01930-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	7.186	1811	1818	1823	rBV2	754	1138	0.19%	0.025%
38	7.398	1880	1884	1887	rBV	245	177	0.03%	0.004%
39	7.562	1923	1935	1950	rBV	79651	138913	22.84%	3.060%
40	7.690	1971	1975	1983	rVB3	639	713	0.12%	0.016%
41	7.742	1987	1991	1994	rVB	276	187	0.03%	0.004%
42	7.790	2004	2006	2008	rBV	141	63	0.01%	0.001%
43	7.825	2016	2017	2019	rBV	138	45	0.01%	0.001%
44	7.893	2025	2038	2054	rBV	274717	466402	76.69%	10.272%
45	8.009	2071	2074	2078	rBV2	269	201	0.03%	0.004%
46	8.089	2097	2099	2104	rBV	187	92	0.02%	0.002%
47	8.173	2114	2125	2139	rBV	54234	90470	14.88%	1.993%
48	8.456	2210	2213	2217	rBV	198	98	0.02%	0.002%
49	8.571	2247	2249	2250	rBV	131	56	0.01%	0.001%
50	8.626	2255	2266	2296	rVV	140023	259834	42.73%	5.723%
51	8.954	2364	2368	2370	rBV	210	168	0.03%	0.004%
52	9.086	2407	2409	2412	rBV2	176	111	0.02%	0.002%
53	9.301	2473	2476	2485	rVB2	292	265	0.04%	0.006%
54	9.411	2498	2510	2535	rBV	264523	437432	71.93%	9.634%
55	9.565	2555	2558	2560	rBV	268	169	0.03%	0.004%
56	9.697	2597	2599	2603	rVB	333	135	0.02%	0.003%
57	9.722	2605	2607	2610	rVV	191	74	0.01%	0.002%
58	9.777	2622	2624	2626	rBV	139	79	0.01%	0.002%
59	9.954	2676	2679	2681	rBV	187	139	0.02%	0.003%
60	10.018	2696	2699	2701	rBV	208	103	0.02%	0.002%
61	10.118	2728	2730	2732	rBV	127	53	0.01%	0.001%
62	10.333	2794	2797	2799	rBV2	199	132	0.02%	0.003%
63	10.391	2813	2815	2820	rVB	164	60	0.01%	0.001%
64	10.542	2859	2862	2867	rBV2	230	210	0.03%	0.005%
65	10.681	2903	2905	2913	rVB	244	190	0.03%	0.004%
66	10.751	2913	2927	2949	rBV	183815	293195	48.21%	6.458%
67	10.996	3001	3003	3005	rBV	186	77	0.01%	0.002%
68	11.057	3019	3022	3025	rVB2	188	132	0.02%	0.003%
69	11.073	3025	3027	3028	rBV2	154	49	0.01%	0.001%
70	11.128	3041	3044	3050	rBV2	190	207	0.03%	0.005%
71	11.484	3153	3155	3157	rBV	143	61	0.01%	0.001%
72	11.681	3214	3216	3219	rBV	173	75	0.01%	0.002%
73	11.738	3231	3234	3237	rBV	194	133	0.02%	0.003%
74	11.806	3243	3255	3277	rBV	282514	446593	73.43%	9.836%
75	11.941	3293	3297	3301	rBV	212	148	0.02%	0.003%
76	12.189	3362	3374	3394	rBV	246213	395295	65.00%	8.706%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053233.D
 Acq On : 16 Mar 2023 17:52
 Operator : JC/MD
 Sample : 01930-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M

Title : VOC Analysis

77	12.314	3406	3413	3415	rBV2	649	804	0.13%	0.018%
78	12.555	3486	3488	3490	rBV	158	48	0.01%	0.001%
79	12.639	3513	3514	3516	rBV	132	34	0.01%	0.001%
80	12.655	3516	3519	3520	rBV	168	81	0.01%	0.002%
81	12.983	3619	3621	3623	rBV	192	74	0.01%	0.002%
82	13.201	3687	3689	3691	rBV	168	54	0.01%	0.001%
83	13.581	3804	3807	3809	rBV	259	153	0.03%	0.003%
84	13.629	3821	3822	3824	rBV	203	86	0.01%	0.002%
85	13.742	3854	3857	3860	rBV2	233	174	0.03%	0.004%
86	14.304	4030	4032	4034	rBV	202	80	0.01%	0.002%
87	15.565	4420	4424	4425	rBV2	392	301	0.05%	0.007%




Sum of corrected areas: 4540302

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053233.D
Acq On : 16 Mar 2023 17:52
Operator : JC/MD
Sample : 01930-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

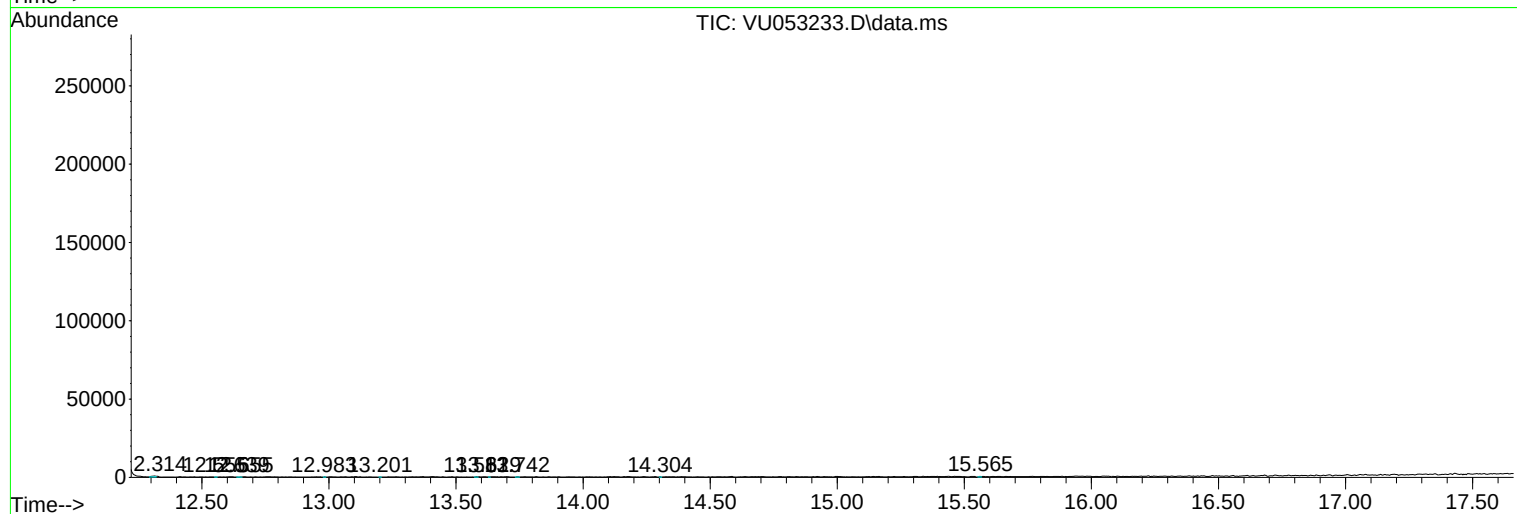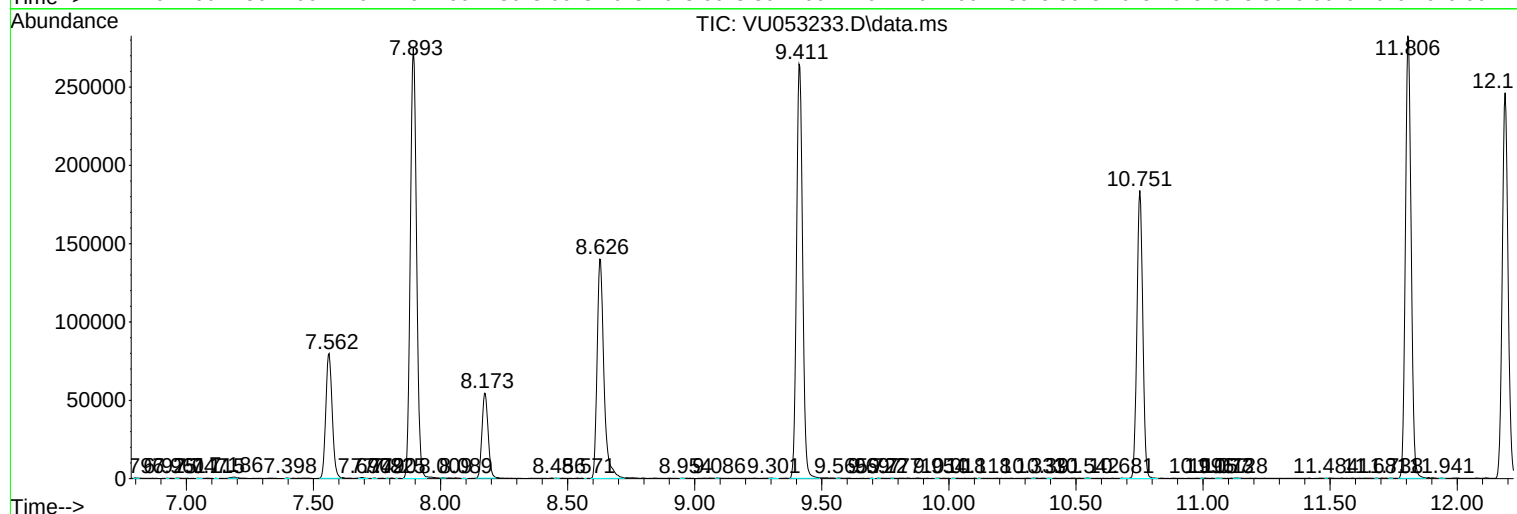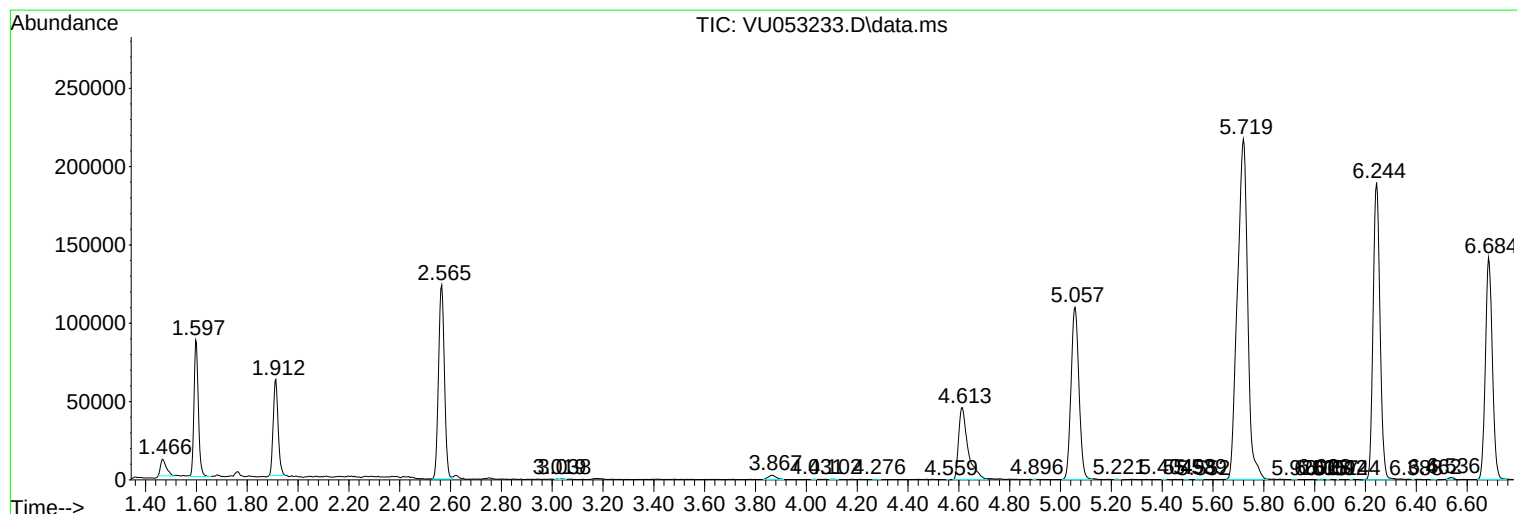

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053233.D
Acq On : 16 Mar 2023 17:52
Operator : JC/MD
Sample : 01930-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053233.D
Acq On : 16 Mar 2023 17:52
Operator : JC/MD
Sample : 01930-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc