

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053234.D
 Acq On : 16 Mar 2023 18:16
 Operator : JC/MD
 Sample : 01929-11 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053234.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rVB	80229	90881	15.51%	2.063%
2	1.912	170	178	196	rVB	61486	84242	14.38%	1.912%
3	2.565	370	381	396	rVB	122370	196287	33.50%	4.456%
4	2.996	511	515	519	rBV2	290	371	0.06%	0.008%
5	3.038	523	528	537	rVB4	893	1497	0.26%	0.034%
6	3.379	632	634	639	rVB	185	115	0.02%	0.003%
7	3.437	649	652	655	rBV2	188	144	0.02%	0.003%
8	3.556	683	689	692	rBV2	248	289	0.05%	0.007%
9	3.742	745	747	750	rVB	214	97	0.02%	0.002%
10	3.842	776	778	779	rBV	151	43	0.01%	0.001%
11	4.047	841	842	846	rBV	133	58	0.01%	0.001%
12	4.105	857	860	863	rBV	211	123	0.02%	0.003%
13	4.218	893	895	897	rBV	157	56	0.01%	0.001%
14	4.411	952	955	956	rBV	211	97	0.02%	0.002%
15	4.459	967	970	972	rBV	203	109	0.02%	0.002%
16	4.539	991	995	996	rBV	189	111	0.02%	0.003%
17	4.613	1006	1018	1045	rBV	46615	116979	19.96%	2.656%
18	4.945	1119	1121	1124	rBV	195	90	0.02%	0.002%
19	4.977	1129	1131	1137	rBV2	205	177	0.03%	0.004%
20	5.057	1141	1156	1177	rBV	109292	237270	40.49%	5.386%
21	5.276	1223	1224	1225	rBV	104	22	0.00%	0.000%
22	5.301	1230	1232	1234	rBV	198	86	0.01%	0.002%
23	5.330	1239	1241	1244	rBV	153	63	0.01%	0.001%
24	5.440	1272	1275	1277	rBV	164	84	0.01%	0.002%
25	5.514	1296	1298	1300	rBV	189	86	0.01%	0.002%
26	5.719	1342	1362	1384	rBV2	219846	585946	100.00%	13.302%
27	5.906	1417	1420	1421	rBV	183	89	0.02%	0.002%
28	5.993	1446	1447	1449	rBV	137	45	0.01%	0.001%
29	6.031	1457	1459	1461	rVB	131	54	0.01%	0.001%
30	6.128	1488	1489	1490	rVB	94	18	0.00%	0.000%
31	6.244	1510	1525	1548	rBV	184535	346647	59.16%	7.869%
32	6.488	1598	1601	1603	rBV	152	70	0.01%	0.002%
33	6.501	1603	1605	1607	rVV	159	67	0.01%	0.002%
34	6.530	1609	1614	1626	rVB7	1336	2520	0.43%	0.057%
35	6.581	1628	1630	1632	rVB	140	36	0.01%	0.001%
36	6.607	1635	1638	1640	rBV	169	94	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053234.D
 Acq On : 16 Mar 2023 18:16
 Operator : JC/MD
 Sample : 01929-11 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.684	1648	1662	1679	rBV2	138451	268599	45.84%	6.097%
38	6.771	1686	1689	1691	rVB2	237	118	0.02%	0.003%
39	6.832	1702	1708	1711	rBV2	216	240	0.04%	0.005%
40	6.870	1717	1720	1726	rVB2	203	166	0.03%	0.004%
41	6.896	1726	1728	1729	rBV2	147	64	0.01%	0.001%
42	6.999	1757	1760	1762	rBV	290	237	0.04%	0.005%
43	7.063	1777	1780	1781	rBV	263	147	0.03%	0.003%
44	7.182	1811	1817	1821	rBV2	1028	1023	0.17%	0.023%
45	7.227	1830	1831	1832	rVB2	102	20	0.00%	0.000%
46	7.253	1837	1839	1844	rVB	155	61	0.01%	0.001%
47	7.401	1883	1885	1887	rVB	268	121	0.02%	0.003%
48	7.420	1887	1891	1893	rBV	208	207	0.04%	0.005%
49	7.562	1923	1935	1952	rBV	78349	137950	23.54%	3.132%
50	7.793	2004	2007	2010	rVB	194	104	0.02%	0.002%
51	7.893	2026	2038	2057	rBV	267045	459773	78.47%	10.437%
52	8.076	2093	2095	2097	rBB	122	66	0.01%	0.001%
53	8.092	2097	2100	2103	rBV	241	224	0.04%	0.005%
54	8.173	2115	2125	2149	rVB	54458	90805	15.50%	2.061%
55	8.260	2149	2152	2156	rBV	201	191	0.03%	0.004%
56	8.295	2162	2163	2164	rBV	122	31	0.01%	0.001%
57	8.420	2199	2202	2204	rVB	166	77	0.01%	0.002%
58	8.497	2225	2226	2227	rBV	115	26	0.00%	0.001%
59	8.626	2255	2266	2299	rBV2	134590	251789	42.97%	5.716%
60	8.841	2331	2333	2338	rBV	202	155	0.03%	0.004%
61	8.970	2369	2373	2375	rBV2	215	186	0.03%	0.004%
62	9.073	2403	2405	2409	rVB2	198	120	0.02%	0.003%
63	9.095	2409	2412	2415	rBV2	237	193	0.03%	0.004%
64	9.118	2416	2419	2422	rBV2	246	180	0.03%	0.004%
65	9.157	2428	2431	2434	rBV	285	205	0.03%	0.005%
66	9.192	2441	2442	2443	rBV	114	29	0.00%	0.001%
67	9.414	2499	2511	2527	rBV	254673	422996	72.19%	9.602%
68	9.555	2552	2555	2558	rVB2	151	94	0.02%	0.002%
69	9.645	2580	2583	2585	rBV	154	88	0.02%	0.002%
70	9.732	2607	2610	2612	rBV2	219	189	0.03%	0.004%
71	9.851	2643	2647	2650	rBV2	256	239	0.04%	0.005%
72	10.517	2852	2854	2857	rVB	169	73	0.01%	0.002%
73	10.533	2857	2859	2862	rBV	207	110	0.02%	0.002%
74	10.610	2881	2883	2888	rVB2	185	140	0.02%	0.003%
75	10.700	2908	2911	2915	rVB2	266	242	0.04%	0.005%
76	10.751	2915	2927	2943	rBV	174685	282169	48.16%	6.405%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053234.D
 Acq On : 16 Mar 2023 18:16
 Operator : JC/MD
 Sample : 01929-11 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.893	2967	2971	2976	rBV	318	253	0.04%	0.006%
78	11.459	3145	3147	3150	rBV	168	66	0.01%	0.001%
79	11.806	3244	3255	3273	rBV	269339	429153	73.24%	9.742%
80	11.922	3287	3291	3298	rVB3	275	372	0.06%	0.008%
81	12.082	3340	3341	3343	rBV	136	45	0.01%	0.001%
82	12.121	3350	3353	3355	rBV	200	146	0.02%	0.003%
83	12.189	3362	3374	3395	rBV	243983	388940	66.38%	8.829%
84	12.327	3415	3417	3421	rBV	220	132	0.02%	0.003%
85	12.378	3430	3433	3434	rBV	218	134	0.02%	0.003%
86	12.751	3547	3549	3553	rVB	206	94	0.02%	0.002%
87	12.771	3553	3555	3557	rBV	215	113	0.02%	0.003%
88	13.073	3646	3649	3651	rBV2	222	164	0.03%	0.004%
89	13.552	3795	3798	3803	rBV	197	141	0.02%	0.003%
90	13.832	3882	3885	3887	rBV	323	196	0.03%	0.004%
91	14.934	4224	4228	4230	rBV	294	249	0.04%	0.006%
92	16.812	4810	4812	4816	rBV4	730	502	0.09%	0.011%


Sum of corrected areas: 4405110

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053234.D
Acq On : 16 Mar 2023 18:16
Operator : JC/MD
Sample : 01929-11 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

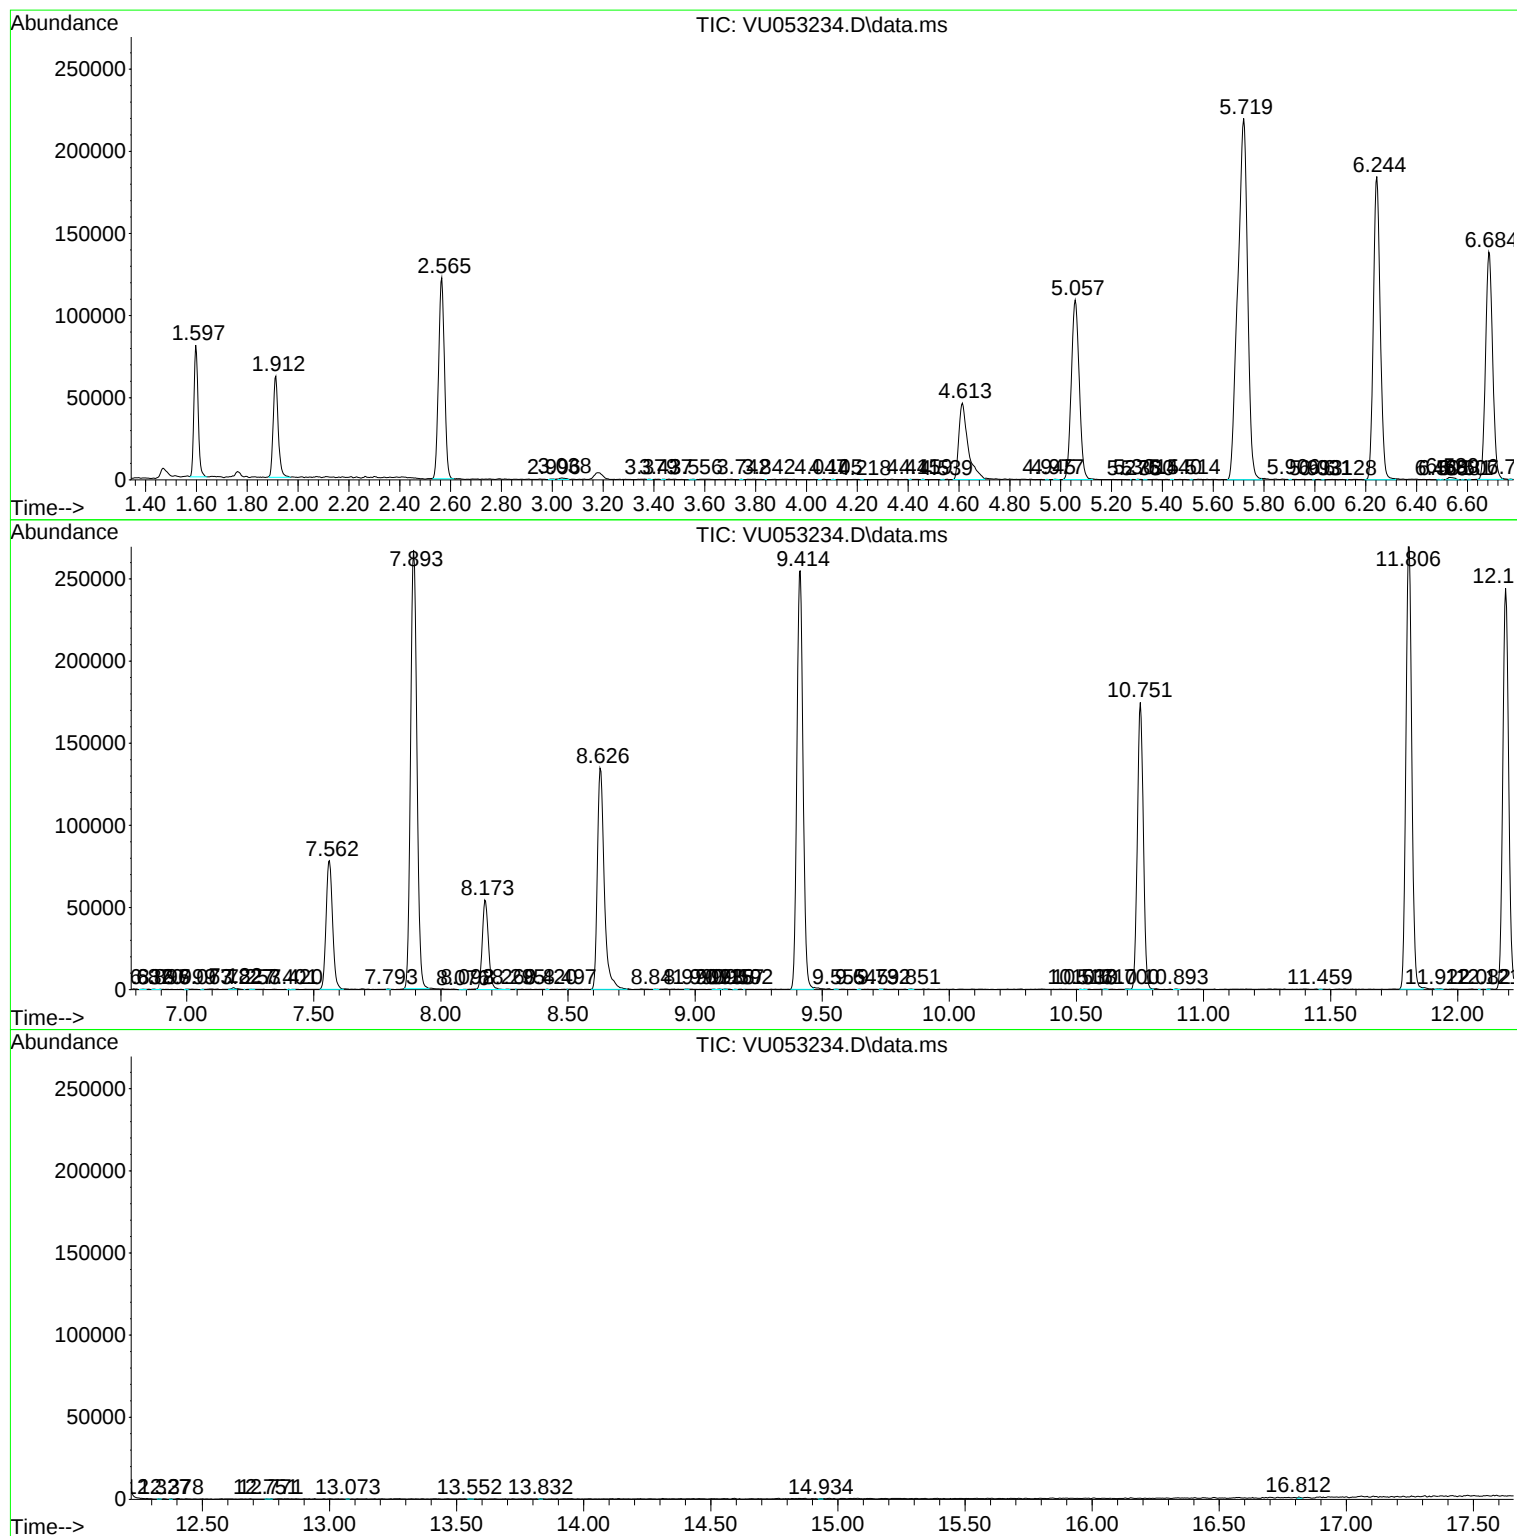

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053234.D
Acq On : 16 Mar 2023 18:16
Operator : JC/MD
Sample : 01929-11 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053234.D
Acq On : 16 Mar 2023 18:16
Operator : JC/MD
Sample : 01929-11 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------