

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053235.D
 Acq On : 16 Mar 2023 18:40
 Operator : JC/MD
 Sample : 01929-13 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053235.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rVB	77392	87440	14.73%	1.954%
2	1.909	169	177	190	rBV	62257	84352	14.21%	1.885%
3	2.565	369	381	395	rVB	124429	200163	33.72%	4.473%
4	2.993	512	514	515	rBV	188	66	0.01%	0.001%
5	3.176	561	571	586	rVB2	5162	11803	1.99%	0.264%
6	3.703	732	735	737	rBV2	227	150	0.03%	0.003%
7	3.964	813	816	818	rBV2	249	163	0.03%	0.004%
8	4.102	857	859	860	rBV2	229	100	0.02%	0.002%
9	4.128	866	867	869	rBV2	130	54	0.01%	0.001%
10	4.311	921	924	925	rBV2	197	92	0.02%	0.002%
11	4.346	932	935	939	rBV	115	104	0.02%	0.002%
12	4.411	953	955	956	rBV	110	26	0.00%	0.001%
13	4.610	1006	1017	1043	rBV	47650	115147	19.40%	2.573%
14	5.002	1137	1139	1141	rVB	201	84	0.01%	0.002%
15	5.057	1141	1156	1176	rBV2	109064	239016	40.27%	5.341%
16	5.160	1186	1188	1191	rVB	178	58	0.01%	0.001%
17	5.468	1283	1284	1285	rBV	99	21	0.00%	0.000%
18	5.613	1326	1329	1333	rBV2	201	196	0.03%	0.004%
19	5.636	1334	1336	1340	rVB	204	84	0.01%	0.002%
20	5.719	1340	1362	1387	rBV2	219304	593526	100.00%	13.263%
21	5.970	1437	1440	1444	rBV2	278	211	0.04%	0.005%
22	6.025	1454	1457	1460	rVB2	167	104	0.02%	0.002%
23	6.057	1464	1467	1469	rBV	183	138	0.02%	0.003%
24	6.086	1475	1476	1478	rVB	151	54	0.01%	0.001%
25	6.243	1512	1525	1542	rBV	185349	346653	58.41%	7.746%
26	6.372	1562	1565	1567	rBV	188	139	0.02%	0.003%
27	6.385	1567	1569	1573	rVV3	229	141	0.02%	0.003%
28	6.452	1587	1590	1592	rBV	138	108	0.02%	0.002%
29	6.472	1594	1596	1599	rVB2	156	93	0.02%	0.002%
30	6.533	1606	1615	1616	rBV2	1280	1328	0.22%	0.030%
31	6.626	1642	1644	1646	rVB	150	82	0.01%	0.002%
32	6.684	1648	1662	1685	rVV	142007	274009	46.17%	6.123%
33	6.793	1692	1696	1698	rBV3	303	228	0.04%	0.005%
34	6.857	1714	1716	1721	rVB	225	113	0.02%	0.003%
35	6.938	1737	1741	1743	rBV2	252	185	0.03%	0.004%
36	7.005	1760	1762	1764	rBV	220	107	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053235.D
 Acq On : 16 Mar 2023 18:40
 Operator : JC/MD
 Sample : 01929-13 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	7.060	1777	1779	1781	rBV	186	120	0.02%	0.003%
38	7.076	1782	1784	1786	rVB	163	82	0.01%	0.002%
39	7.137	1800	1803	1804	rBV	147	67	0.01%	0.001%
40	7.182	1811	1817	1820	rBV3	950	1060	0.18%	0.024%
41	7.256	1836	1840	1843	rBV	151	131	0.02%	0.003%
42	7.298	1850	1853	1857	rBV2	289	223	0.04%	0.005%
43	7.353	1868	1870	1871	rVB	119	44	0.01%	0.001%
44	7.404	1883	1886	1888	rBV	138	119	0.02%	0.003%
45	7.468	1901	1906	1909	rBV	234	288	0.05%	0.006%
46	7.558	1922	1934	1950	rBV	82430	142827	24.06%	3.192%
47	7.668	1964	1968	1970	rBV	222	147	0.02%	0.003%
48	7.684	1970	1973	1983	rVV3	675	920	0.16%	0.021%
49	7.742	1988	1991	1994	rVB2	190	126	0.02%	0.003%
50	7.828	2016	2018	2024	rVB2	226	202	0.03%	0.005%
51	7.893	2024	2038	2065	rBV	276436	471846	79.50%	10.544%
52	8.041	2080	2084	2087	rBV	246	203	0.03%	0.005%
53	8.092	2099	2100	2101	rBV	129	31	0.01%	0.001%
54	8.172	2115	2125	2139	rBV2	53463	90754	15.29%	2.028%
55	8.266	2151	2154	2155	rBV	209	149	0.03%	0.003%
56	8.359	2181	2183	2185	rBV2	139	75	0.01%	0.002%
57	8.436	2204	2207	2210	rBV	223	131	0.02%	0.003%
58	8.497	2224	2226	2229	rBV2	130	74	0.01%	0.002%
59	8.517	2229	2232	2233	rBV2	135	62	0.01%	0.001%
60	8.568	2246	2248	2251	rBV	181	60	0.01%	0.001%
61	8.626	2255	2266	2292	rBV2	139713	255005	42.96%	5.698%
62	8.767	2308	2310	2315	rVB2	317	247	0.04%	0.006%
63	8.931	2358	2361	2364	rBV	151	110	0.02%	0.002%
64	8.992	2378	2380	2384	rVB	204	107	0.02%	0.002%
65	9.095	2410	2412	2413	rBV	127	36	0.01%	0.001%
66	9.314	2478	2480	2481	rBV	124	33	0.01%	0.001%
67	9.336	2484	2487	2489	rVB2	188	97	0.02%	0.002%
68	9.349	2489	2491	2492	rBV2	189	79	0.01%	0.002%
69	9.410	2498	2510	2530	rBV	260604	430346	72.51%	9.616%
70	9.725	2605	2608	2613	rBV	210	149	0.03%	0.003%
71	9.790	2624	2628	2631	rBV	226	221	0.04%	0.005%
72	10.172	2744	2747	2748	rBV	167	83	0.01%	0.002%
73	10.288	2781	2783	2785	rBV	198	82	0.01%	0.002%
74	10.443	2826	2831	2834	rBV2	233	246	0.04%	0.005%
75	10.491	2843	2846	2850	rBV2	221	171	0.03%	0.004%
76	10.594	2876	2878	2879	rBV2	125	31	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053235.D
 Acq On : 16 Mar 2023 18:40
 Operator : JC/MD
 Sample : 01929-13 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.751	2915	2927	2950	rVB	178417	287907	48.51%	6.433%
78	10.832	2950	2952	2954	rVV	186	90	0.02%	0.002%
79	10.844	2954	2956	2959	rVB	256	130	0.02%	0.003%
80	10.867	2961	2963	2966	rVB2	199	114	0.02%	0.003%
81	10.883	2966	2968	2971	rBV2	187	96	0.02%	0.002%
82	10.925	2978	2981	2985	rVB	205	100	0.02%	0.002%
83	10.989	2998	3001	3004	rVB	205	113	0.02%	0.003%
84	11.307	3098	3100	3103	rBV	180	100	0.02%	0.002%
85	11.510	3160	3163	3169	rBV	227	164	0.03%	0.004%
86	11.677	3212	3215	3217	rBV	161	73	0.01%	0.002%
87	11.806	3244	3255	3276	rBV	271446	435427	73.36%	9.730%
88	12.073	3336	3338	3343	rVB2	289	185	0.03%	0.004%
89	12.188	3362	3374	3394	rBV	249025	395640	66.66%	8.841%
90	12.417	3441	3445	3447	rBV	254	225	0.04%	0.005%
91	12.468	3457	3461	3466	rBV2	260	304	0.05%	0.007%
92	12.497	3467	3470	3473	rBV	215	127	0.02%	0.003%
93	12.825	3570	3572	3578	rVB	217	134	0.02%	0.003%
94	13.307	3719	3722	3724	rBV2	154	113	0.02%	0.003%
95	13.664	3830	3833	3836	rBV	183	111	0.02%	0.002%
96	13.880	3897	3900	3902	rBV	204	128	0.02%	0.003%
97	14.179	3992	3993	3998	rBV	207	122	0.02%	0.003%
98	14.220	4002	4006	4010	rVB2	211	167	0.03%	0.004%
99	14.301	4029	4031	4034	rBV	189	80	0.01%	0.002%
100	14.343	4035	4044	4045	rBV	276	415	0.07%	0.009%




Sum of corrected areas: 4475187

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053235.D
Acq On : 16 Mar 2023 18:40
Operator : JC/MD
Sample : 01929-13 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

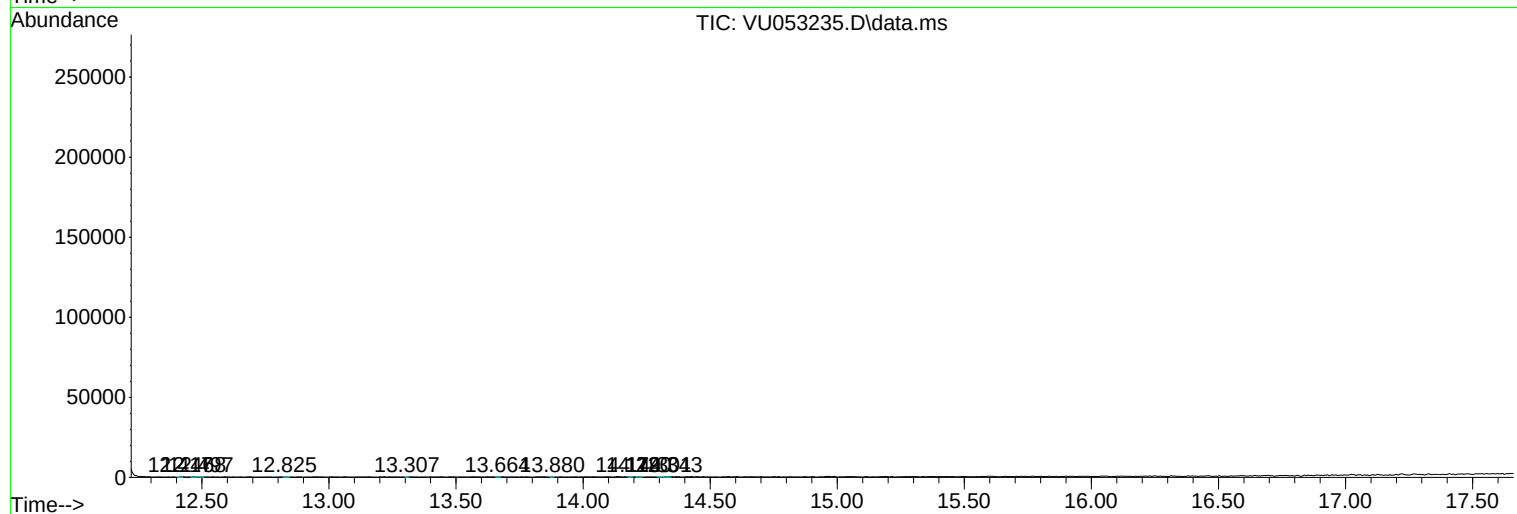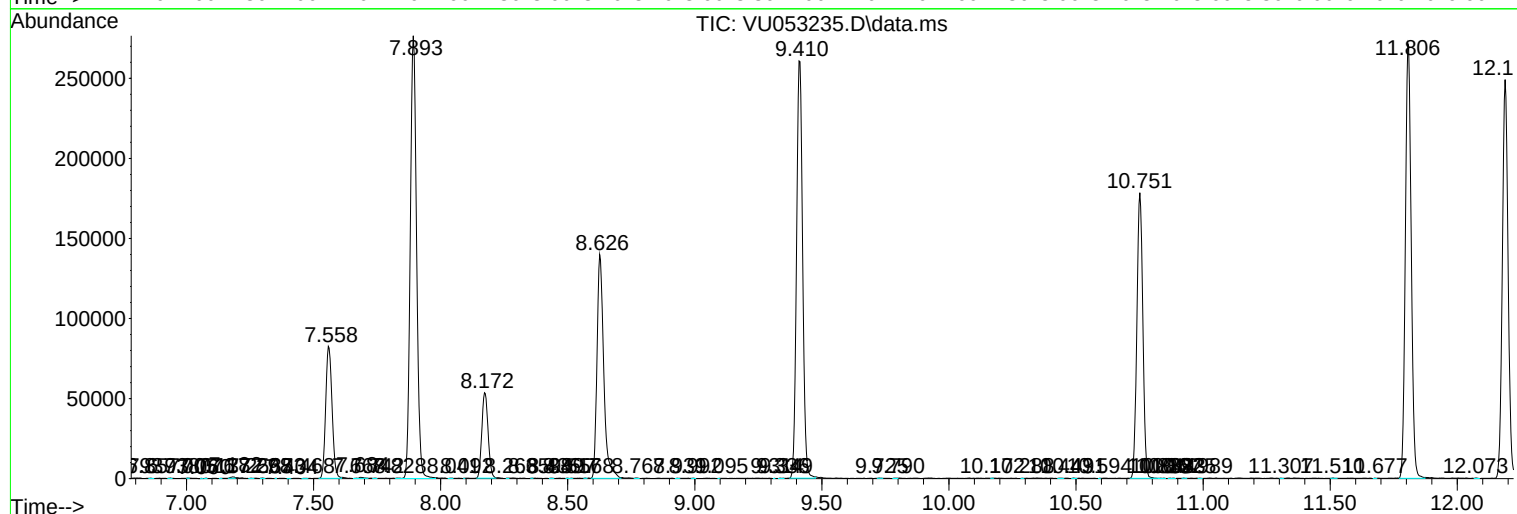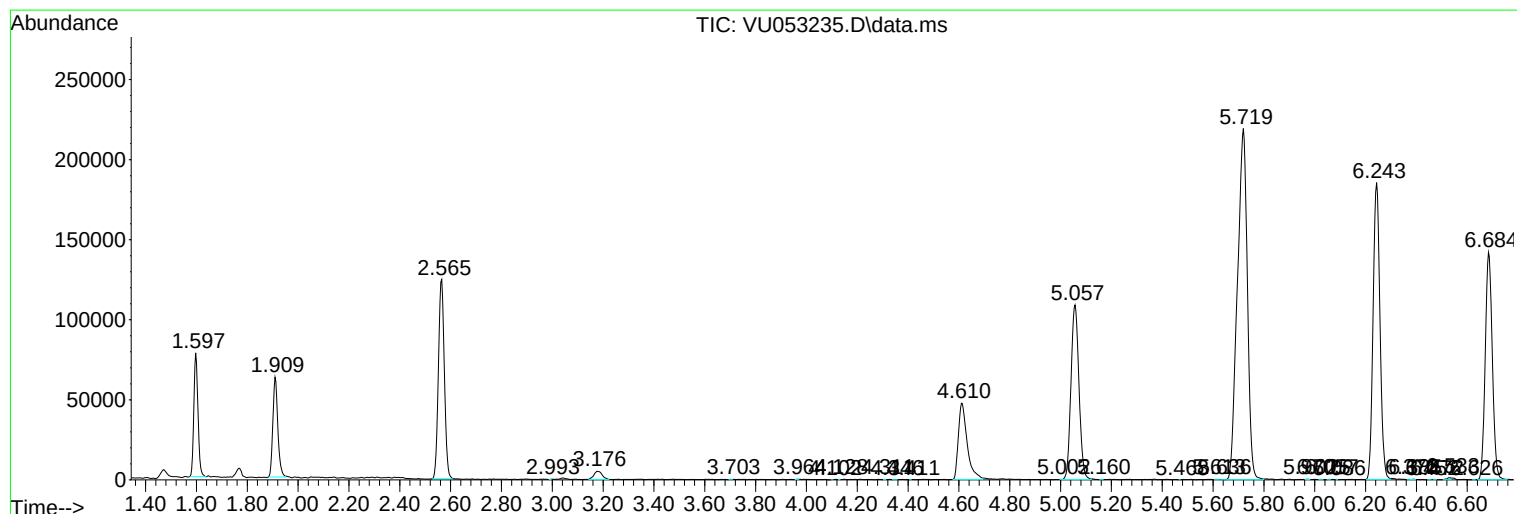

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053235.D
Acq On : 16 Mar 2023 18:40
Operator : JC/MD
Sample : 01929-13 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053235.D
Acq On : 16 Mar 2023 18:40
Operator : JC/MD
Sample : 01929-13 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc