

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053236.D
 Acq On : 16 Mar 2023 19:03
 Operator : JC/MD
 Sample : 01929-15 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053236.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	96	rVB2	95032	114048	19.37%	2.584%
2	1.909	169	177	195	rVB	60157	82570	14.03%	1.871%
3	2.565	369	381	394	rBV	120026	193841	32.93%	4.392%
4	3.038	523	528	537	rBV4	874	1201	0.20%	0.027%
5	3.125	552	555	558	rVB	253	158	0.03%	0.004%
6	3.179	560	572	587	rVV2	5451	12127	2.06%	0.275%
7	3.642	714	716	717	rBV2	153	52	0.01%	0.001%
8	3.777	755	758	760	rBV	183	148	0.03%	0.003%
9	3.809	765	768	772	rVB	234	145	0.02%	0.003%
10	3.967	814	817	820	rBV	167	88	0.01%	0.002%
11	4.083	849	853	854	rBV	150	101	0.02%	0.002%
12	4.247	899	904	907	rBV2	228	234	0.04%	0.005%
13	4.372	941	943	947	rVB	217	119	0.02%	0.003%
14	4.472	970	974	977	rBV	263	210	0.04%	0.005%
15	4.613	1006	1018	1025	rBV	46473	98239	16.69%	2.226%
16	5.057	1140	1156	1175	rBV	108816	236754	40.22%	5.364%
17	5.195	1197	1199	1202	rVB	155	48	0.01%	0.001%
18	5.285	1224	1227	1229	rBV2	404	263	0.04%	0.006%
19	5.324	1237	1239	1240	rBV	124	51	0.01%	0.001%
20	5.475	1284	1286	1288	rBV	160	77	0.01%	0.002%
21	5.536	1302	1305	1309	rBV2	241	168	0.03%	0.004%
22	5.587	1318	1321	1326	rBV	185	92	0.02%	0.002%
23	5.719	1341	1362	1388	rBV2	215510	588690	100.00%	13.337%
24	5.899	1416	1418	1419	rBV2	169	53	0.01%	0.001%
25	5.935	1427	1429	1430	rBV2	137	37	0.01%	0.001%
26	5.980	1438	1443	1445	rVB	174	144	0.02%	0.003%
27	6.025	1455	1457	1460	rBV	149	94	0.02%	0.002%
28	6.092	1475	1478	1481	rBV2	246	221	0.04%	0.005%
29	6.243	1512	1525	1551	rBV	187155	348735	59.24%	7.901%
30	6.385	1567	1569	1573	rBV2	182	123	0.02%	0.003%
31	6.491	1596	1602	1604	rBV	230	279	0.05%	0.006%
32	6.530	1610	1614	1623	rVB5	939	1471	0.25%	0.033%
33	6.594	1631	1634	1639	rVB2	216	169	0.03%	0.004%
34	6.684	1647	1662	1687	rBV	140171	270770	46.00%	6.135%
35	6.803	1698	1699	1702	rVB	290	116	0.02%	0.003%
36	6.838	1707	1710	1715	rVB	214	193	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053236.D
 Acq On : 16 Mar 2023 19:03
 Operator : JC/MD
 Sample : 01929-15 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	7.047	1773	1775	1778	rVB	195	79	0.01%	0.002%
38	7.095	1787	1790	1791	rBV	154	73	0.01%	0.002%
39	7.140	1802	1804	1808	rVB	320	178	0.03%	0.004%
40	7.192	1808	1820	1827	rBV4	754	1699	0.29%	0.038%
41	7.256	1838	1840	1841	rBV	127	30	0.01%	0.001%
42	7.269	1841	1844	1848	rVB	210	117	0.02%	0.003%
43	7.288	1848	1850	1851	rBV	143	40	0.01%	0.001%
44	7.459	1900	1903	1904	rBV	165	76	0.01%	0.002%
45	7.562	1922	1935	1956	rBV	76835	136150	23.13%	3.085%
46	7.719	1982	1984	1987	rVB2	243	98	0.02%	0.002%
47	7.739	1987	1990	1992	rBV2	174	97	0.02%	0.002%
48	7.774	1996	2001	2005	rVB2	206	195	0.03%	0.004%
49	7.803	2007	2010	2014	rVB	312	241	0.04%	0.005%
50	7.825	2014	2017	2020	rBV	219	196	0.03%	0.004%
51	7.893	2024	2038	2058	rBV	268838	460423	78.21%	10.431%
52	8.054	2085	2088	2091	rBV2	186	128	0.02%	0.003%
53	8.070	2091	2093	2098	rVB2	453	328	0.06%	0.007%
54	8.092	2098	2100	2102	rBV	390	215	0.04%	0.005%
55	8.131	2110	2112	2113	rBV	154	65	0.01%	0.001%
56	8.173	2114	2125	2142	rVV	53515	89699	15.24%	2.032%
57	8.292	2160	2162	2163	rBV2	131	71	0.01%	0.002%
58	8.484	2217	2222	2223	rBV	281	193	0.03%	0.004%
59	8.546	2239	2241	2243	rBV	129	50	0.01%	0.001%
60	8.578	2250	2251	2252	rBV	114	26	0.00%	0.001%
61	8.626	2255	2266	2291	rBV2	133543	247583	42.06%	5.609%
62	8.790	2313	2317	2318	rBV	154	95	0.02%	0.002%
63	8.944	2360	2365	2367	rBV2	249	188	0.03%	0.004%
64	9.025	2386	2390	2391	rBV	218	129	0.02%	0.003%
65	9.092	2409	2411	2416	rBB	138	71	0.01%	0.002%
66	9.118	2416	2419	2424	rBV	196	146	0.02%	0.003%
67	9.140	2424	2426	2427	rBV	110	25	0.00%	0.001%
68	9.340	2484	2488	2489	rBV	167	111	0.02%	0.003%
69	9.414	2498	2511	2533	rBV	258914	427012	72.54%	9.674%
70	9.549	2550	2553	2556	rBV	192	127	0.02%	0.003%
71	9.661	2586	2588	2590	rBV	123	69	0.01%	0.002%
72	9.819	2633	2637	2638	rBV	265	189	0.03%	0.004%
73	9.880	2655	2656	2660	rVB	291	155	0.03%	0.004%
74	9.909	2660	2665	2666	rBV	250	227	0.04%	0.005%
75	10.021	2699	2700	2702	rVB	123	47	0.01%	0.001%
76	10.089	2718	2721	2723	rBV	249	141	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053236.D
 Acq On : 16 Mar 2023 19:03
 Operator : JC/MD
 Sample : 01929-15 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.237	2765	2767	2770	rBV2	132	70	0.01%	0.002%
78	10.407	2816	2820	2824	rBV2	268	234	0.04%	0.005%
79	10.433	2826	2828	2832	rVB2	246	157	0.03%	0.004%
80	10.751	2915	2927	2947	rVB	178070	280279	47.61%	6.350%
81	10.854	2957	2959	2961	rBV2	156	90	0.02%	0.002%
82	10.899	2969	2973	2977	rBV	230	191	0.03%	0.004%
83	11.182	3059	3061	3063	rBV	168	88	0.01%	0.002%
84	11.365	3116	3118	3121	rBV	192	63	0.01%	0.001%
85	11.809	3244	3256	3278	rBV	271892	427164	72.56%	9.678%
86	12.057	3331	3333	3336	rBV2	161	91	0.02%	0.002%
87	12.188	3362	3374	3391	rBV	238014	385578	65.50%	8.736%
88	12.369	3427	3430	3431	rBV	216	112	0.02%	0.003%
89	12.809	3559	3567	3569	rBV	303	402	0.07%	0.009%
90	12.851	3578	3580	3585	rVB	172	100	0.02%	0.002%
91	12.873	3585	3587	3588	rBV	107	25	0.00%	0.001%
92	13.568	3801	3803	3805	rBV	142	40	0.01%	0.001%
93	13.680	3836	3838	3841	rBV	167	80	0.01%	0.002%
94	13.729	3850	3853	3855	rBV	203	93	0.02%	0.002%
95	14.089	3962	3965	3968	rVB	236	131	0.02%	0.003%
96	14.751	4169	4171	4172	rBV	228	75	0.01%	0.002%
97	15.131	4287	4289	4292	rBV2	348	180	0.03%	0.004%


Sum of corrected areas: 4413854

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053236.D
Acq On : 16 Mar 2023 19:03
Operator : JC/MD
Sample : 01929-15 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

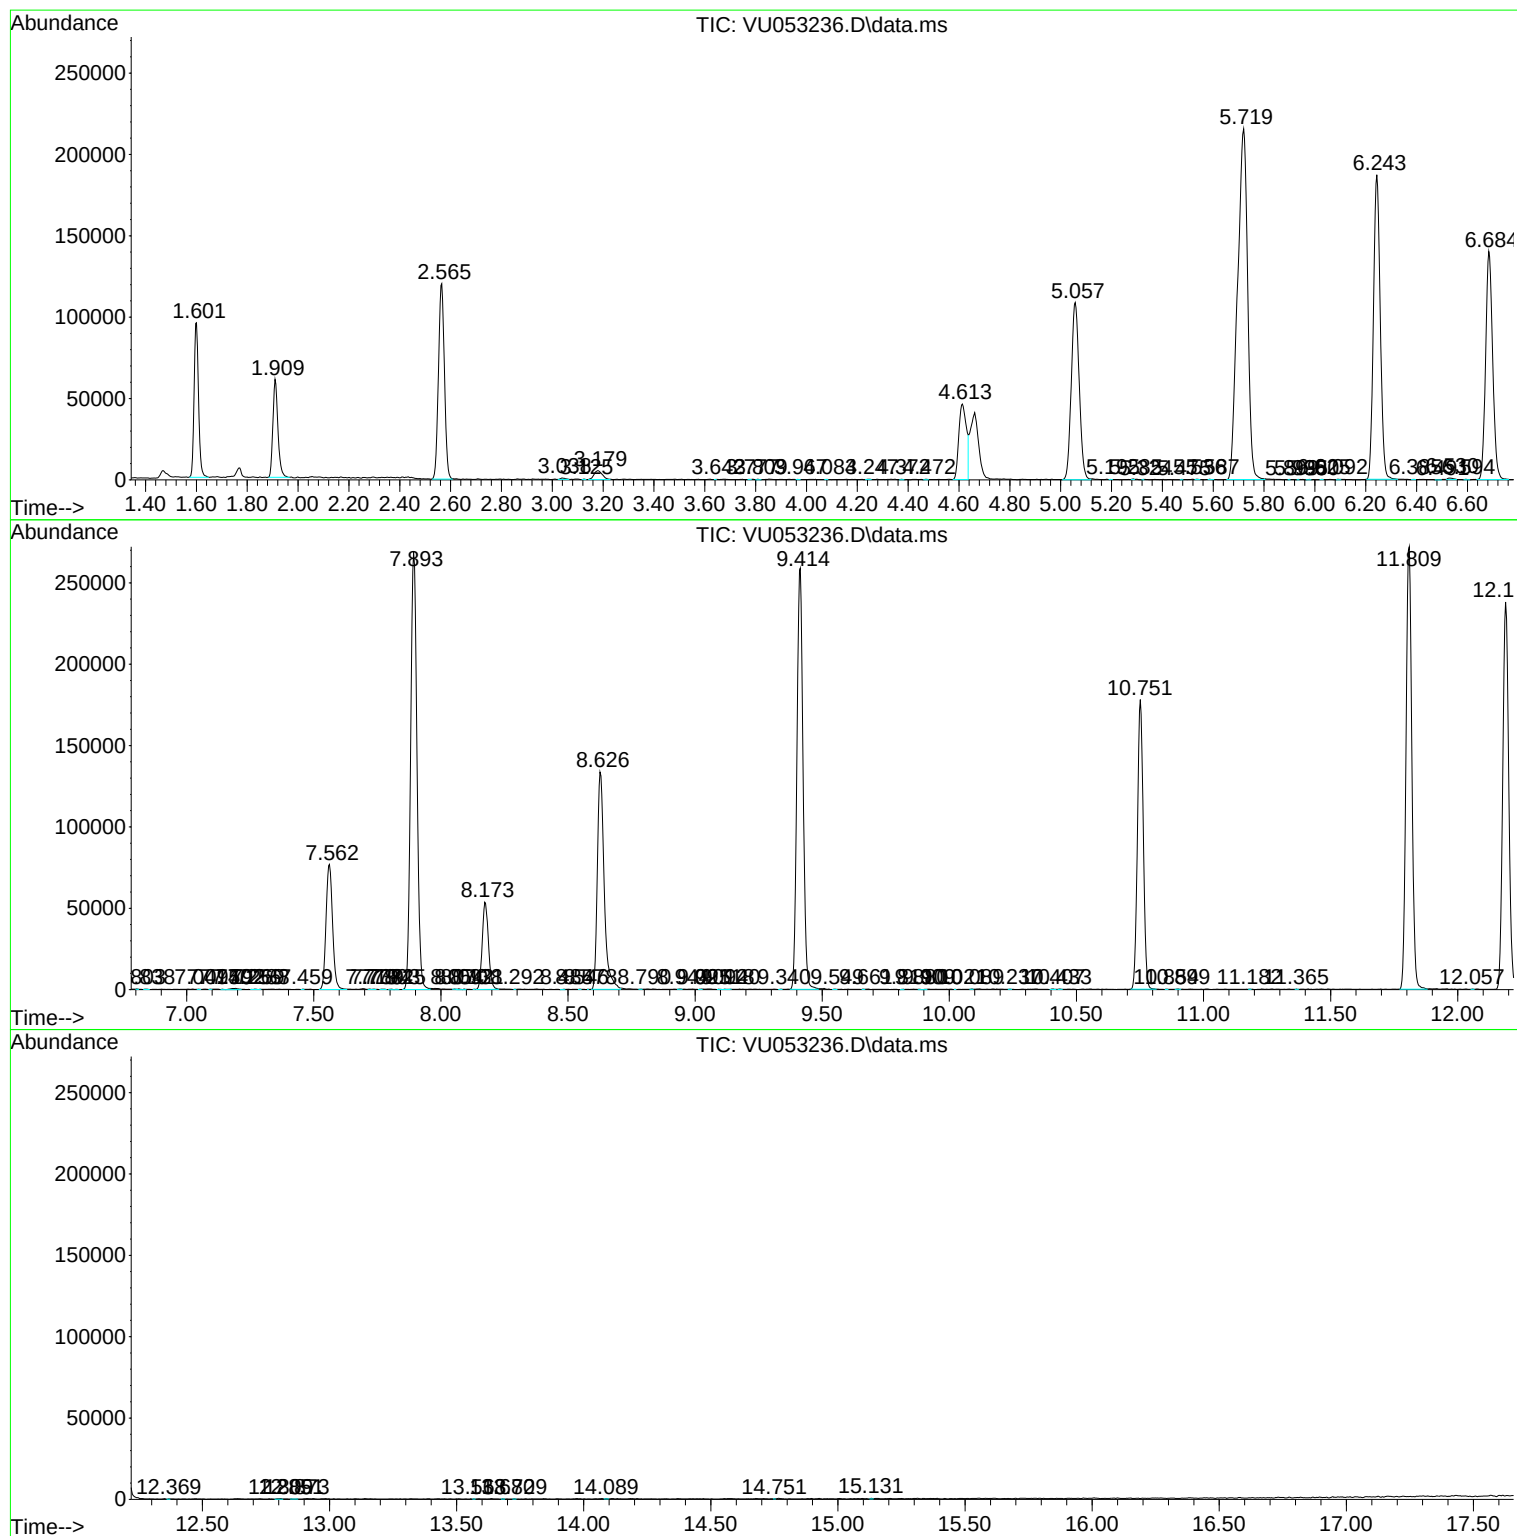

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053236.D
Acq On : 16 Mar 2023 19:03
Operator : JC/MD
Sample : 01929-15 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053236.D
Acq On : 16 Mar 2023 19:03
Operator : JC/MD
Sample : 01929-15 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------