

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053237.D
 Acq On : 16 Mar 2023 19:27
 Operator : JC/MD
 Sample : 01929-20 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053237.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	73	82	101	rVB2	303991	369492	64.44%	8.082%
2	1.912	169	178	192	rBV	59587	82655	14.41%	1.808%
3	2.565	369	381	395	rBV	119507	191071	33.32%	4.179%
4	3.041	520	529	541	rVB2	4826	9274	1.62%	0.203%
5	3.179	562	572	583	rBV	2731	5560	0.97%	0.122%
6	3.543	682	685	687	rBV	206	127	0.02%	0.003%
7	3.652	717	719	722	rBV	192	92	0.02%	0.002%
8	3.951	808	812	813	rBV	239	167	0.03%	0.004%
9	4.549	995	998	1001	rBV2	273	191	0.03%	0.004%
10	4.613	1007	1018	1021	rBV	46225	76173	13.28%	1.666%
11	4.864	1093	1096	1098	rBV	170	84	0.01%	0.002%
12	4.948	1120	1122	1125	rVB	179	76	0.01%	0.002%
13	5.057	1140	1156	1175	rBV2	106558	231314	40.34%	5.060%
14	5.189	1194	1197	1198	rBV2	144	61	0.01%	0.001%
15	5.263	1218	1220	1224	rVB	237	173	0.03%	0.004%
16	5.282	1224	1226	1228	rBV	125	60	0.01%	0.001%
17	5.314	1234	1236	1239	rVB	191	82	0.01%	0.002%
18	5.362	1248	1251	1254	rVB	216	159	0.03%	0.003%
19	5.401	1260	1263	1267	rBV2	195	150	0.03%	0.003%
20	5.443	1274	1276	1279	rBV	151	42	0.01%	0.001%
21	5.478	1285	1287	1291	rBV	197	103	0.02%	0.002%
22	5.604	1323	1326	1329	rBV2	161	118	0.02%	0.003%
23	5.645	1335	1339	1341	rBV2	258	209	0.04%	0.005%
24	5.719	1342	1362	1387	rVV2	213944	573428	100.00%	12.543%
25	5.854	1400	1404	1407	rBV2	362	298	0.05%	0.007%
26	6.038	1458	1461	1463	rBV	168	111	0.02%	0.002%
27	6.243	1512	1525	1550	rBV	179825	342388	59.71%	7.489%
28	6.443	1583	1587	1588	rBV	240	170	0.03%	0.004%
29	6.533	1608	1615	1628	rVB7	1283	2451	0.43%	0.054%
30	6.587	1628	1632	1636	rBB	198	211	0.04%	0.005%
31	6.623	1637	1643	1644	rBV2	296	330	0.06%	0.007%
32	6.684	1649	1662	1680	rBV	134176	260619	45.45%	5.701%
33	6.829	1705	1707	1710	rVB2	191	111	0.02%	0.002%
34	6.867	1716	1719	1721	rVB	237	131	0.02%	0.003%
35	6.948	1741	1744	1749	rVB2	203	126	0.02%	0.003%
36	6.993	1756	1758	1761	rVB	145	99	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053237.D
 Acq On : 16 Mar 2023 19:27
 Operator : JC/MD
 Sample : 01929-20 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	7.044	1772	1774	1779	rVB2	231	170	0.03%	0.004%
38	7.185	1811	1818	1826	rVB3	650	1009	0.18%	0.022%
39	7.227	1830	1831	1833	rVB3	232	64	0.01%	0.001%
40	7.243	1833	1836	1838	rBV2	364	317	0.06%	0.007%
41	7.333	1862	1864	1867	rVB	173	53	0.01%	0.001%
42	7.356	1867	1871	1874	rBV2	175	109	0.02%	0.002%
43	7.411	1886	1888	1893	rVB	260	152	0.03%	0.003%
44	7.436	1893	1896	1899	rBV2	204	138	0.02%	0.003%
45	7.501	1914	1916	1921	rBV	112	62	0.01%	0.001%
46	7.562	1921	1935	1951	rBV	76485	132852	23.17%	2.906%
47	7.690	1973	1975	1979	rVB	513	303	0.05%	0.007%
48	7.745	1987	1992	1995	rBV2	238	269	0.05%	0.006%
49	7.893	2025	2038	2057	rBV	261604	450292	78.53%	9.849%
50	8.050	2084	2087	2090	rBV2	165	136	0.02%	0.003%
51	8.173	2114	2125	2145	rBV	53173	89820	15.66%	1.965%
52	8.439	2205	2208	2211	rBV	193	93	0.02%	0.002%
53	8.481	2218	2221	2223	rBV	186	93	0.02%	0.002%
54	8.539	2236	2239	2240	rBV	161	81	0.01%	0.002%
55	8.626	2255	2266	2293	rBV2	133645	248074	43.26%	5.426%
56	8.925	2356	2359	2361	rBV2	197	112	0.02%	0.002%
57	8.980	2375	2376	2380	rBV	123	75	0.01%	0.002%
58	8.999	2380	2382	2386	rVV	201	119	0.02%	0.003%
59	9.079	2406	2407	2408	rBV	116	30	0.01%	0.001%
60	9.144	2426	2427	2431	rBV	146	70	0.01%	0.002%
61	9.163	2431	2433	2435	rBV	178	117	0.02%	0.003%
62	9.269	2463	2466	2469	rVB	187	93	0.02%	0.002%
63	9.314	2477	2480	2482	rBV	381	298	0.05%	0.007%
64	9.414	2498	2511	2529	rBV	252800	419631	73.18%	9.179%
65	9.571	2559	2560	2563	rVB	153	53	0.01%	0.001%
66	9.648	2581	2584	2588	rVB	241	176	0.03%	0.004%
67	9.980	2684	2687	2691	rBV	251	191	0.03%	0.004%
68	10.054	2708	2710	2712	rVB	167	68	0.01%	0.001%
69	10.095	2720	2723	2725	rBV	180	84	0.01%	0.002%
70	10.137	2735	2736	2737	rBV	130	37	0.01%	0.001%
71	10.218	2759	2761	2763	rBV2	145	73	0.01%	0.002%
72	10.272	2775	2778	2780	rBV	349	246	0.04%	0.005%
73	10.385	2810	2813	2818	rBV	133	132	0.02%	0.003%
74	10.494	2845	2847	2849	rBV	146	69	0.01%	0.002%
75	10.751	2916	2927	2940	rBV	171523	273844	47.76%	5.990%
76	11.230	3073	3076	3078	rBV	210	125	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053237.D
 Acq On : 16 Mar 2023 19:27
 Operator : JC/MD
 Sample : 01929-20 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	11.388	3121	3125	3127	rBV	232	197	0.03%	0.004%
78	11.497	3156	3159	3160	rBV2	156	89	0.02%	0.002%
79	11.536	3169	3171	3172	rBV	135	35	0.01%	0.001%
80	11.668	3209	3212	3213	rBV	180	95	0.02%	0.002%
81	11.806	3244	3255	3273	rBV	269653	422435	73.67%	9.240%
82	11.967	3302	3305	3308	rBV2	220	146	0.03%	0.003%
83	12.189	3361	3374	3396	rBV	233173	377805	65.89%	8.264%
84	12.369	3427	3430	3435	rBV2	218	241	0.04%	0.005%
85	12.439	3449	3452	3454	rBV	191	121	0.02%	0.003%
86	12.716	3537	3538	3544	rBV	138	94	0.02%	0.002%
87	13.079	3647	3651	3662	rVB2	305	322	0.06%	0.007%
88	13.160	3673	3676	3677	rBV2	133	60	0.01%	0.001%
89	13.912	3907	3910	3913	rVB	211	117	0.02%	0.003%
90	14.047	3949	3952	3955	rBV	232	156	0.03%	0.003%
91	14.124	3974	3976	3979	rVB2	347	183	0.03%	0.004%
92	14.375	4051	4054	4057	rBV	231	162	0.03%	0.004%
93	14.426	4067	4070	4072	rBV	245	155	0.03%	0.003%
94	14.764	4171	4175	4176	rBV	358	231	0.04%	0.005%
95	14.812	4187	4190	4192	rBV	256	147	0.03%	0.003%
96	14.864	4202	4206	4210	rBV2	292	285	0.05%	0.006%
97	14.999	4245	4248	4251	rBV	222	166	0.03%	0.004%
98	15.028	4255	4257	4259	rBV	209	106	0.02%	0.002%
99	15.060	4264	4267	4274	rVB3	372	419	0.07%	0.009%
100	15.484	4395	4399	4404	rBV2	353	430	0.07%	0.009%


Sum of corrected areas: 4571833

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053237.D
Acq On : 16 Mar 2023 19:27
Operator : JC/MD
Sample : 01929-20 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

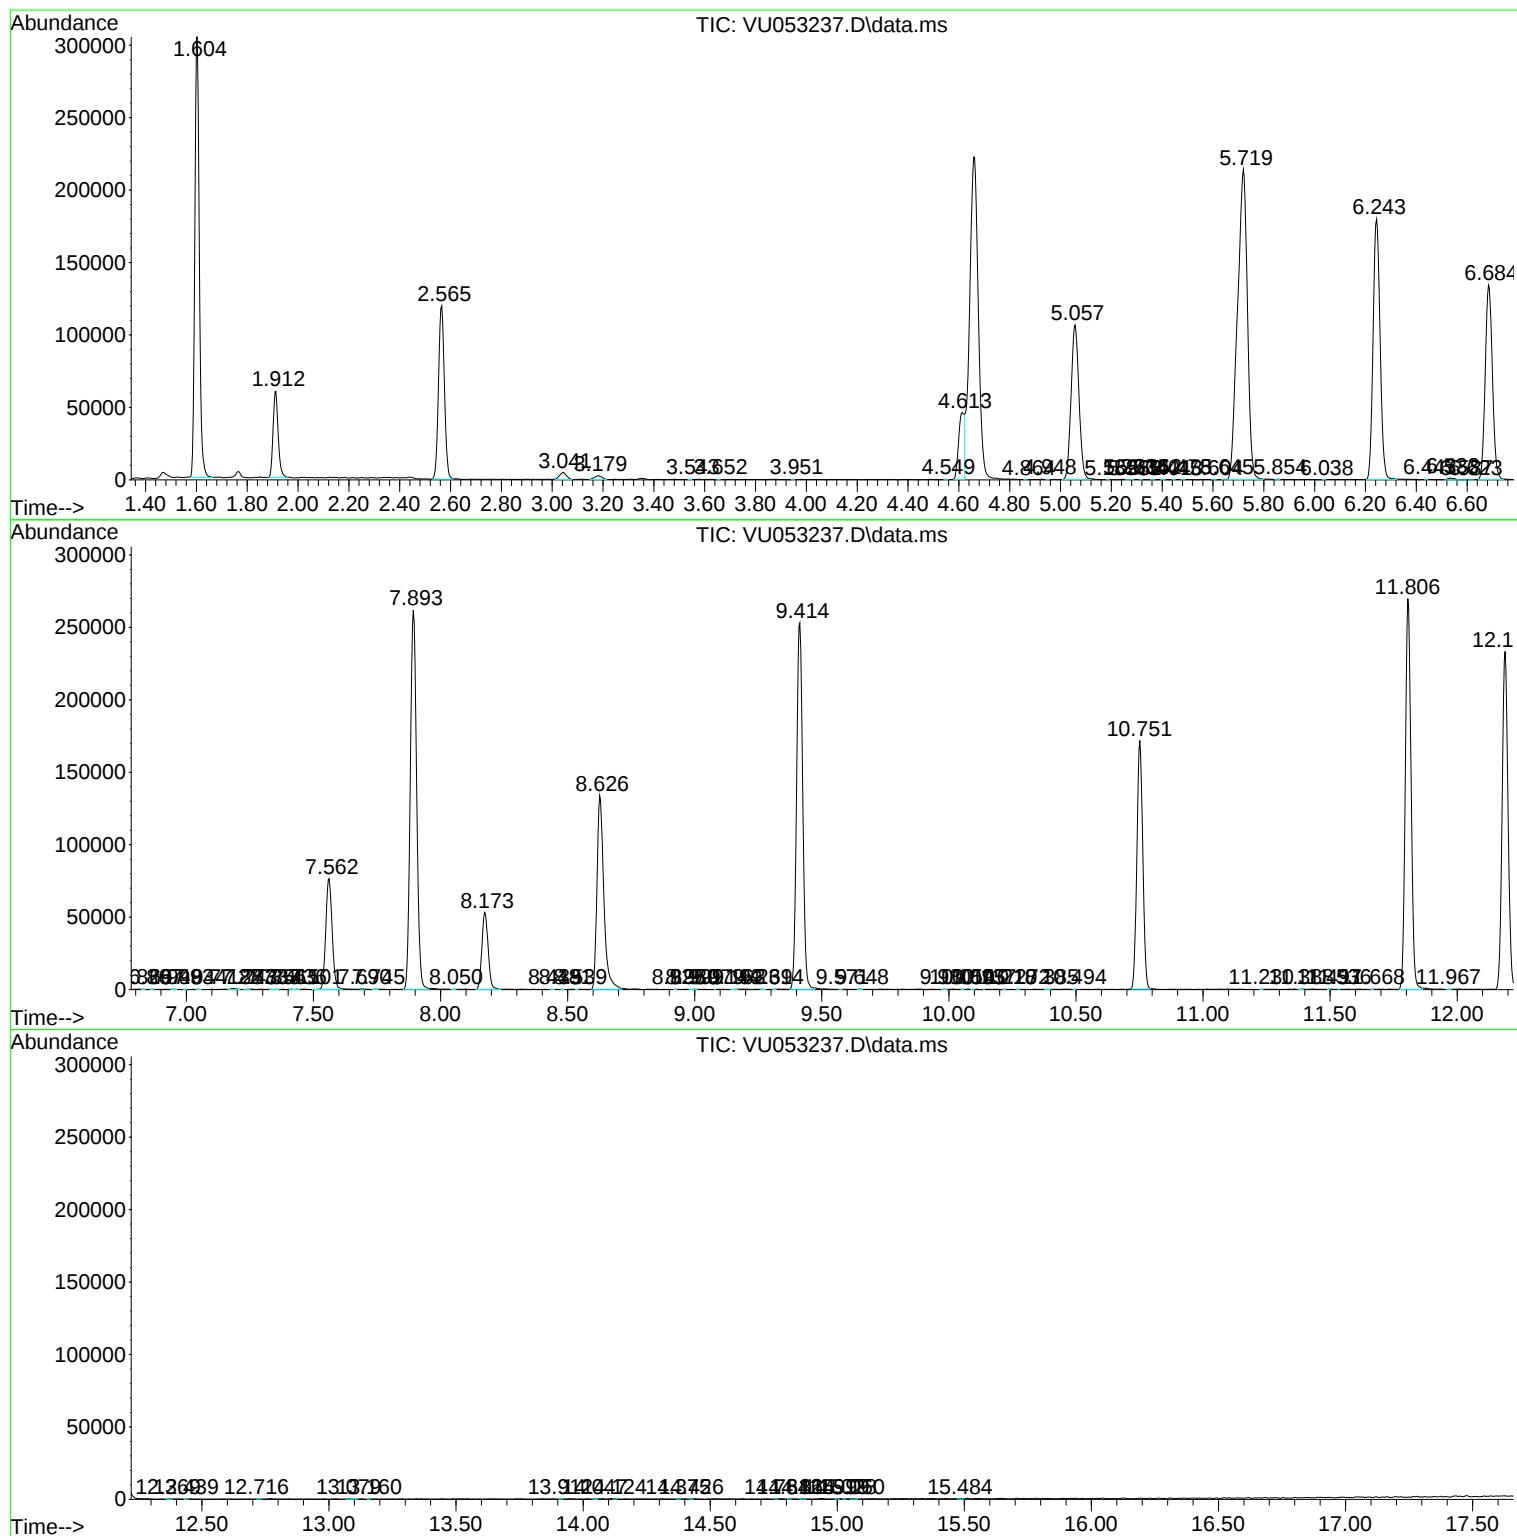

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053237.D
Acq On : 16 Mar 2023 19:27
Operator : JC/MD
Sample : 01929-20 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053237.D
Acq On : 16 Mar 2023 19:27
Operator : JC/MD
Sample : 01929-20 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------