

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053243.D
 Acq On : 16 Mar 2023 22:12
 Operator : JC/MD
 Sample : 01930-14 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFC0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053243.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.598	73	80	95	rVB	74230	83084	14.72%	1.943%
2	1.910	169	177	195	rVB	58248	82172	14.56%	1.922%
3	2.566	369	381	397	rVB	118335	191718	33.98%	4.483%
4	3.035	524	527	536	rVB3	963	1103	0.20%	0.026%
5	3.180	559	572	587	rVB	4369	10390	1.84%	0.243%
6	3.688	728	730	734	rBV	160	74	0.01%	0.002%
7	3.791	759	762	764	rBV2	287	201	0.04%	0.005%
8	3.897	793	795	800	rVB	227	130	0.02%	0.003%
9	4.524	988	990	992	rBV	169	68	0.01%	0.002%
10	4.610	1006	1017	1048	rBV	44064	106891	18.94%	2.500%
11	4.784	1070	1071	1076	rVB	324	248	0.04%	0.006%
12	4.813	1076	1080	1082	rBV2	424	351	0.06%	0.008%
13	5.057	1140	1156	1182	rBV	105543	227665	40.35%	5.324%
14	5.180	1190	1194	1197	rBV	300	309	0.05%	0.007%
15	5.247	1213	1215	1218	rVB	171	60	0.01%	0.001%
16	5.305	1229	1233	1236	rBV	204	243	0.04%	0.006%
17	5.366	1249	1252	1255	rBV2	215	156	0.03%	0.004%
18	5.443	1274	1276	1279	rBV	205	91	0.02%	0.002%
19	5.565	1312	1314	1316	rBV	165	63	0.01%	0.001%
20	5.598	1322	1324	1326	rVB	122	48	0.01%	0.001%
21	5.720	1340	1362	1388	rBV2	207445	564279	100.00%	13.196%
22	5.858	1403	1405	1407	rBV	179	104	0.02%	0.002%
23	5.874	1407	1410	1413	rVB2	201	122	0.02%	0.003%
24	5.893	1414	1416	1418	rBV	270	120	0.02%	0.003%
25	5.977	1440	1442	1443	rBV	229	108	0.02%	0.003%
26	6.022	1454	1456	1459	rBV	206	86	0.02%	0.002%
27	6.115	1482	1485	1488	rVB	162	71	0.01%	0.002%
28	6.128	1488	1489	1493	rBV	134	54	0.01%	0.001%
29	6.244	1511	1525	1547	rBV	182152	341217	60.47%	7.980%
30	6.401	1571	1574	1578	rBV	286	252	0.04%	0.006%
31	6.482	1597	1599	1603	rVB	339	219	0.04%	0.005%
32	6.507	1604	1607	1608	rBV	351	199	0.04%	0.005%
33	6.533	1608	1615	1623	rVB5	761	1246	0.22%	0.029%
34	6.581	1628	1630	1631	rBV5	149	66	0.01%	0.002%
35	6.639	1644	1648	1649	rBV	166	99	0.02%	0.002%
36	6.684	1649	1662	1680	rVV	134037	258814	45.87%	6.052%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053243.D
 Acq On : 16 Mar 2023 22:12
 Operator : JC/MD
 Sample : 01930-14 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFC0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.826	1703	1706	1709	rVB	206	107	0.02%	0.003%
38	6.938	1739	1741	1742	rBV	162	74	0.01%	0.002%
39	7.003	1757	1761	1763	rBV	188	155	0.03%	0.004%
40	7.112	1793	1795	1797	rBV	154	87	0.02%	0.002%
41	7.179	1812	1816	1819	rBV3	667	637	0.11%	0.015%
42	7.331	1859	1863	1869	rBV2	357	429	0.08%	0.010%
43	7.388	1878	1881	1884	rVB	246	125	0.02%	0.003%
44	7.462	1901	1904	1906	rBV	196	165	0.03%	0.004%
45	7.559	1919	1934	1953	rBV	75083	131220	23.25%	3.069%
46	7.694	1969	1976	1979	rBV2	635	723	0.13%	0.017%
47	7.794	2003	2007	2008	rBV	226	147	0.03%	0.003%
48	7.893	2025	2038	2055	rBV	260681	446198	79.07%	10.435%
49	8.051	2084	2087	2092	rVB2	191	137	0.02%	0.003%
50	8.077	2092	2095	2096	rBV2	200	97	0.02%	0.002%
51	8.115	2104	2107	2109	rVB2	253	168	0.03%	0.004%
52	8.134	2110	2113	2115	rBV	148	120	0.02%	0.003%
53	8.173	2115	2125	2140	rBV	52120	86316	15.30%	2.019%
54	8.282	2157	2159	2161	rVB	143	57	0.01%	0.001%
55	8.314	2167	2169	2170	rBV	123	54	0.01%	0.001%
56	8.356	2178	2182	2189	rBV2	224	312	0.06%	0.007%
57	8.491	2221	2224	2226	rBV2	147	94	0.02%	0.002%
58	8.562	2243	2246	2250	rVB2	323	264	0.05%	0.006%
59	8.585	2250	2253	2255	rBV	310	209	0.04%	0.005%
60	8.626	2255	2266	2295	rVV2	130034	239261	42.40%	5.595%
61	8.919	2355	2357	2360	rVB	183	87	0.02%	0.002%
62	9.012	2383	2386	2387	rBV	173	120	0.02%	0.003%
63	9.080	2404	2407	2409	rBV	156	71	0.01%	0.002%
64	9.295	2472	2474	2477	rVB	230	97	0.02%	0.002%
65	9.350	2487	2491	2496	rBV	211	283	0.05%	0.007%
66	9.411	2497	2510	2536	rVV	256592	417162	73.93%	9.756%
67	9.578	2554	2562	2565	rVB2	345	438	0.08%	0.010%
68	9.610	2569	2572	2575	rVV	164	93	0.02%	0.002%
69	9.938	2672	2674	2677	rBV	145	85	0.02%	0.002%
70	10.022	2698	2700	2703	rBV	154	55	0.01%	0.001%
71	10.048	2706	2708	2711	rBV	164	67	0.01%	0.002%
72	10.244	2767	2769	2771	rBV	127	59	0.01%	0.001%
73	10.302	2786	2787	2791	rBV	131	70	0.01%	0.002%
74	10.568	2867	2870	2871	rBV	166	73	0.01%	0.002%
75	10.665	2897	2900	2902	rBV	254	163	0.03%	0.004%
76	10.752	2915	2927	2943	rBV	172149	272739	48.33%	6.378%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053243.D
 Acq On : 16 Mar 2023 22:12
 Operator : JC/MD
 Sample : 01930-14 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFC0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.842	2953	2955	2957	rVB	149	59	0.01%	0.001%
78	11.057	3020	3022	3026	rBV	205	117	0.02%	0.003%
79	11.089	3026	3032	3036	rVB2	609	647	0.11%	0.015%
80	11.289	3091	3094	3097	rBV2	239	198	0.04%	0.005%
81	11.465	3144	3149	3156	rVB2	506	684	0.12%	0.016%
82	11.523	3164	3167	3171	rBV	156	145	0.03%	0.003%
83	11.739	3231	3234	3242	rBV4	473	489	0.09%	0.011%
84	11.806	3243	3255	3277	rBV	271826	422752	74.92%	9.886%
85	12.144	3357	3360	3361	rBV	145	82	0.01%	0.002%
86	12.189	3362	3374	3392	rVV	234509	376447	66.71%	8.803%
87	12.279	3400	3402	3409	rVB2	383	320	0.06%	0.007%
88	12.555	3486	3488	3490	rBV	224	81	0.01%	0.002%
89	13.002	3624	3627	3628	rBV	134	54	0.01%	0.001%
90	13.350	3732	3735	3739	rBV	296	282	0.05%	0.007%
91	13.530	3789	3791	3798	rVB	219	156	0.03%	0.004%
92	13.639	3821	3825	3829	rBV2	273	206	0.04%	0.005%
93	13.845	3884	3889	3899	rVB3	1199	1220	0.22%	0.029%
94	14.359	4047	4049	4056	rVB	269	157	0.03%	0.004%
95	14.414	4063	4066	4072	rBV	276	260	0.05%	0.006%
96	14.777	4177	4179	4181	rVB	226	74	0.01%	0.002%
97	15.121	4284	4286	4290	rVB2	303	139	0.02%	0.003%
98	15.198	4307	4310	4312	rBV	290	185	0.03%	0.004%
99	15.533	4411	4414	4420	rVB2	353	345	0.06%	0.008%
100	15.559	4420	4422	4424	rBV	253	114	0.02%	0.003%




Sum of corrected areas: 4276152

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053243.D
Acq On : 16 Mar 2023 22:12
Operator : JC/MD
Sample : 01930-14 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

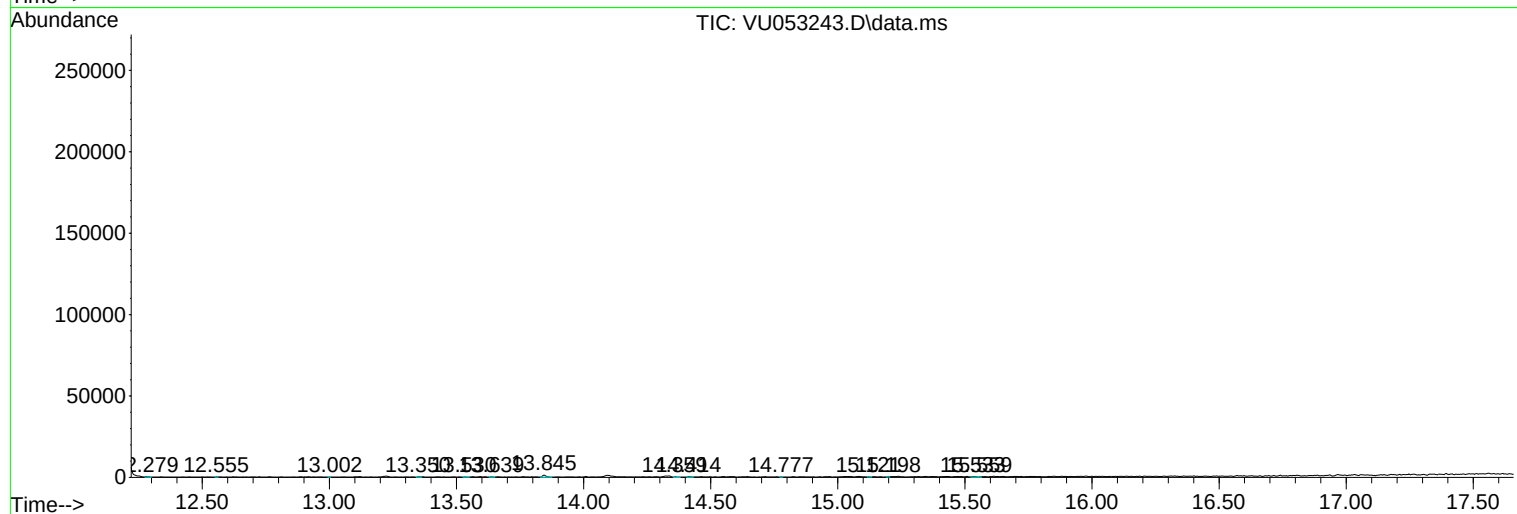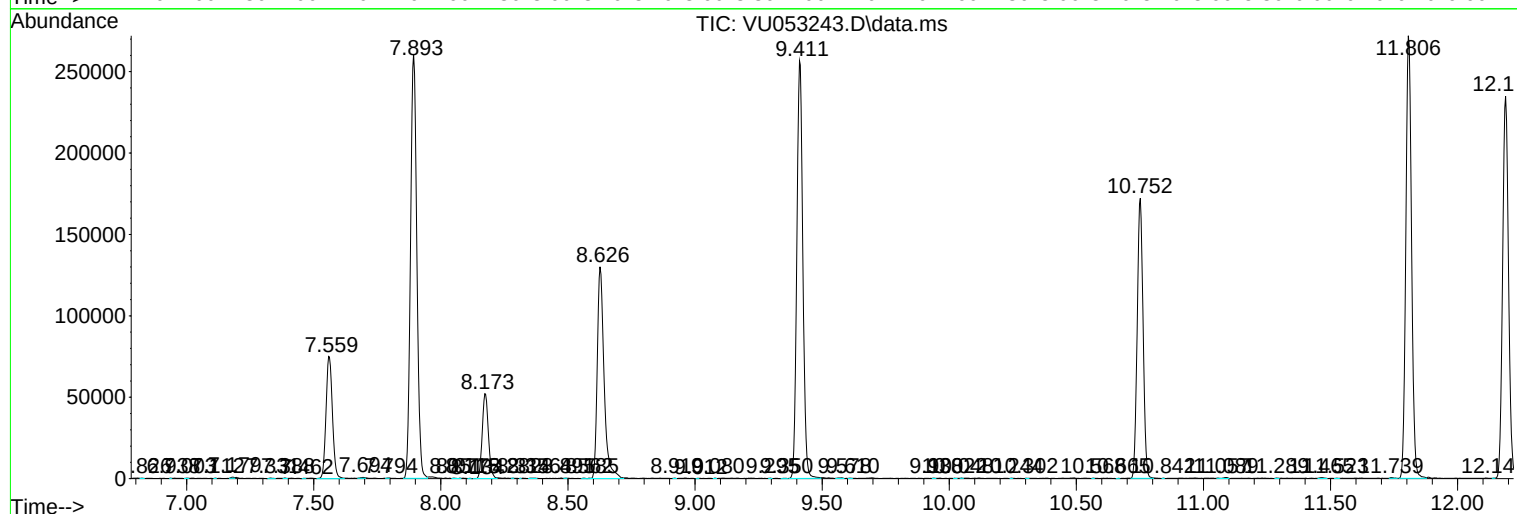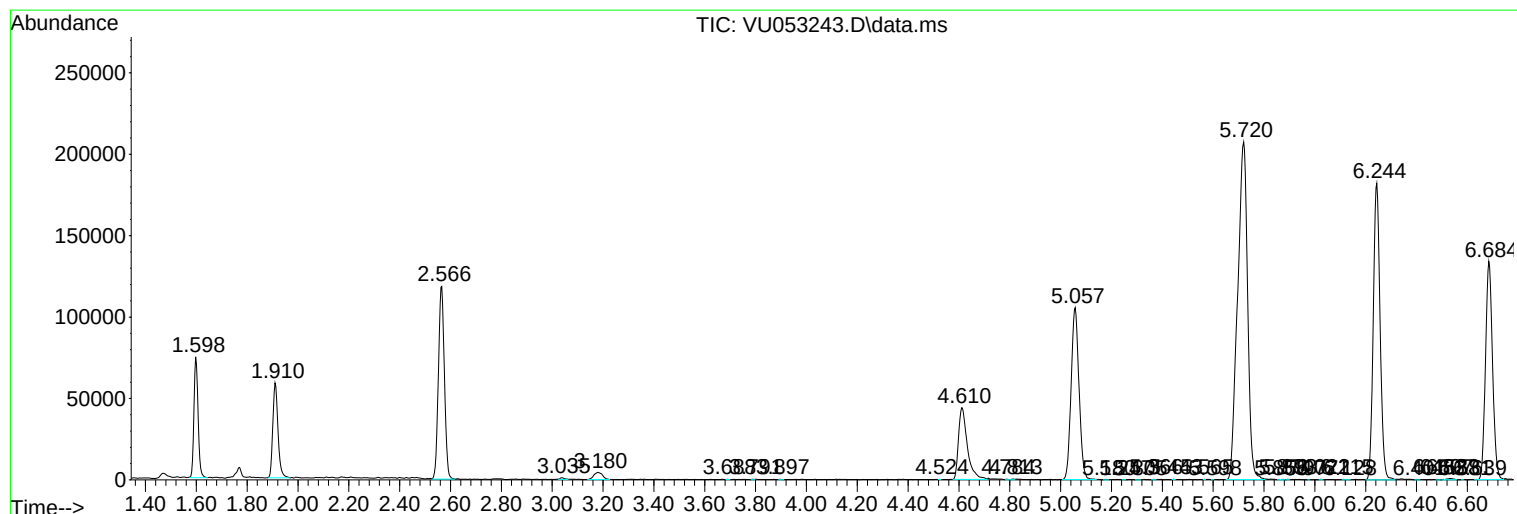

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053243.D
Acq On : 16 Mar 2023 22:12
Operator : JC/MD
Sample : 01930-14 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053243.D
Acq On : 16 Mar 2023 22:12
Operator : JC/MD
Sample : 01930-14 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------