

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053244.D
 Acq On : 16 Mar 2023 22:35
 Operator : JC/MD
 Sample : 01930-15 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFC1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053244.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB	72633	82031	14.73%	1.933%
2	1.909	169	177	194	rVB	58753	81317	14.61%	1.916%
3	2.565	369	381	397	rVB	114875	186850	33.56%	4.403%
4	2.999	512	516	517	rBV2	286	208	0.04%	0.005%
5	3.176	560	571	589	rVB	3463	7159	1.29%	0.169%
6	3.350	622	625	634	rVB2	251	272	0.05%	0.006%
7	3.556	686	689	690	rBV	194	116	0.02%	0.003%
8	3.591	696	700	701	rBV2	268	177	0.03%	0.004%
9	3.768	752	755	758	rBV	184	109	0.02%	0.003%
10	4.051	841	843	847	rVB	128	85	0.02%	0.002%
11	4.115	860	863	867	rBV2	210	185	0.03%	0.004%
12	4.298	918	920	924	rVB	187	71	0.01%	0.002%
13	4.446	965	966	968	rVB	122	47	0.01%	0.001%
14	4.613	1006	1018	1041	rBV	45105	107626	19.33%	2.536%
15	4.912	1107	1111	1114	rVB	279	169	0.03%	0.004%
16	4.935	1115	1118	1122	rVV	259	177	0.03%	0.004%
17	5.057	1140	1156	1176	rBV2	102578	226452	40.67%	5.337%
18	5.301	1230	1232	1234	rBV	163	112	0.02%	0.003%
19	5.433	1266	1273	1278	rBV	211	385	0.07%	0.009%
20	5.546	1302	1308	1312	rBV2	368	548	0.10%	0.013%
21	5.591	1314	1322	1328	rBV	390	716	0.13%	0.017%
22	5.719	1342	1362	1388	rBV2	203110	556774	100.00%	13.121%
23	5.903	1416	1419	1423	rVB	241	168	0.03%	0.004%
24	5.941	1429	1431	1432	rBV	155	83	0.01%	0.002%
25	5.967	1437	1439	1442	rVB2	235	145	0.03%	0.003%
26	5.983	1442	1444	1445	rBV	125	53	0.01%	0.001%
27	6.044	1460	1463	1466	rVB2	236	147	0.03%	0.003%
28	6.086	1474	1476	1479	rBV2	209	126	0.02%	0.003%
29	6.244	1512	1525	1543	rBV	180572	337362	60.59%	7.950%
30	6.398	1570	1573	1576	rBV	204	109	0.02%	0.003%
31	6.526	1606	1613	1615	rBV	690	651	0.12%	0.015%
32	6.584	1628	1631	1632	rBV	282	148	0.03%	0.003%
33	6.633	1643	1646	1647	rBV	133	83	0.01%	0.002%
34	6.684	1649	1662	1683	rVV	132764	255484	45.89%	6.021%
35	6.809	1695	1701	1704	rBV2	326	384	0.07%	0.009%
36	6.851	1711	1714	1716	rBV	186	122	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053244.D
 Acq On : 16 Mar 2023 22:35
 Operator : JC/MD
 Sample : 01930-15 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFC1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	7.006	1760	1762	1764	rVB	146	75	0.01%	0.002%
38	7.099	1788	1791	1794	rVB2	187	116	0.02%	0.003%
39	7.182	1811	1817	1825	rBV4	765	1180	0.21%	0.028%
40	7.250	1834	1838	1841	rBV	175	201	0.04%	0.005%
41	7.388	1875	1881	1883	rBV	190	234	0.04%	0.006%
42	7.456	1896	1902	1905	rBV2	226	285	0.05%	0.007%
43	7.498	1912	1915	1916	rBV	148	103	0.02%	0.002%
44	7.562	1923	1935	1948	rBV	75175	128711	23.12%	3.033%
45	7.642	1958	1960	1964	rBV2	263	150	0.03%	0.004%
46	7.681	1969	1972	1973	rBV	364	156	0.03%	0.004%
47	7.729	1985	1987	1991	rVB	164	86	0.02%	0.002%
48	7.800	2007	2009	2015	rVB	342	309	0.06%	0.007%
49	7.825	2015	2017	2019	rBV	156	109	0.02%	0.003%
50	7.893	2025	2038	2060	rBV	259590	443389	79.64%	10.449%
51	8.002	2069	2072	2073	rBV	249	112	0.02%	0.003%
52	8.057	2087	2089	2090	rBV	118	51	0.01%	0.001%
53	8.076	2094	2095	2097	rVB	175	61	0.01%	0.001%
54	8.176	2113	2126	2147	rBV	50534	85332	15.33%	2.011%
55	8.424	2201	2203	2206	rBV	166	79	0.01%	0.002%
56	8.475	2217	2219	2223	rVB2	161	100	0.02%	0.002%
57	8.536	2235	2238	2244	rBV	193	284	0.05%	0.007%
58	8.565	2244	2247	2251	rVB2	397	347	0.06%	0.008%
59	8.626	2255	2266	2296	rVV2	130678	240633	43.22%	5.671%
60	9.076	2403	2406	2409	rVB2	226	129	0.02%	0.003%
61	9.247	2456	2459	2460	rBV2	149	68	0.01%	0.002%
62	9.353	2489	2492	2495	rBV	167	93	0.02%	0.002%
63	9.414	2498	2511	2531	rVV	255187	416892	74.88%	9.825%
64	9.645	2578	2583	2588	rVB2	238	253	0.05%	0.006%
65	9.700	2597	2600	2604	rBV2	175	114	0.02%	0.003%
66	9.758	2615	2618	2620	rVB	238	122	0.02%	0.003%
67	9.800	2628	2631	2636	rBV	183	108	0.02%	0.003%
68	10.060	2709	2712	2715	rVB	203	119	0.02%	0.003%
69	10.092	2720	2722	2724	rBV	170	72	0.01%	0.002%
70	10.182	2747	2750	2753	rBV2	154	109	0.02%	0.003%
71	10.301	2781	2787	2791	rVB	338	427	0.08%	0.010%
72	10.327	2791	2795	2799	rBV	346	348	0.06%	0.008%
73	10.456	2833	2835	2838	rVB	163	71	0.01%	0.002%
74	10.478	2839	2842	2846	rBV2	315	321	0.06%	0.008%
75	10.626	2886	2888	2891	rVB	249	115	0.02%	0.003%
76	10.642	2891	2893	2894	rBV	143	69	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053244.D
 Acq On : 16 Mar 2023 22:35
 Operator : JC/MD
 Sample : 01930-15 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFC1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.703	2910	2912	2915	rVB	213	95	0.02%	0.002%
78	10.751	2915	2927	2944	rBV	173872	273814	49.18%	6.453%
79	10.964	2991	2993	2999	rVB2	207	163	0.03%	0.004%
80	11.083	3028	3030	3035	rBV2	316	268	0.05%	0.006%
81	11.372	3118	3120	3122	rVB	179	72	0.01%	0.002%
82	11.623	3196	3198	3200	rVB	175	71	0.01%	0.002%
83	11.652	3205	3207	3210	rBV	186	108	0.02%	0.003%
84	11.806	3243	3255	3274	rBV	265089	424757	76.29%	10.010%
85	12.189	3361	3374	3398	rBV	228154	373142	67.02%	8.794%
86	12.282	3401	3403	3406	rBV	185	95	0.02%	0.002%
87	12.298	3406	3408	3409	rVB	211	63	0.01%	0.001%
88	12.867	3583	3585	3587	rBV	182	85	0.02%	0.002%
89	13.156	3670	3675	3678	rBV2	225	287	0.05%	0.007%
90	13.224	3692	3696	3700	rVB3	443	423	0.08%	0.010%
91	13.356	3733	3737	3740	rBV2	164	111	0.02%	0.003%
92	13.372	3740	3742	3743	rBV2	139	39	0.01%	0.001%
93	13.513	3784	3786	3789	rBV2	212	138	0.02%	0.003%
94	13.594	3808	3811	3813	rBV	193	98	0.02%	0.002%
95	14.089	3959	3965	3966	rBV2	509	461	0.08%	0.011%
96	14.279	4022	4024	4026	rBV	167	53	0.01%	0.001%
97	14.844	4198	4200	4205	rVB	346	186	0.03%	0.004%
98	14.996	4245	4247	4252	rVB	313	189	0.03%	0.004%
99	15.295	4337	4340	4344	rBV2	291	253	0.05%	0.006%
100	15.533	4411	4414	4416	rBV2	245	172	0.03%	0.004%




Sum of corrected areas: 4243327

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053244.D
Acq On : 16 Mar 2023 22:35
Operator : JC/MD
Sample : 01930-15 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

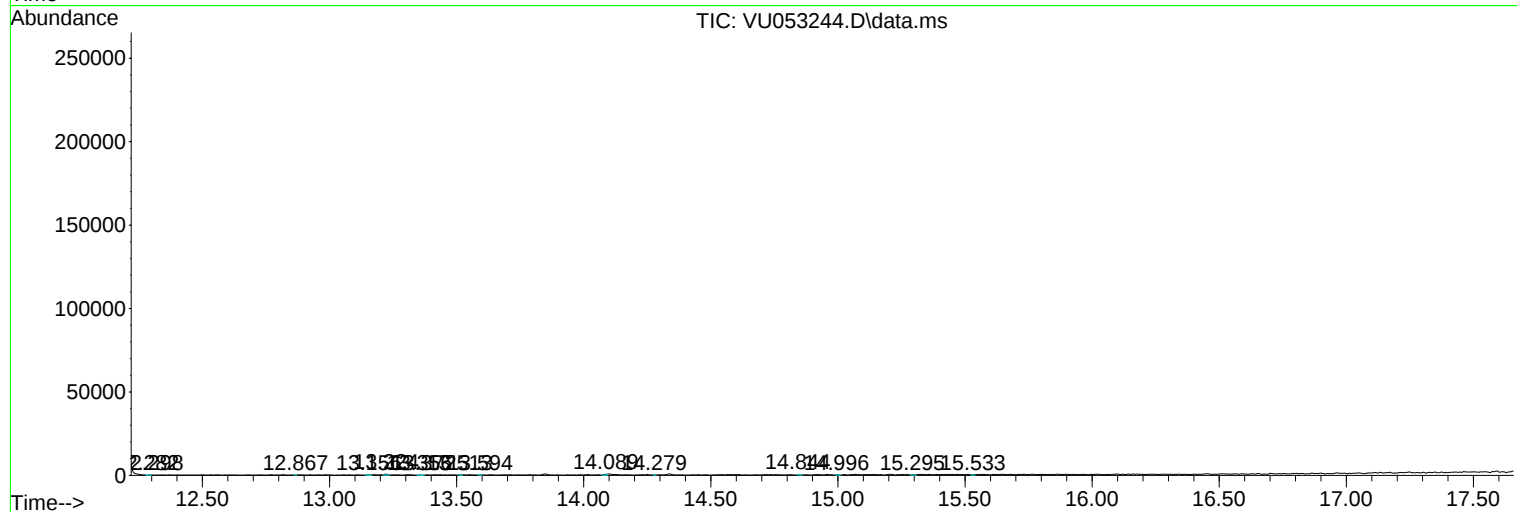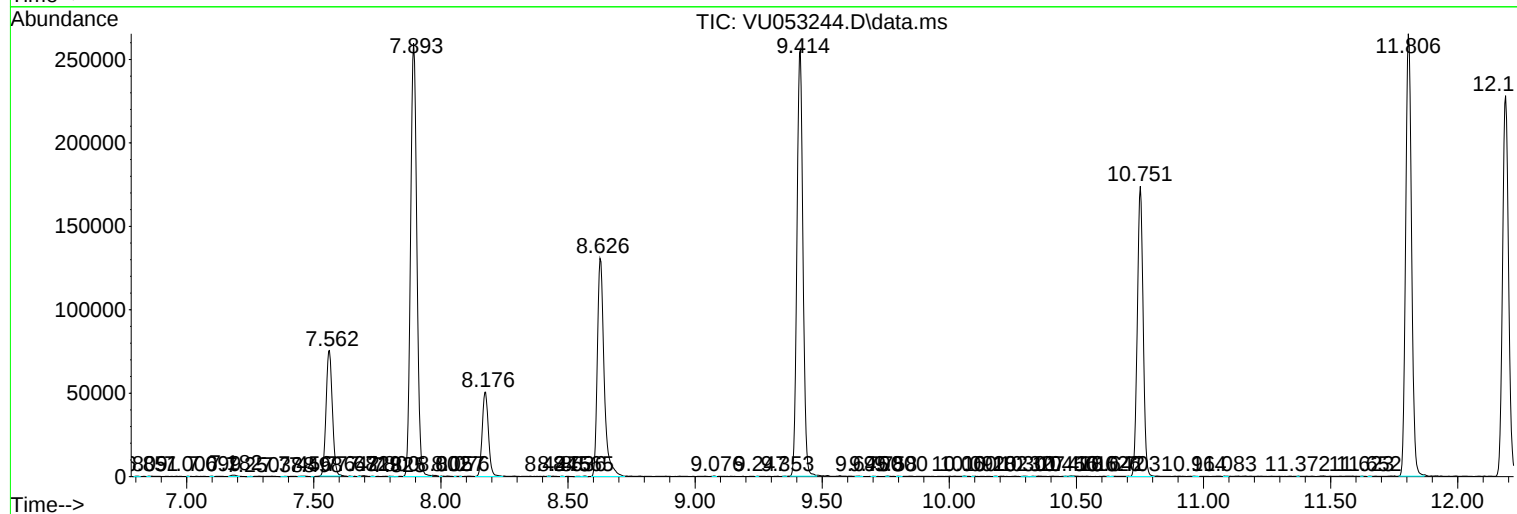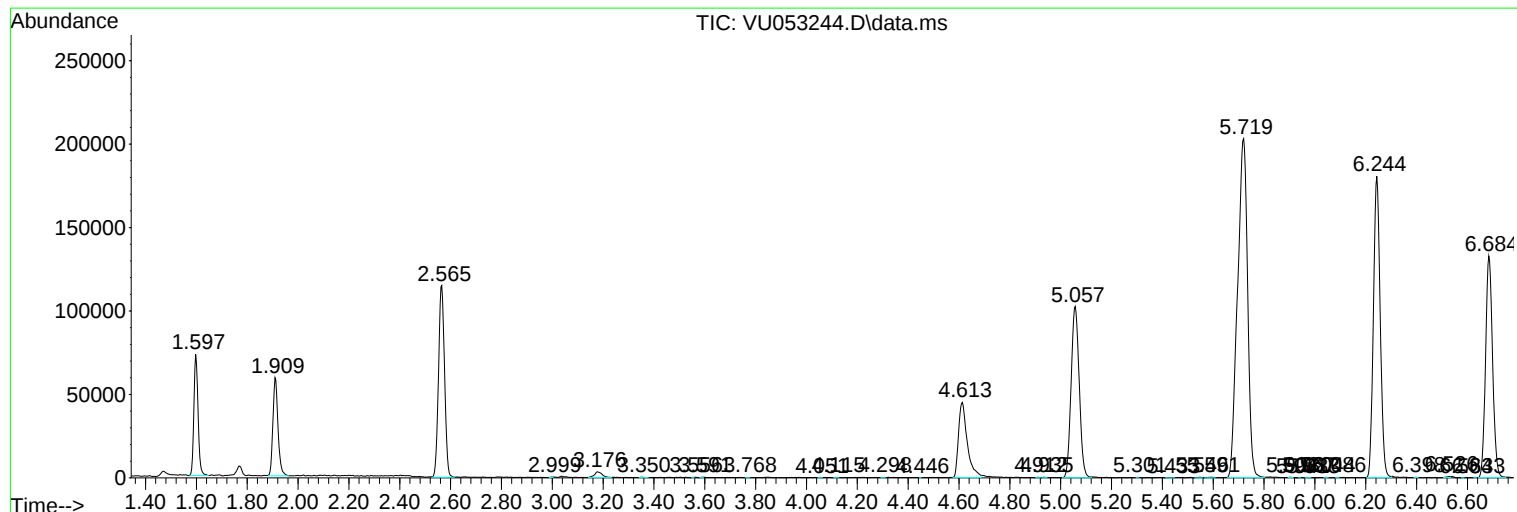

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053244.D
Acq On : 16 Mar 2023 22:35
Operator : JC/MD
Sample : 01930-15 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053244.D
Acq On : 16 Mar 2023 22:35
Operator : JC/MD
Sample : 01930-15 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc