

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053245.D
 Acq On : 16 Mar 2023 22:59
 Operator : JC/MD
 Sample : 01930-16 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053245.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	92	rVB	72124	81263	13.65%	1.887%
2	1.909	169	177	189	rBV	60885	80878	13.59%	1.878%
3	2.565	369	381	396	rVB	116393	188377	31.65%	4.373%
4	3.182	561	573	585	rBV2	2966	6364	1.07%	0.148%
5	3.411	641	644	651	rBV	211	141	0.02%	0.003%
6	3.607	702	705	707	rBV	166	77	0.01%	0.002%
7	3.690	729	731	733	rBV2	204	117	0.02%	0.003%
8	3.870	785	787	794	rVB	203	148	0.02%	0.003%
9	3.906	794	798	802	rBV2	208	214	0.04%	0.005%
10	4.256	904	907	912	rBV	207	142	0.02%	0.003%
11	4.414	953	956	959	rBV2	177	138	0.02%	0.003%
12	4.542	993	996	1000	rBV	222	157	0.03%	0.004%
13	4.613	1007	1018	1047	rBV2	43927	107959	18.14%	2.506%
14	4.819	1079	1082	1085	rBV	200	191	0.03%	0.004%
15	4.854	1090	1093	1098	rVB	191	145	0.02%	0.003%
16	5.057	1141	1156	1175	rBV2	103953	226385	38.04%	5.256%
17	5.189	1193	1197	1199	rBV	194	189	0.03%	0.004%
18	5.208	1200	1203	1210	rVB	294	300	0.05%	0.007%
19	5.276	1220	1224	1227	rBV2	287	204	0.03%	0.005%
20	5.513	1296	1298	1305	rBV	173	117	0.02%	0.003%
21	5.719	1342	1362	1392	rVV2	206621	595134	100.00%	13.816%
22	5.857	1403	1405	1408	rVB	288	99	0.02%	0.002%
23	5.909	1418	1421	1423	rBV	181	111	0.02%	0.003%
24	6.025	1455	1457	1459	rBV	159	92	0.02%	0.002%
25	6.121	1483	1487	1492	rVB2	210	205	0.03%	0.005%
26	6.147	1492	1495	1497	rBV	200	102	0.02%	0.002%
27	6.176	1501	1504	1505	rBV	184	83	0.01%	0.002%
28	6.243	1511	1525	1545	rBV	182788	342782	57.60%	7.958%
29	6.446	1586	1588	1589	rBV	131	74	0.01%	0.002%
30	6.501	1602	1605	1607	rBV	238	192	0.03%	0.004%
31	6.520	1607	1611	1612	rBV	384	253	0.04%	0.006%
32	6.684	1649	1662	1682	rBV	134744	259896	43.67%	6.033%
33	6.793	1694	1696	1698	rBV	140	78	0.01%	0.002%
34	6.861	1713	1717	1719	rBV	260	240	0.04%	0.006%
35	6.996	1756	1759	1763	rVB	183	93	0.02%	0.002%
36	7.050	1774	1776	1778	rBV	187	124	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053245.D
 Acq On : 16 Mar 2023 22:59
 Operator : JC/MD
 Sample : 01930-16 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	7.121	1795	1798	1800	rBV	209	153	0.03%	0.004%
38	7.179	1813	1816	1819	rBV3	479	388	0.07%	0.009%
39	7.311	1848	1857	1859	rBV	233	393	0.07%	0.009%
40	7.346	1866	1868	1871	rBV	212	81	0.01%	0.002%
41	7.462	1901	1904	1906	rBV	214	163	0.03%	0.004%
42	7.475	1906	1908	1910	rVV2	173	105	0.02%	0.002%
43	7.558	1921	1934	1957	rBV	74765	130821	21.98%	3.037%
44	7.652	1959	1963	1967	rVB2	273	214	0.04%	0.005%
45	7.671	1967	1969	1971	rBV	202	85	0.01%	0.002%
46	7.687	1971	1974	1975	rBV	354	218	0.04%	0.005%
47	7.828	2016	2018	2021	rVB	207	93	0.02%	0.002%
48	7.893	2021	2038	2059	rBV	260038	443590	74.54%	10.298%
49	8.176	2115	2126	2145	rBV	50126	84240	14.15%	1.956%
50	8.269	2152	2155	2157	rVB2	190	108	0.02%	0.003%
51	8.333	2173	2175	2177	rBV	172	118	0.02%	0.003%
52	8.381	2186	2190	2196	rBB	244	293	0.05%	0.007%
53	8.410	2196	2199	2201	rBV	197	150	0.03%	0.003%
54	8.626	2255	2266	2292	rBV2	131579	239948	40.32%	5.570%
55	8.835	2329	2331	2337	rBV	213	169	0.03%	0.004%
56	8.896	2347	2350	2353	rBV	195	156	0.03%	0.004%
57	9.021	2387	2389	2392	rBV2	252	170	0.03%	0.004%
58	9.092	2409	2411	2415	rBV	135	65	0.01%	0.002%
59	9.169	2431	2435	2436	rBV	271	201	0.03%	0.005%
60	9.224	2450	2452	2457	rVB	135	71	0.01%	0.002%
61	9.414	2498	2511	2527	rBV	257377	424659	71.36%	9.858%
62	9.565	2556	2558	2559	rBV	251	115	0.02%	0.003%
63	9.893	2658	2660	2664	rVB	180	74	0.01%	0.002%
64	9.922	2666	2669	2672	rBV	193	112	0.02%	0.003%
65	10.047	2706	2708	2710	rBV	176	72	0.01%	0.002%
66	10.179	2746	2749	2750	rBV	152	66	0.01%	0.002%
67	10.243	2766	2769	2770	rBV	221	130	0.02%	0.003%
68	10.295	2782	2785	2788	rBV2	201	135	0.02%	0.003%
69	10.346	2798	2801	2802	rBV	151	70	0.01%	0.002%
70	10.401	2815	2818	2824	rBV2	267	264	0.04%	0.006%
71	10.436	2828	2829	2833	rVB	154	64	0.01%	0.001%
72	10.561	2866	2868	2871	rVB	149	61	0.01%	0.001%
73	10.751	2914	2927	2945	rBV	174176	273438	45.95%	6.348%
74	10.889	2968	2970	2972	rBV	160	68	0.01%	0.002%
75	11.089	3029	3032	3038	rVB2	501	324	0.05%	0.008%
76	11.188	3060	3063	3065	rVB2	172	95	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053245.D
 Acq On : 16 Mar 2023 22:59
 Operator : JC/MD
 Sample : 01930-16 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	11.426	3135	3137	3142	rVB	180	65	0.01%	0.002%
78	11.745	3234	3236	3238	rVB2	210	91	0.02%	0.002%
79	11.761	3238	3241	3243	rBV2	284	179	0.03%	0.004%
80	11.806	3244	3255	3276	rVV	272536	429524	72.17%	9.971%
81	11.954	3299	3301	3304	rVB	189	78	0.01%	0.002%
82	12.188	3362	3374	3398	rBV	236358	379014	63.69%	8.799%
83	12.311	3408	3412	3415	rBV	181	130	0.02%	0.003%
84	12.484	3464	3466	3472	rVB2	154	116	0.02%	0.003%
85	12.626	3508	3510	3514	rBV	236	125	0.02%	0.003%
86	12.848	3577	3579	3584	rBV2	188	152	0.03%	0.004%
87	13.060	3643	3645	3649	rBV	217	87	0.01%	0.002%
88	13.217	3691	3694	3699	rBV2	440	354	0.06%	0.008%
89	13.452	3764	3767	3770	rVB2	260	151	0.03%	0.004%
90	13.468	3770	3772	3774	rBV	209	95	0.02%	0.002%
91	13.848	3886	3890	3897	rVB2	465	543	0.09%	0.013%
92	13.957	3922	3924	3929	rVB	309	236	0.04%	0.005%
93	14.050	3951	3953	3959	rVB	223	102	0.02%	0.002%
94	14.098	3962	3968	3969	rBV2	718	614	0.10%	0.014%
95	14.214	4001	4004	4005	rBV2	192	91	0.02%	0.002%
96	14.323	4036	4038	4039	rBV2	392	171	0.03%	0.004%
97	14.423	4064	4069	4071	rBV2	292	300	0.05%	0.007%
98	14.613	4124	4128	4132	rVB2	363	255	0.04%	0.006%
99	14.700	4152	4155	4159	rVB2	334	212	0.04%	0.005%
100	15.015	4251	4253	4254	rBV	234	73	0.01%	0.002%




Sum of corrected areas: 4307562

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053245.D
Acq On : 16 Mar 2023 22:59
Operator : JC/MD
Sample : 01930-16 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFC4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

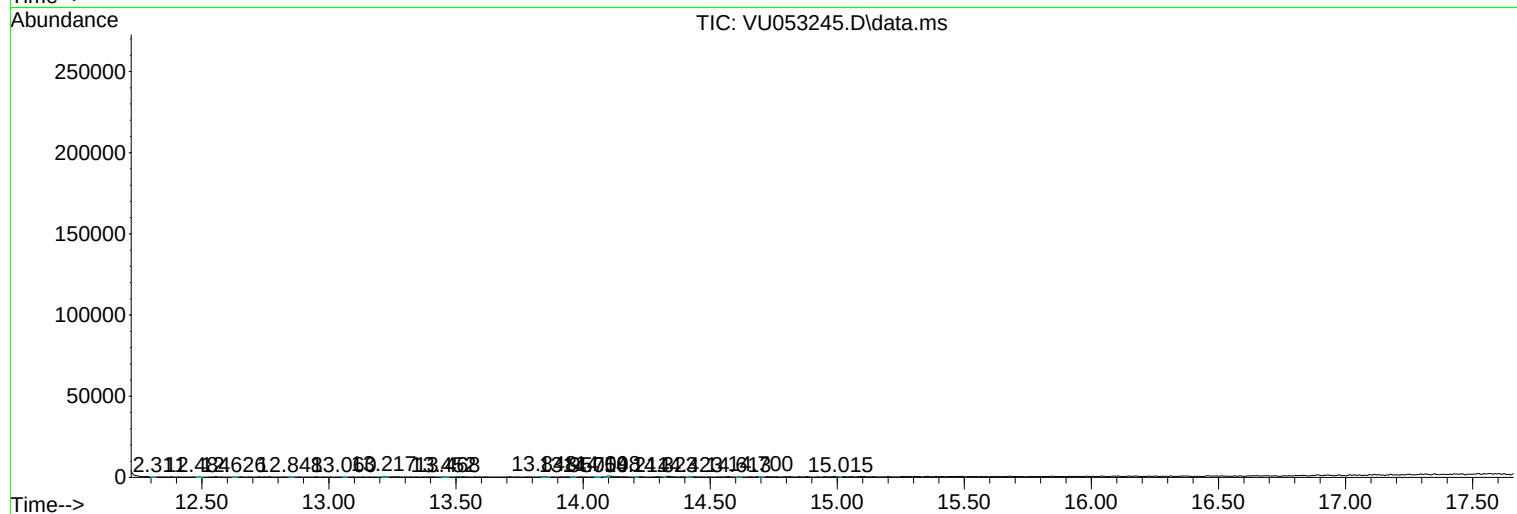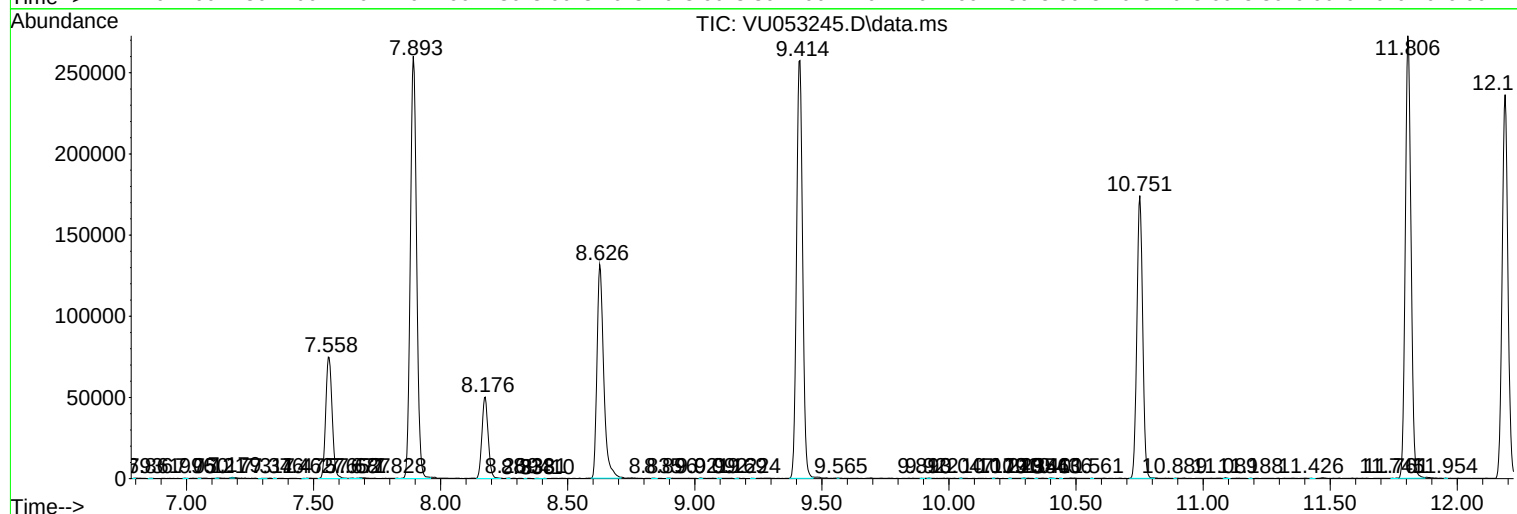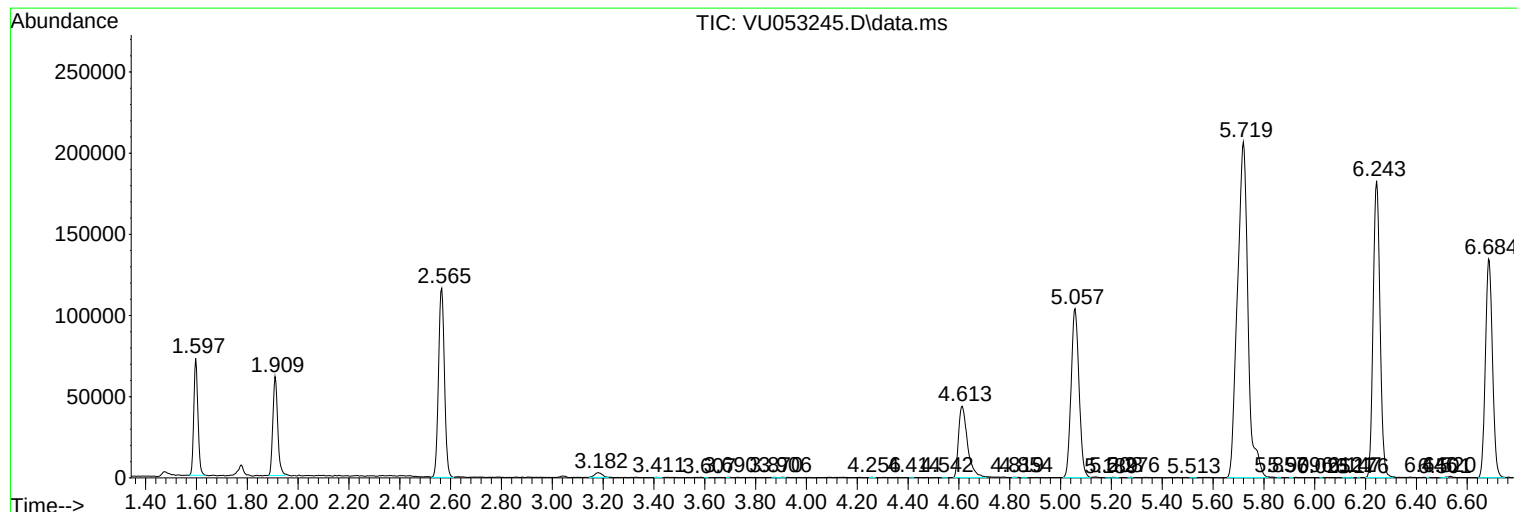

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053245.D
Acq On : 16 Mar 2023 22:59
Operator : JC/MD
Sample : 01930-16 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFC4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053245.D
Acq On : 16 Mar 2023 22:59
Operator : JC/MD
Sample : 01930-16 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFC4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------