

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053246.D
 Acq On : 16 Mar 2023 23:22
 Operator : JC/MD
 Sample : 01930-17 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053246.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB	71044	82628	14.95%	1.984%
2	1.909	169	177	193	rVB	59093	79706	14.43%	1.914%
3	2.565	369	381	395	rBV	116012	187020	33.85%	4.491%
4	3.047	523	531	538	rVB5	792	1311	0.24%	0.031%
5	3.176	562	571	573	rBV3	2524	3359	0.61%	0.081%
6	3.379	632	634	636	rVB	130	49	0.01%	0.001%
7	3.662	720	722	726	rBV	183	82	0.01%	0.002%
8	3.912	798	800	803	rBV	172	107	0.02%	0.003%
9	4.125	863	866	870	rBV	263	202	0.04%	0.005%
10	4.324	926	928	931	rVB	203	100	0.02%	0.002%
11	4.404	951	953	956	rBV	240	153	0.03%	0.004%
12	4.424	956	959	962	rBV2	201	161	0.03%	0.004%
13	4.481	973	977	984	rBV2	209	225	0.04%	0.005%
14	4.510	984	986	988	rVB	136	33	0.01%	0.001%
15	4.533	990	993	996	rBV	200	155	0.03%	0.004%
16	4.613	1007	1018	1049	rBV2	43426	107069	19.38%	2.571%
17	4.928	1114	1116	1119	rVB	148	43	0.01%	0.001%
18	5.057	1141	1156	1178	rBV	101894	222906	40.34%	5.353%
19	5.160	1186	1188	1189	rBV	123	30	0.01%	0.001%
20	5.205	1196	1202	1204	rBV	305	291	0.05%	0.007%
21	5.514	1296	1298	1299	rBV	176	83	0.02%	0.002%
22	5.719	1340	1362	1381	rBV2	203054	552542	100.00%	13.269%
23	6.096	1477	1479	1481	rBV2	175	98	0.02%	0.002%
24	6.134	1488	1491	1492	rBV2	296	170	0.03%	0.004%
25	6.189	1502	1508	1510	rBV	316	313	0.06%	0.008%
26	6.243	1512	1525	1548	rVV	173680	328183	59.40%	7.881%
27	6.462	1589	1593	1595	rBV2	194	173	0.03%	0.004%
28	6.526	1609	1613	1614	rBV2	692	432	0.08%	0.010%
29	6.578	1627	1629	1632	rVB	153	49	0.01%	0.001%
30	6.684	1649	1662	1684	rBV	128797	251633	45.54%	6.043%
31	6.777	1689	1691	1695	rBV	156	49	0.01%	0.001%
32	6.977	1752	1753	1756	rVB	133	50	0.01%	0.001%
33	6.996	1757	1759	1761	rBV	166	77	0.01%	0.002%
34	7.092	1786	1789	1791	rBV	151	130	0.02%	0.003%
35	7.108	1793	1794	1795	rVV	113	29	0.01%	0.001%
36	7.231	1827	1832	1834	rBV	202	233	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053246.D
 Acq On : 16 Mar 2023 23:22
 Operator : JC/MD
 Sample : 01930-17 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	7.343	1864	1867	1872	rBV	251	195	0.04%	0.005%
38	7.562	1923	1935	1951	rBV	72958	125385	22.69%	3.011%
39	7.687	1972	1974	1983	rVB3	715	697	0.13%	0.017%
40	7.809	2011	2012	2013	rVB3	116	22	0.00%	0.001%
41	7.893	2025	2038	2057	rBV	254054	432606	78.29%	10.389%
42	8.063	2088	2091	2094	rBV	330	256	0.05%	0.006%
43	8.079	2094	2096	2099	rVV	337	225	0.04%	0.005%
44	8.099	2099	2102	2107	rVV2	291	274	0.05%	0.007%
45	8.124	2107	2110	2115	rVV2	335	336	0.06%	0.008%
46	8.173	2115	2125	2142	rVV	49679	84611	15.31%	2.032%
47	8.247	2146	2148	2158	rVB2	302	300	0.05%	0.007%
48	8.414	2198	2200	2203	rVB	139	45	0.01%	0.001%
49	8.626	2255	2266	2297	rBV2	127325	235846	42.68%	5.664%
50	8.954	2366	2368	2369	rVB	112	25	0.00%	0.001%
51	8.989	2377	2379	2381	rVB	175	67	0.01%	0.002%
52	9.002	2381	2383	2386	rBV	99	72	0.01%	0.002%
53	9.050	2396	2398	2405	rBV	170	149	0.03%	0.004%
54	9.147	2424	2428	2433	rVB2	316	273	0.05%	0.007%
55	9.173	2434	2436	2437	rVB	115	26	0.00%	0.001%
56	9.211	2446	2448	2453	rVB	195	99	0.02%	0.002%
57	9.295	2471	2474	2477	rBV	282	222	0.04%	0.005%
58	9.414	2498	2511	2532	rBV	247773	406952	73.65%	9.773%
59	9.558	2554	2556	2558	rBV	279	87	0.02%	0.002%
60	9.571	2558	2560	2563	rVB	235	146	0.03%	0.004%
61	9.648	2582	2584	2585	rBV	114	26	0.00%	0.001%
62	9.697	2597	2599	2600	rBV	135	74	0.01%	0.002%
63	9.906	2660	2664	2668	rVB2	250	176	0.03%	0.004%
64	9.996	2689	2692	2695	rVB	213	126	0.02%	0.003%
65	10.082	2716	2719	2720	rBV	183	123	0.02%	0.003%
66	10.243	2767	2769	2772	rBV	106	62	0.01%	0.001%
67	10.272	2776	2778	2783	rVB	247	117	0.02%	0.003%
68	10.459	2835	2836	2837	rBV	146	31	0.01%	0.001%
69	10.491	2844	2846	2847	rBV	130	61	0.01%	0.001%
70	10.539	2857	2861	2862	rBV	191	158	0.03%	0.004%
71	10.587	2873	2876	2877	rBV	139	63	0.01%	0.002%
72	10.645	2892	2894	2899	rVB	200	120	0.02%	0.003%
73	10.751	2914	2927	2945	rVB	169534	267561	48.42%	6.425%
74	10.819	2945	2948	2952	rBV	283	202	0.04%	0.005%
75	10.870	2960	2964	2965	rBV2	186	121	0.02%	0.003%
76	11.259	3079	3085	3086	rBV	274	257	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053246.D
 Acq On : 16 Mar 2023 23:22
 Operator : JC/MD
 Sample : 01930-17 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	11.314	3099	3102	3104	rBV	188	110	0.02%	0.003%
78	11.336	3108	3109	3110	rBV	236	83	0.02%	0.002%
79	11.459	3146	3147	3151	rVB	322	147	0.03%	0.004%
80	11.664	3209	3211	3213	rBV	200	68	0.01%	0.002%
81	11.745	3234	3236	3242	rBV2	398	325	0.06%	0.008%
82	11.806	3243	3255	3275	rBV	264285	415226	75.15%	9.972%
83	12.021	3319	3322	3324	rBV	199	155	0.03%	0.004%
84	12.089	3341	3343	3346	rBV	173	85	0.02%	0.002%
85	12.189	3361	3374	3394	rBV	228076	368145	66.63%	8.841%
86	12.574	3492	3494	3496	rBV	173	55	0.01%	0.001%
87	13.131	3666	3667	3671	rBV	122	83	0.02%	0.002%
88	13.230	3694	3698	3701	rBV2	277	204	0.04%	0.005%
89	13.336	3729	3731	3733	rBV	164	53	0.01%	0.001%
90	13.832	3881	3885	3888	rBV	222	195	0.04%	0.005%
91	13.934	3915	3917	3919	rBV	155	63	0.01%	0.002%
92	14.176	3990	3992	3994	rBV	168	60	0.01%	0.001%
93	14.214	3999	4004	4010	rBV2	264	317	0.06%	0.008%
94	14.333	4038	4041	4044	rBV2	294	238	0.04%	0.006%
95	14.478	4085	4086	4090	rBV	135	53	0.01%	0.001%
96	14.571	4112	4115	4120	rBV2	207	203	0.04%	0.005%
97	14.671	4143	4146	4149	rBV	262	156	0.03%	0.004%




Sum of corrected areas: 4164092

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053246.D
Acq On : 16 Mar 2023 23:22
Operator : JC/MD
Sample : 01930-17 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

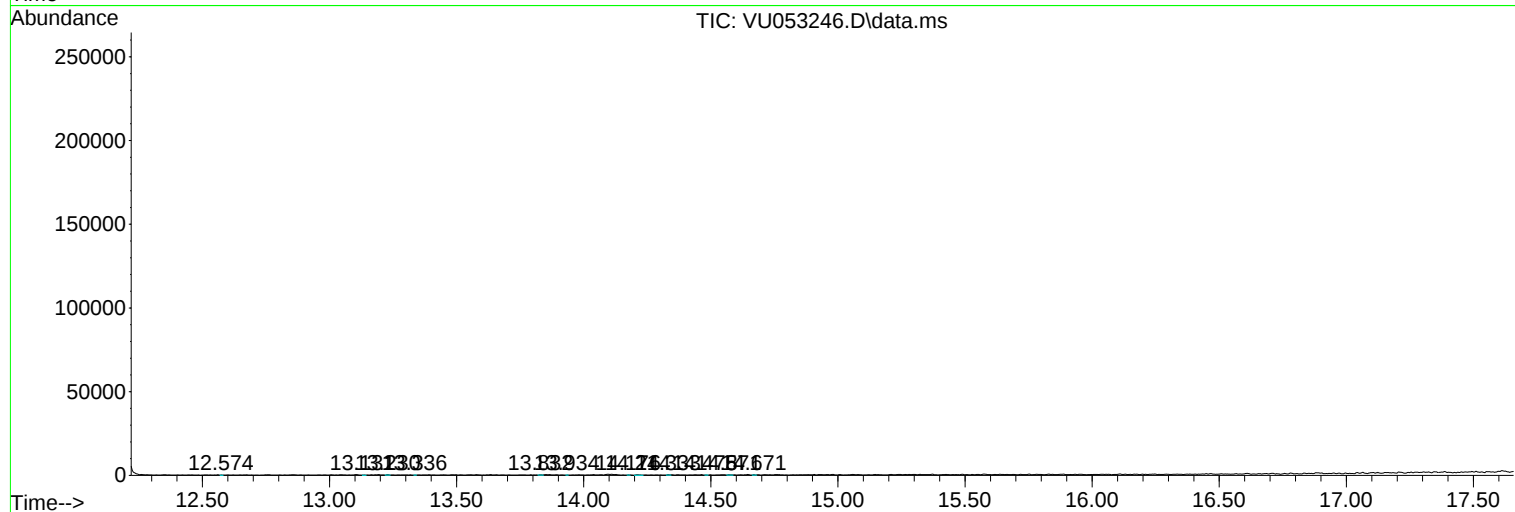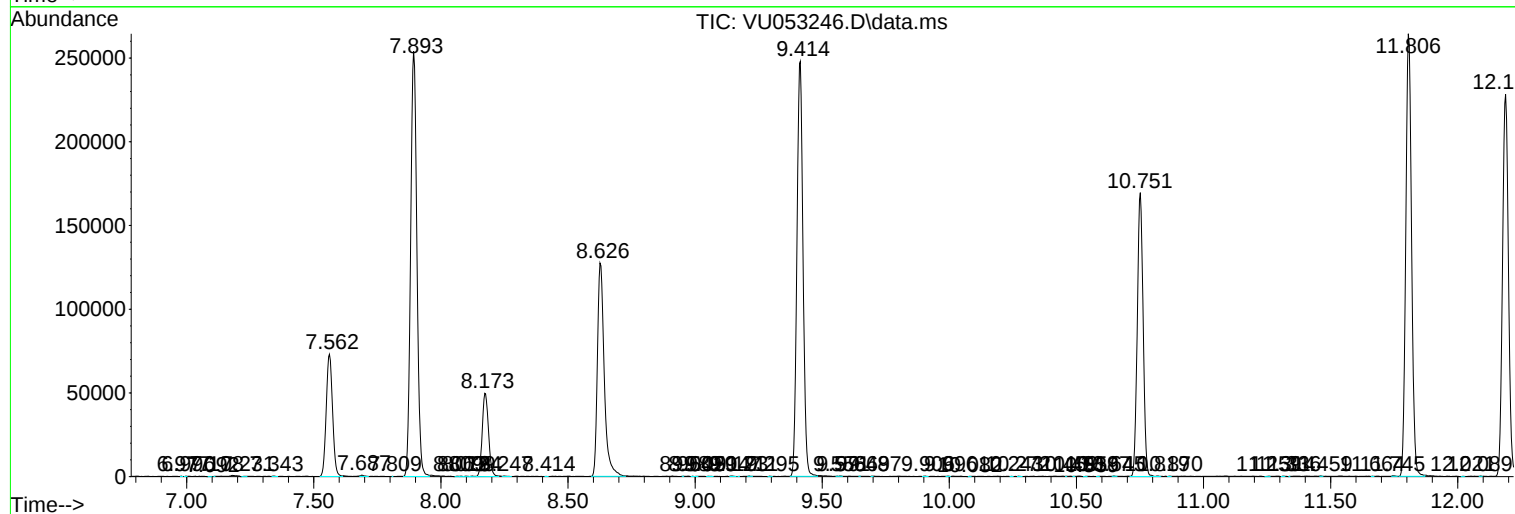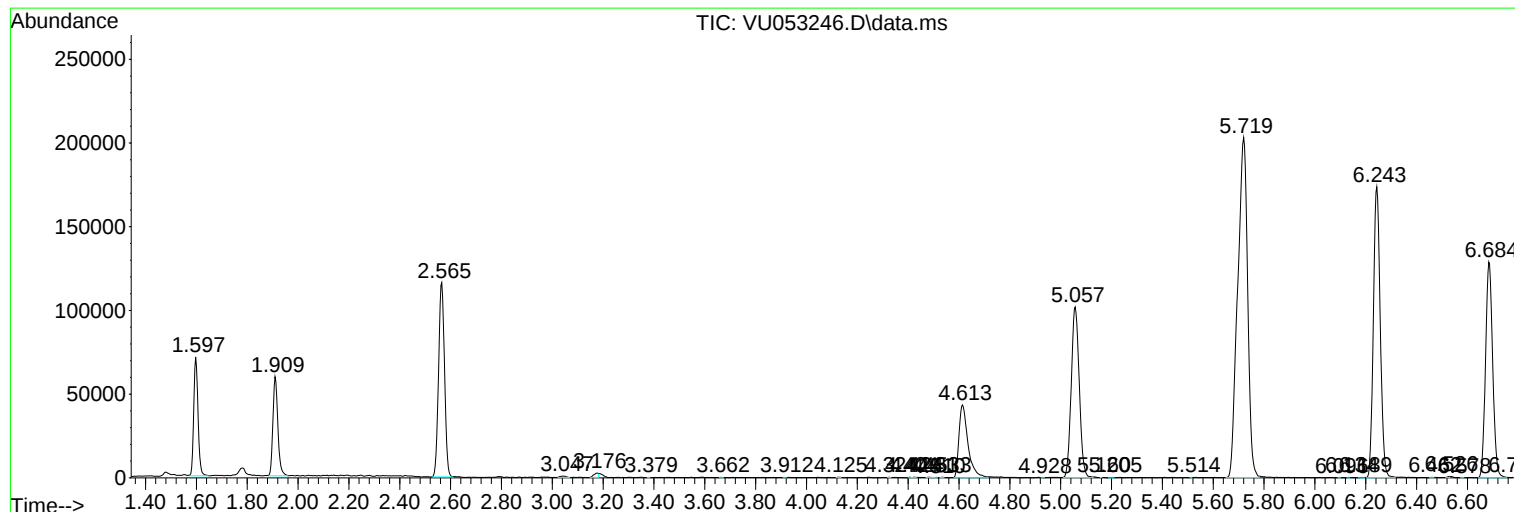

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053246.D
Acq On : 16 Mar 2023 23:22
Operator : JC/MD
Sample : 01930-17 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053246.D
Acq On : 16 Mar 2023 23:22
Operator : JC/MD
Sample : 01930-17 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------