

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053248.D
 Acq On : 17 Mar 2023 00:10
 Operator : JC/MD
 Sample : 01930-19 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053248.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB	72021	82291	14.41%	1.909%
2	1.909	169	177	197	rVB	59896	80008	14.01%	1.856%
3	2.565	369	381	395	rBV	115916	183794	32.17%	4.265%
4	3.041	523	529	532	rBV4	664	838	0.15%	0.019%
5	3.388	635	637	641	rBV	153	79	0.01%	0.002%
6	3.681	725	728	730	rVB2	234	132	0.02%	0.003%
7	3.723	739	741	744	rBV	154	85	0.01%	0.002%
8	3.954	811	813	816	rVB	192	85	0.01%	0.002%
9	4.044	838	841	843	rBV	150	73	0.01%	0.002%
10	4.096	855	857	858	rBV	155	47	0.01%	0.001%
11	4.263	907	909	910	rBV	144	39	0.01%	0.001%
12	4.298	917	920	924	rVB	203	132	0.02%	0.003%
13	4.356	935	938	943	rBV	209	187	0.03%	0.004%
14	4.485	976	978	979	rBV	128	35	0.01%	0.001%
15	4.510	984	986	989	rVV	193	70	0.01%	0.002%
16	4.578	1004	1007	1008	rBV	265	144	0.03%	0.003%
17	4.613	1008	1018	1041	rVV	43968	106889	18.71%	2.480%
18	4.816	1078	1081	1083	rBV2	249	162	0.03%	0.004%
19	4.829	1083	1085	1088	rBV	152	46	0.01%	0.001%
20	4.896	1103	1106	1111	rBV2	311	209	0.04%	0.005%
21	4.928	1114	1116	1120	rBV	267	205	0.04%	0.005%
22	5.057	1141	1156	1173	rBV	107173	229713	40.21%	5.330%
23	5.186	1195	1196	1198	rBV	144	66	0.01%	0.002%
24	5.298	1229	1231	1235	rBV	134	146	0.03%	0.003%
25	5.317	1235	1237	1238	rVB	107	32	0.01%	0.001%
26	5.597	1320	1324	1330	rBV2	351	477	0.08%	0.011%
27	5.719	1341	1362	1384	rBV2	209579	571256	100.00%	13.255%
28	6.243	1512	1525	1548	rBV	189702	355226	62.18%	8.242%
29	6.382	1566	1568	1572	rBV	166	89	0.02%	0.002%
30	6.526	1610	1613	1615	rBV2	493	348	0.06%	0.008%
31	6.575	1625	1628	1629	rBV	255	146	0.03%	0.003%
32	6.600	1633	1636	1639	rBV	162	167	0.03%	0.004%
33	6.684	1648	1662	1687	rVB	135570	262644	45.98%	6.094%
34	6.771	1687	1689	1692	rVB	265	150	0.03%	0.003%
35	6.793	1692	1696	1699	rBV	289	251	0.04%	0.006%
36	6.809	1699	1701	1704	rBV	175	83	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053248.D
 Acq On : 17 Mar 2023 00:10
 Operator : JC/MD
 Sample : 01930-19 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.867	1716	1719	1726	rVB	236	163	0.03%	0.004%
38	6.909	1730	1732	1733	rBV	124	69	0.01%	0.002%
39	6.993	1756	1758	1759	rBV	117	65	0.01%	0.002%
40	7.031	1768	1770	1773	rBV	193	85	0.01%	0.002%
41	7.076	1782	1784	1787	rVB	220	91	0.02%	0.002%
42	7.179	1813	1816	1817	rBV	528	318	0.06%	0.007%
43	7.243	1834	1836	1838	rBV	142	44	0.01%	0.001%
44	7.311	1856	1857	1859	rVB	226	64	0.01%	0.001%
45	7.343	1860	1867	1868	rBV	306	301	0.05%	0.007%
46	7.427	1891	1893	1895	rBV	177	84	0.01%	0.002%
47	7.562	1923	1935	1950	rBV	73699	129760	22.71%	3.011%
48	7.684	1969	1973	1974	rBV	461	293	0.05%	0.007%
49	7.796	2002	2008	2010	rBV	200	226	0.04%	0.005%
50	7.893	2025	2038	2064	rBV	257344	445980	78.07%	10.348%
51	8.089	2097	2099	2100	rBV	135	58	0.01%	0.001%
52	8.173	2114	2125	2144	rVB	52158	85747	15.01%	1.990%
53	8.250	2147	2149	2152	rBV	213	143	0.03%	0.003%
54	8.330	2172	2174	2177	rBV2	161	98	0.02%	0.002%
55	8.372	2183	2187	2191	rVB	333	328	0.06%	0.008%
56	8.404	2192	2197	2202	rBV	234	383	0.07%	0.009%
57	8.626	2256	2266	2294	rBV2	129076	241337	42.25%	5.600%
58	8.832	2328	2330	2332	rBV	223	122	0.02%	0.003%
59	9.317	2479	2481	2486	rVB	160	83	0.01%	0.002%
60	9.414	2498	2511	2534	rBV	267119	437243	76.54%	10.145%
61	9.533	2545	2548	2552	rBV2	338	236	0.04%	0.005%
62	9.603	2568	2570	2572	rVB	190	76	0.01%	0.002%
63	9.668	2588	2590	2592	rVB	176	73	0.01%	0.002%
64	9.700	2598	2600	2603	rVB	156	46	0.01%	0.001%
65	9.845	2643	2645	2649	rBV	159	66	0.01%	0.002%
66	9.925	2666	2670	2671	rBV	204	168	0.03%	0.004%
67	10.028	2698	2702	2706	rBV	264	324	0.06%	0.008%
68	10.099	2720	2724	2727	rVB	357	309	0.05%	0.007%
69	10.118	2727	2730	2734	rBV	221	252	0.04%	0.006%
70	10.160	2739	2743	2745	rBV2	239	176	0.03%	0.004%
71	10.288	2781	2783	2786	rVB	151	44	0.01%	0.001%
72	10.385	2811	2813	2814	rBV	156	45	0.01%	0.001%
73	10.571	2867	2871	2876	rBV2	271	254	0.04%	0.006%
74	10.751	2915	2927	2942	rBV	172146	275630	48.25%	6.395%
75	10.835	2950	2953	2959	rVB	203	132	0.02%	0.003%
76	11.009	3005	3007	3008	rBV	120	28	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053248.D
 Acq On : 17 Mar 2023 00:10
 Operator : JC/MD
 Sample : 01930-19 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	11.044	3015	3018	3021	rBV	215	122	0.02%	0.003%
78	11.279	3089	3091	3093	rBV	152	106	0.02%	0.002%
79	11.317	3101	3103	3105	rBV	314	200	0.04%	0.005%
80	11.655	3205	3208	3211	rBV	229	137	0.02%	0.003%
81	11.738	3232	3234	3235	rBV	144	64	0.01%	0.001%
82	11.806	3244	3255	3278	rBV	274485	434828	76.12%	10.089%
83	12.189	3362	3374	3396	rBV	235814	376160	65.85%	8.728%
84	12.308	3409	3411	3419	rVB	216	185	0.03%	0.004%
85	12.607	3501	3504	3508	rBV2	198	164	0.03%	0.004%
86	12.771	3553	3555	3557	rBV	189	80	0.01%	0.002%
87	12.893	3590	3593	3595	rBV	187	100	0.02%	0.002%
88	13.346	3732	3734	3738	rVB	181	77	0.01%	0.002%
89	14.134	3975	3979	3980	rBV2	331	165	0.03%	0.004%
90	14.414	4063	4066	4071	rVB	248	179	0.03%	0.004%




Sum of corrected areas: 4309855

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053248.D
Acq On : 17 Mar 2023 00:10
Operator : JC/MD
Sample : 01930-19 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFF8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

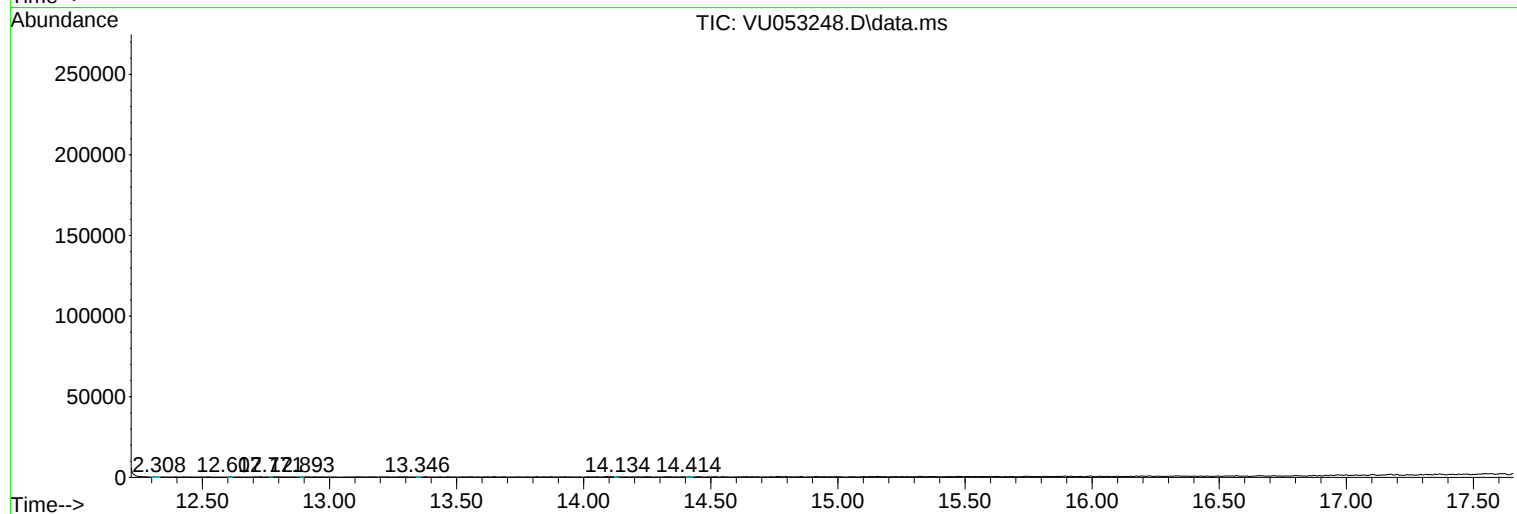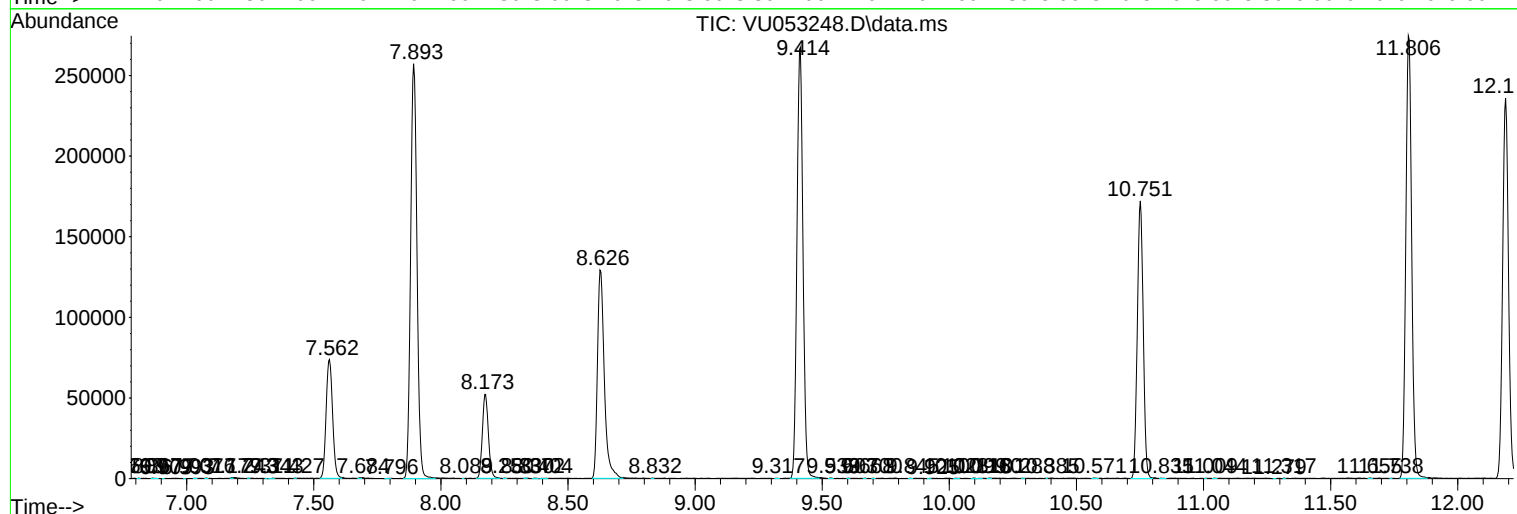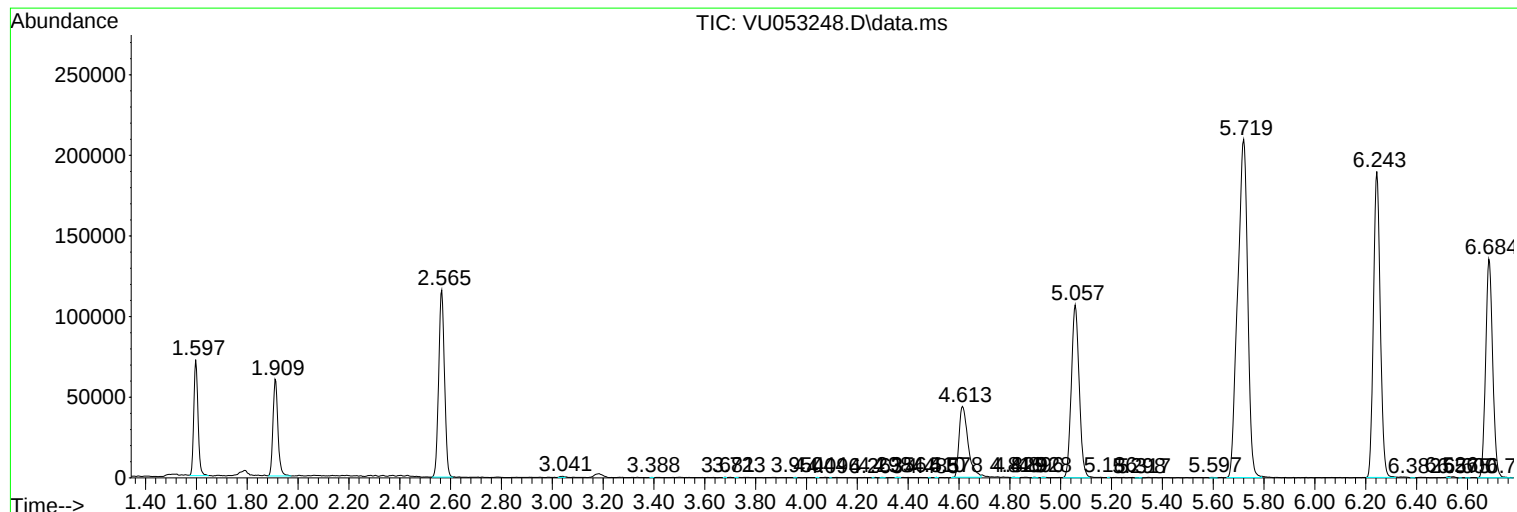

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053248.D
Acq On : 17 Mar 2023 00:10
Operator : JC/MD
Sample : 01930-19 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFF8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053248.D
Acq On : 17 Mar 2023 00:10
Operator : JC/MD
Sample : 01930-19 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFF8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc