

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053250.D
 Acq On : 17 Mar 2023 00:57
 Operator : JC/MD
 Sample : 01930-21 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053250.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rVB	70628	78836	14.17%	1.876%
2	1.909	169	177	194	rBV	58204	77987	14.02%	1.856%
3	2.565	369	381	397	rVB	113448	181033	32.54%	4.308%
4	2.806	454	456	462	rVB	277	196	0.04%	0.005%
5	3.073	537	539	541	rBV	213	91	0.02%	0.002%
6	3.182	560	573	591	rBV2	3016	6412	1.15%	0.153%
7	3.867	784	786	787	rBV	137	33	0.01%	0.001%
8	3.883	788	791	793	rBV	230	158	0.03%	0.004%
9	3.989	820	824	825	rBV	230	141	0.03%	0.003%
10	4.112	860	862	865	rBV	184	90	0.02%	0.002%
11	4.141	869	871	872	rBV	146	42	0.01%	0.001%
12	4.285	913	916	918	rBV	217	119	0.02%	0.003%
13	4.526	988	991	992	rBV	168	102	0.02%	0.002%
14	4.616	1008	1019	1046	rBV	46488	112432	20.21%	2.675%
15	4.819	1080	1082	1085	rBV	186	85	0.02%	0.002%
16	4.858	1092	1094	1097	rVB2	278	139	0.02%	0.003%
17	4.874	1097	1099	1100	rVV	131	36	0.01%	0.001%
18	4.887	1100	1103	1106	rVB2	235	151	0.03%	0.004%
19	5.057	1140	1156	1180	rVB	103866	222412	39.98%	5.293%
20	5.144	1180	1183	1187	rBV	148	123	0.02%	0.003%
21	5.176	1191	1193	1195	rVB	157	83	0.01%	0.002%
22	5.285	1224	1227	1230	rBV	168	104	0.02%	0.002%
23	5.324	1236	1239	1243	rVB2	246	195	0.04%	0.005%
24	5.401	1260	1263	1266	rBB2	206	118	0.02%	0.003%
25	5.501	1291	1294	1295	rBV	169	118	0.02%	0.003%
26	5.594	1321	1323	1327	rBV	144	83	0.01%	0.002%
27	5.719	1341	1362	1393	rBV2	200463	556266	100.00%	13.237%
28	5.944	1428	1432	1433	rBV	234	162	0.03%	0.004%
29	6.054	1464	1466	1467	rBV	127	58	0.01%	0.001%
30	6.243	1512	1525	1544	rBV	180461	340769	61.26%	8.109%
31	6.475	1594	1597	1602	rBV	326	279	0.05%	0.007%
32	6.513	1607	1609	1610	rVV2	217	114	0.02%	0.003%
33	6.530	1611	1614	1615	rVV2	531	303	0.05%	0.007%
34	6.542	1615	1618	1627	rVB4	753	628	0.11%	0.015%
35	6.587	1629	1632	1636	rBV	196	165	0.03%	0.004%
36	6.632	1644	1646	1648	rBV	159	64	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053250.D
 Acq On : 17 Mar 2023 00:57
 Operator : JC/MD
 Sample : 01930-21 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.684	1648	1662	1681	rBV2	129123	253239	45.52%	6.026%
38	6.784	1691	1693	1696	rBV	252	168	0.03%	0.004%
39	6.803	1696	1699	1701	rVV2	314	206	0.04%	0.005%
40	6.957	1743	1747	1751	rBB	246	263	0.05%	0.006%
41	6.986	1751	1756	1757	rBV	246	212	0.04%	0.005%
42	7.102	1784	1792	1794	rBV	236	324	0.06%	0.008%
43	7.173	1812	1814	1815	rBV	349	161	0.03%	0.004%
44	7.259	1837	1841	1842	rBV	249	167	0.03%	0.004%
45	7.513	1917	1920	1923	rBV2	177	125	0.02%	0.003%
46	7.562	1923	1935	1952	rVV	72388	124736	22.42%	2.968%
47	7.677	1968	1971	1973	rBV2	394	321	0.06%	0.008%
48	7.793	2004	2007	2009	rBV	255	138	0.02%	0.003%
49	7.816	2012	2014	2017	rBV2	186	83	0.01%	0.002%
50	7.893	2025	2038	2064	rBV	247883	428146	76.97%	10.188%
51	8.134	2110	2113	2115	rBV	232	182	0.03%	0.004%
52	8.176	2115	2126	2142	rVV	49615	81999	14.74%	1.951%
53	8.253	2146	2150	2153	rVB	208	184	0.03%	0.004%
54	8.427	2202	2204	2206	rBV	146	104	0.02%	0.002%
55	8.626	2256	2266	2296	rBV2	129372	238994	42.96%	5.687%
56	8.800	2317	2320	2323	rBV2	155	136	0.02%	0.003%
57	9.031	2388	2392	2395	rBV2	189	151	0.03%	0.004%
58	9.121	2418	2420	2422	rVB	163	83	0.01%	0.002%
59	9.205	2442	2446	2449	rBV2	296	229	0.04%	0.005%
60	9.288	2470	2472	2474	rBV	177	110	0.02%	0.003%
61	9.414	2498	2511	2534	rBV	261019	423798	76.19%	10.085%
62	9.571	2555	2560	2563	rBV	174	188	0.03%	0.004%
63	9.607	2566	2571	2575	rBV2	285	245	0.04%	0.006%
64	9.693	2597	2598	2600	rBV2	229	76	0.01%	0.002%
65	9.870	2651	2653	2656	rVB	180	60	0.01%	0.001%
66	9.957	2678	2680	2684	rBV	186	91	0.02%	0.002%
67	10.105	2723	2726	2729	rVB	281	177	0.03%	0.004%
68	10.211	2757	2759	2765	rVB	239	144	0.03%	0.003%
69	10.237	2765	2767	2769	rBV	170	74	0.01%	0.002%
70	10.266	2774	2776	2777	rVB	109	26	0.00%	0.001%
71	10.359	2802	2805	2806	rBV	141	61	0.01%	0.001%
72	10.401	2815	2818	2823	rBV2	197	161	0.03%	0.004%
73	10.436	2827	2829	2832	rBV	162	74	0.01%	0.002%
74	10.478	2840	2842	2846	rBV	292	194	0.03%	0.005%
75	10.751	2915	2927	2947	rVB	169907	268237	48.22%	6.383%
76	11.108	3036	3038	3039	rBV	146	60	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
 Data File : VU053250.D
 Acq On : 17 Mar 2023 00:57
 Operator : JC/MD
 Sample : 01930-21 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	11.468	3148	3150	3153	rVB2	292	155	0.03%	0.004%
78	11.745	3234	3236	3240	rVB	227	119	0.02%	0.003%
79	11.806	3243	3255	3278	rBV	272353	427543	76.86%	10.174%
80	12.092	3341	3344	3346	rBV	219	125	0.02%	0.003%
81	12.188	3361	3374	3390	rBV	227402	368677	66.28%	8.773%
82	12.455	3455	3457	3459	rBV	175	65	0.01%	0.002%
83	12.873	3584	3587	3588	rBV	211	101	0.02%	0.002%
84	12.970	3615	3617	3620	rVB	196	63	0.01%	0.001%
85	13.311	3719	3723	3727	rBV	281	223	0.04%	0.005%
86	13.333	3727	3730	3734	rVB	378	232	0.04%	0.006%
87	13.989	3932	3934	3936	rBV	136	45	0.01%	0.001%
88	14.221	4005	4006	4009	rBV2	219	115	0.02%	0.003%
89	14.320	4034	4037	4040	rVB2	282	185	0.03%	0.004%
90	14.516	4096	4098	4104	rBV	163	110	0.02%	0.003%
91	14.928	4224	4226	4227	rBV	143	37	0.01%	0.001%
92	15.069	4268	4270	4278	rBV2	251	258	0.05%	0.006%




Sum of corrected areas: 4202307

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053250.D
Acq On : 17 Mar 2023 00:57
Operator : JC/MD
Sample : 01930-21 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

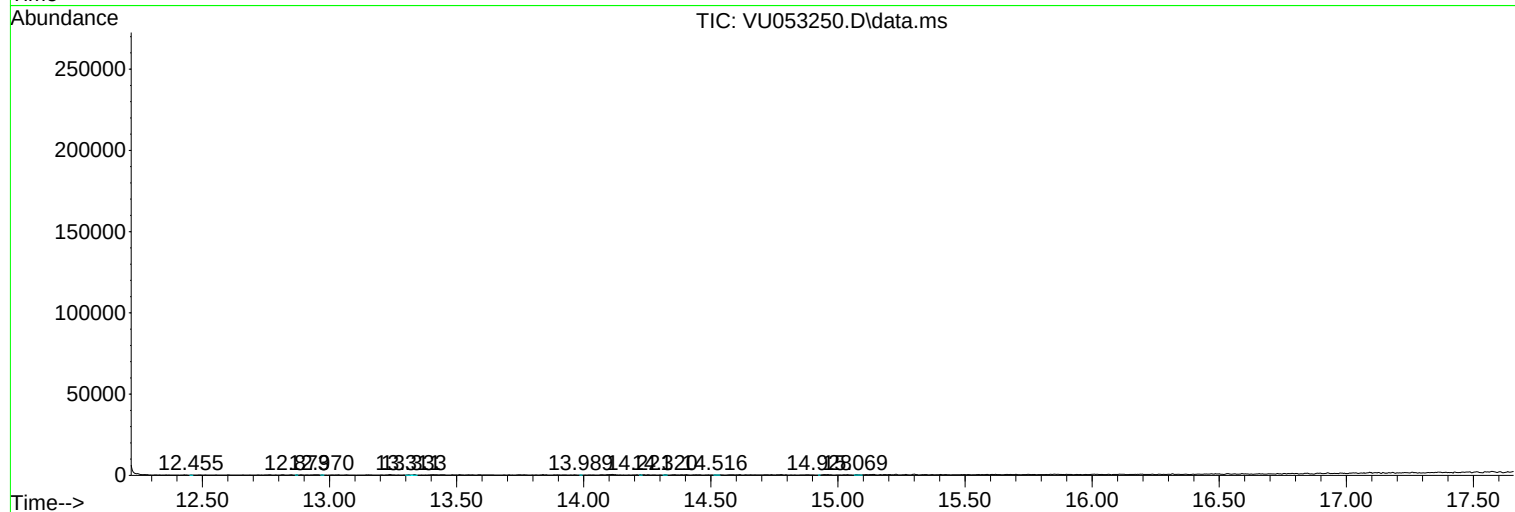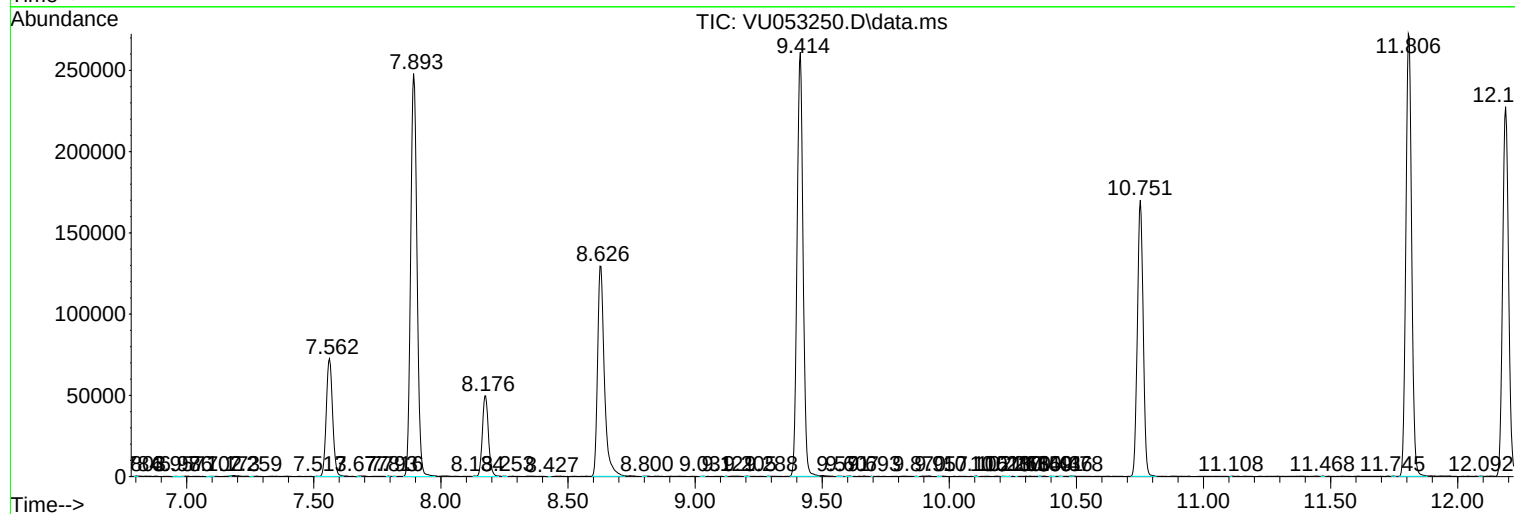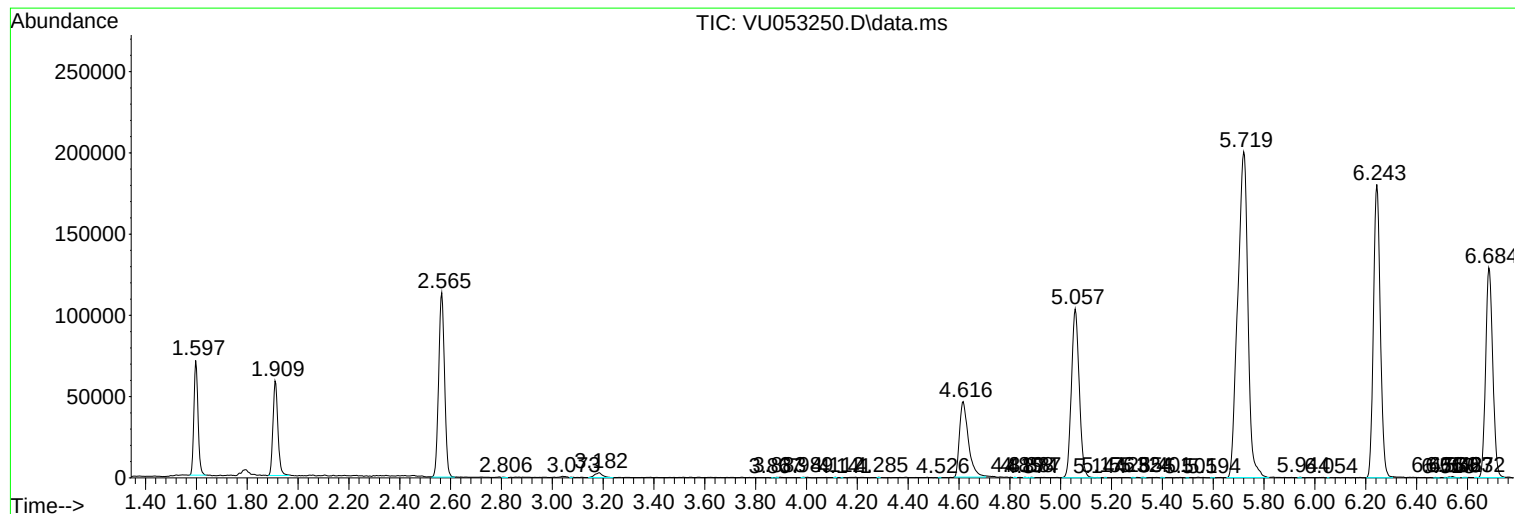

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053250.D
Acq On : 17 Mar 2023 00:57
Operator : JC/MD
Sample : 01930-21 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053250.D
Acq On : 17 Mar 2023 00:57
Operator : JC/MD
Sample : 01930-21 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc