
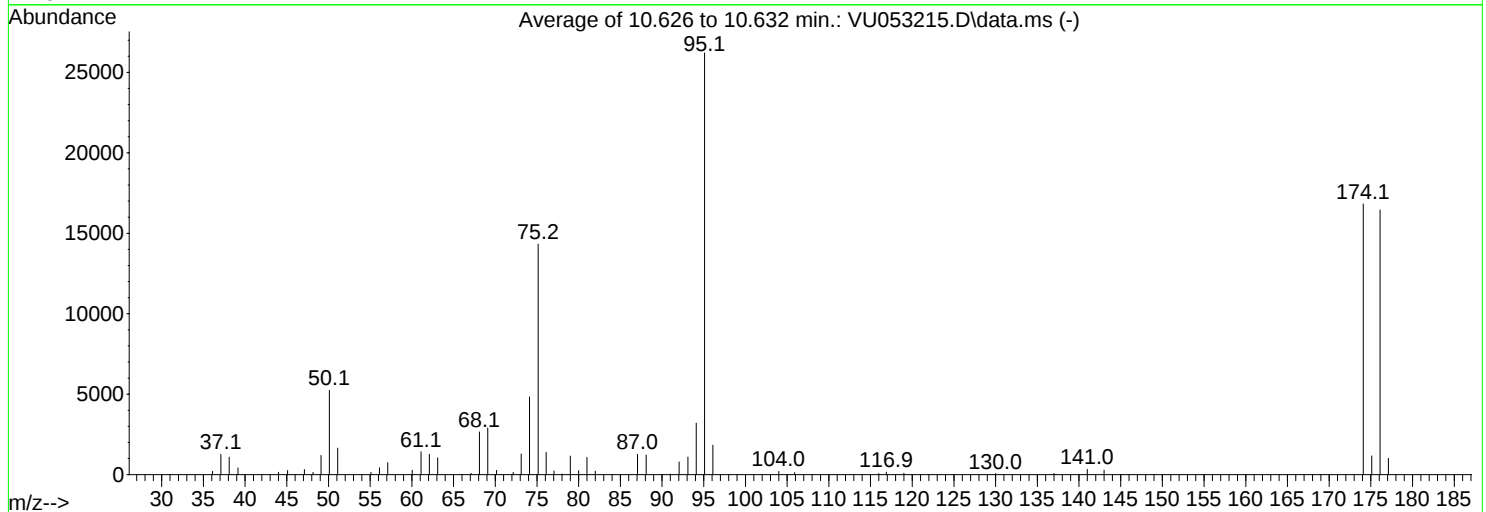


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031623\
Data File : VU053215.D
Acq On : 16 Mar 2023 09:08
Operator : JC/MD
Sample : BFB164
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB164

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Title : VOC Analysis
Last Update : Tue Mar 21 01:25:41 2023

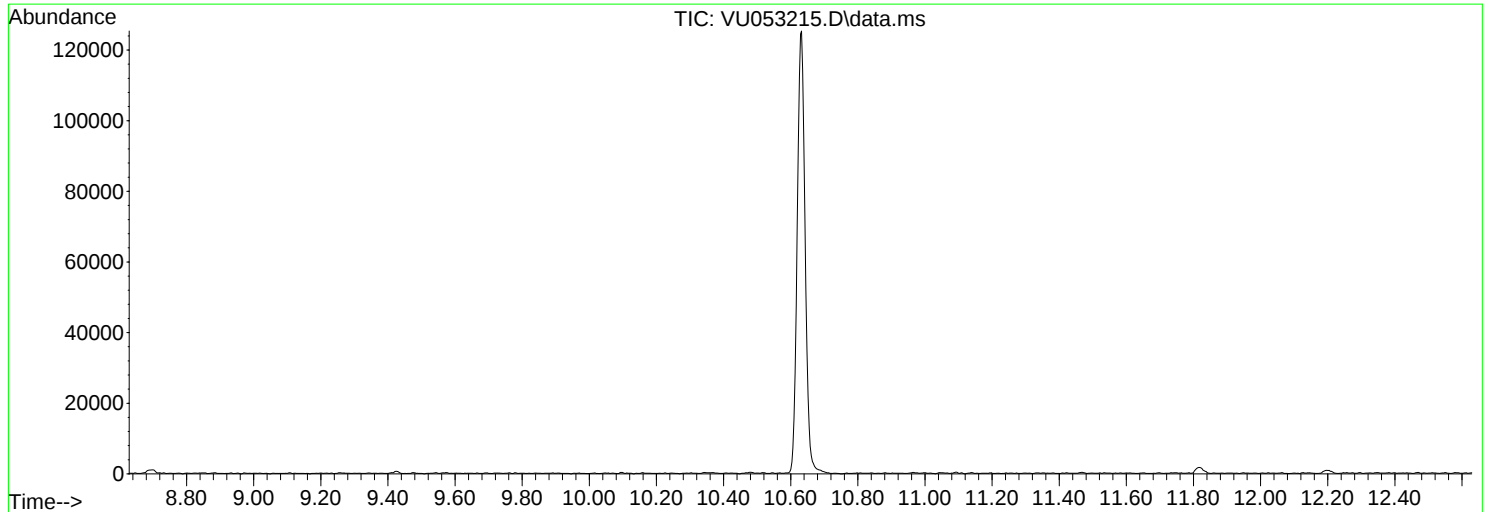

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2877

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.0	5245	PASS
75	95	30	80	54.7	14334	PASS
95	95	100	100	100.0	26213	PASS
96	95	5	9	7.0	1832	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	64.2	16821	PASS
175	174	5	9	6.9	1163	PASS
176	174	95	101	97.8	16449	PASS
177	176	5	9	6.1	1010	PASS

m/z	Abundance
40.00	120.0
44.00	147.0

Instrument :
MSVOA_U
ClientSampleId :
BFB164

m/z	Abundance
36.10	230.0
37.10	1195.0
38.10	1109.0
39.20	361.0
44.10	303.0
45.10	267.0
47.10	307.0
48.10	108.0
49.10	1111.0
50.10	4994.0
51.10	1614.0
55.10	133.0
56.10	378.0
57.10	747.0
60.00	220.0
61.10	1354.0
62.10	1117.0
63.10	1028.0
68.10	2512.0
69.10	2777.0
70.20	272.0
72.20	107.0
73.10	1132.0
74.10	4651.0
75.10	13281.0
76.10	1265.0
77.00	246.0
79.00	1097.0
80.00	225.0
81.00	1017.0
82.00	169.0
87.00	1326.0
88.10	1226.0
92.10	682.0
93.10	1049.0
94.10	2983.0
95.10	24640.0
96.10	1815.0
104.00	197.0
105.90	130.0
116.00	100.0
116.90	136.0
141.00	305.0
143.00	303.0
174.10	15390.0
175.10	1072.0
176.10	14852.0
177.10	911.0

Instrument :
MSVOA_U
ClientSampleId :
BFB164

m/z	Abundance
36.10	212.0
37.10	1335.0
38.10	1101.0
39.20	422.0
44.10	283.0
45.10	278.0
47.10	329.0
48.10	146.0
49.10	1236.0
50.10	5370.0
51.10	1724.0
55.10	153.0
56.10	446.0
57.10	757.0
60.10	288.0
61.10	1479.0
62.10	1279.0
63.10	1067.0
67.10	124.0
68.10	2675.0
69.10	3005.0
70.20	275.0
72.20	153.0
73.10	1303.0
74.10	4969.0
75.10	14808.0
76.10	1434.0
77.10	257.0
79.00	1190.0
80.00	257.0
81.00	1096.0
82.00	221.0
87.00	1278.0
88.10	1279.0
92.00	818.0
93.10	1129.0
94.10	3291.0
95.10	27032.0
96.10	1872.0
104.00	226.0
105.90	130.0
116.00	107.0
116.90	150.0
119.00	109.0
130.00	101.0
137.00	115.0
141.00	355.0
143.00	275.0
174.10	17376.0
175.10	1181.0
176.10	16960.0
177.10	1041.0

Instrument :
MSVOA_U
ClientSampleId :
BFB164

m/z	Abundance
36.10	181.0
37.10	1271.0
38.10	1051.0
39.10	467.0
44.00	290.0
45.10	222.0
47.10	311.0
48.20	179.0
49.10	1247.0
50.10	5372.0
51.10	1617.0
55.10	162.0
56.10	470.0
57.10	750.0
60.10	336.0
61.10	1442.0
62.10	1382.0
63.10	1027.0
67.10	129.0
68.10	2777.0
69.10	2932.0
70.10	268.0
72.10	157.0
73.10	1422.0
74.10	4884.0
75.20	14912.0
76.10	1449.0
77.10	196.0
78.00	122.0
79.00	1178.0
80.00	271.0
81.00	1098.0
82.00	258.0
87.10	1191.0
88.10	1155.0
91.00	109.0
92.00	855.0
93.10	1119.0
94.10	3345.0
95.10	26968.0
96.10	1808.0
104.00	180.0
105.90	127.0
116.90	149.0
119.00	153.0
130.00	106.0
137.00	127.0
141.00	332.0
143.00	250.0
174.10	17696.0
175.10	1237.0
176.10	17536.0
177.10	1079.0

Instrument :
MSVOA_U
ClientSampleId :
BFB164