

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031719\
 Data File : VU030135.D
 Acq On : 16 Mar 2019 11:20
 Operator : JC/SP
 Sample : VU0317WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK35

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	40	rVB	10572	10281	0.57%	0.072%
2	1.399	89	96	106	rBV	271027	266699	14.83%	1.857%
3	1.678	175	183	204	rBV	194034	251284	13.97%	1.750%
4	2.273	356	368	382	rBV	420361	648288	36.05%	4.514%
5	2.473	427	430	435	rBV3	1525	1667	0.09%	0.012%
6	2.537	447	450	453	rVB	1814	1240	0.07%	0.009%
7	2.559	453	457	459	rBV	1530	1150	0.06%	0.008%
8	2.614	471	474	477	rBV2	990	843	0.05%	0.006%
9	2.707	496	503	506	rVB4	1580	2079	0.12%	0.014%
10	2.727	506	509	513	rBV2	1229	883	0.05%	0.006%
11	2.765	518	521	526	rBV	1204	1236	0.07%	0.009%
12	2.836	540	543	547	rBV	896	827	0.05%	0.006%
13	2.958	577	581	585	rBV3	953	918	0.05%	0.006%
14	3.209	655	659	663	rBV3	749	654	0.04%	0.005%
15	3.254	668	673	679	rBV2	1144	1698	0.09%	0.012%
16	3.286	680	683	686	rBV	1000	728	0.04%	0.005%
17	3.521	752	756	759	rBV	953	802	0.04%	0.006%
18	3.784	836	838	843	rVB	1629	1212	0.07%	0.008%
19	3.823	845	850	853	rBV	1129	1195	0.07%	0.008%
20	3.958	889	892	894	rBV	727	538	0.03%	0.004%
21	4.087	929	932	935	rBV	1370	800	0.04%	0.006%
22	4.106	935	938	941	rVB	1022	648	0.04%	0.005%
23	4.173	946	959	986	rBV	164579	428722	23.84%	2.985%
24	4.646	1090	1106	1132	rBV	292240	695151	38.65%	4.841%
25	4.990	1208	1213	1216	rBV3	914	828	0.05%	0.006%
26	5.125	1248	1255	1257	rBV3	762	865	0.05%	0.006%
27	5.161	1261	1266	1268	rBV2	926	850	0.05%	0.006%
28	5.196	1273	1277	1280	rBV2	781	758	0.04%	0.005%
29	5.254	1293	1295	1298	rVB	1124	612	0.03%	0.004%
30	5.337	1298	1321	1347	rBV2	615873	1798463	100.00%	12.523%
31	5.591	1397	1400	1403	rBV2	963	830	0.05%	0.006%
32	5.659	1416	1421	1424	rBV2	1246	1253	0.07%	0.009%
33	5.701	1431	1434	1436	rBV	1191	884	0.05%	0.006%
34	5.762	1450	1453	1455	rBV	897	550	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031719\
 Data File : VU030135.D
 Acq On : 16 Mar 2019 11:20
 Operator : JC/SP
 Sample : VU0317WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK35

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

35	5.788	1458	1461	1464	rVB2	920	594	0.03%	0.004%
36	5.884	1477	1491	1528	rBV	575030	1161431	64.58%	8.087%
37	6.090	1550	1555	1560	rBV4	938	1164	0.06%	0.008%
38	6.180	1573	1583	1586	rBV6	2903	4565	0.25%	0.032%
39	6.247	1602	1604	1608	rVB2	957	633	0.04%	0.004%
40	6.273	1608	1612	1614	rBV	1788	1316	0.07%	0.009%
41	6.328	1614	1629	1650	rBV	392646	793577	44.13%	5.526%
42	6.505	1682	1684	1696	rVB4	1542	1860	0.10%	0.013%
43	6.582	1704	1708	1711	rVB	1058	817	0.05%	0.006%
44	6.604	1713	1715	1719	rVB	1595	899	0.05%	0.006%
45	6.640	1723	1726	1728	rBV3	1061	725	0.04%	0.005%
46	6.691	1739	1742	1745	rBV	1407	934	0.05%	0.007%
47	6.832	1782	1786	1789	rBV2	874	624	0.03%	0.004%
48	6.874	1793	1799	1803	rBV3	1151	1247	0.07%	0.009%
49	6.961	1822	1826	1829	rBV3	1283	1123	0.06%	0.008%
50	6.977	1829	1831	1835	rVV2	714	542	0.03%	0.004%
51	7.080	1857	1863	1866	rBV	1115	1155	0.06%	0.008%
52	7.183	1891	1895	1897	rBV	1047	805	0.04%	0.006%
53	7.225	1897	1908	1928	rVV	203000	372692	20.72%	2.595%
54	7.424	1966	1970	1973	rBV2	1292	1050	0.06%	0.007%
55	7.469	1980	1984	1988	rBV2	1662	1557	0.09%	0.011%
56	7.562	1998	2013	2036	rBV	832267	1463993	81.40%	10.194%
57	7.849	2092	2102	2124	rBV	138938	242983	13.51%	1.692%
58	8.177	2193	2204	2215	rVB2	11817	22066	1.23%	0.154%
59	8.225	2216	2219	2220	rBV3	1377	822	0.05%	0.006%
60	8.308	2230	2245	2278	rBV	574934	1016841	56.54%	7.081%
61	8.829	2404	2407	2409	rBV2	829	589	0.03%	0.004%
62	8.881	2420	2423	2428	rVB	821	612	0.03%	0.004%
63	8.932	2435	2439	2440	rBV2	948	729	0.04%	0.005%
64	8.984	2452	2455	2458	rBV	857	648	0.04%	0.005%
65	9.003	2458	2461	2465	rVB	1050	753	0.04%	0.005%
66	9.032	2465	2470	2474	rVB	1183	1151	0.06%	0.008%
67	9.086	2474	2487	2514	rBV	856975	1434949	79.79%	9.992%
68	9.369	2570	2575	2577	rBV	1485	1568	0.09%	0.011%
69	9.582	2636	2641	2645	rVB2	1306	1451	0.08%	0.010%
70	9.607	2645	2649	2650	rBV	1098	784	0.04%	0.005%
71	9.620	2650	2653	2656	rBV	1231	878	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031719\
 Data File : VU030135.D
 Acq On : 16 Mar 2019 11:20
 Operator : JC/SP
 Sample : VU0317WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK35

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

72	9.762	2694	2697	2700	rBV	885	758	0.04%	0.005%
73	9.839	2718	2721	2724	rBV2	946	610	0.03%	0.004%
74	9.932	2746	2750	2755	rBV2	1495	1782	0.10%	0.012%
75	10.099	2798	2802	2808	rBV	1081	1436	0.08%	0.010%
76	10.138	2808	2814	2816	rVB2	1406	1273	0.07%	0.009%
77	10.154	2816	2819	2822	rBV2	1025	799	0.04%	0.006%
78	10.373	2882	2887	2891	rBV2	955	969	0.05%	0.007%
79	10.427	2892	2904	2920	rBV	596475	958845	53.31%	6.677%
80	10.601	2955	2958	2959	rBV2	1276	799	0.04%	0.006%
81	10.733	2997	2999	3004	rVB2	899	802	0.04%	0.006%
82	11.012	3082	3086	3087	rBV	1061	760	0.04%	0.005%
83	11.054	3096	3099	3103	rBV	853	704	0.04%	0.005%
84	11.115	3116	3118	3123	rBV	1242	1160	0.06%	0.008%
85	11.347	3187	3190	3192	rBV2	940	612	0.03%	0.004%
86	11.418	3208	3212	3220	rBV5	2290	2980	0.17%	0.021%
87	11.482	3220	3232	3252	rBV	848319	1356640	75.43%	9.447%
88	11.697	3296	3299	3311	rVB	2401	4184	0.23%	0.029%
89	11.742	3311	3313	3315	rBV2	984	583	0.03%	0.004%
90	11.858	3336	3349	3370	rBV	813113	1346188	74.85%	9.374%
91	12.112	3425	3428	3433	rBV2	1150	1123	0.06%	0.008%
92	12.376	3507	3510	3513	rBV	1448	889	0.05%	0.006%
93	12.636	3588	3591	3592	rBV	976	574	0.03%	0.004%
94	12.897	3667	3672	3678	rBV3	2669	3334	0.19%	0.023%
95	13.028	3710	3713	3716	rBV	1283	874	0.05%	0.006%
96	13.170	3754	3757	3763	rBV2	1127	1199	0.07%	0.008%
97	14.154	4060	4063	4064	rBV	1253	799	0.04%	0.006%
98	14.167	4064	4067	4074	rVB	2000	2048	0.11%	0.014%
99	14.228	4083	4086	4090	rBV	1479	1323	0.07%	0.009%
100	15.122	4361	4364	4368	rBV2	1412	1281	0.07%	0.009%


Sum of corrected areas: 14360891

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU031719\
Data File : VU030135.D
Acq On : 16 Mar 2019 11:20
Operator : JC/SP
Sample : VU0317WBL01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK35

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

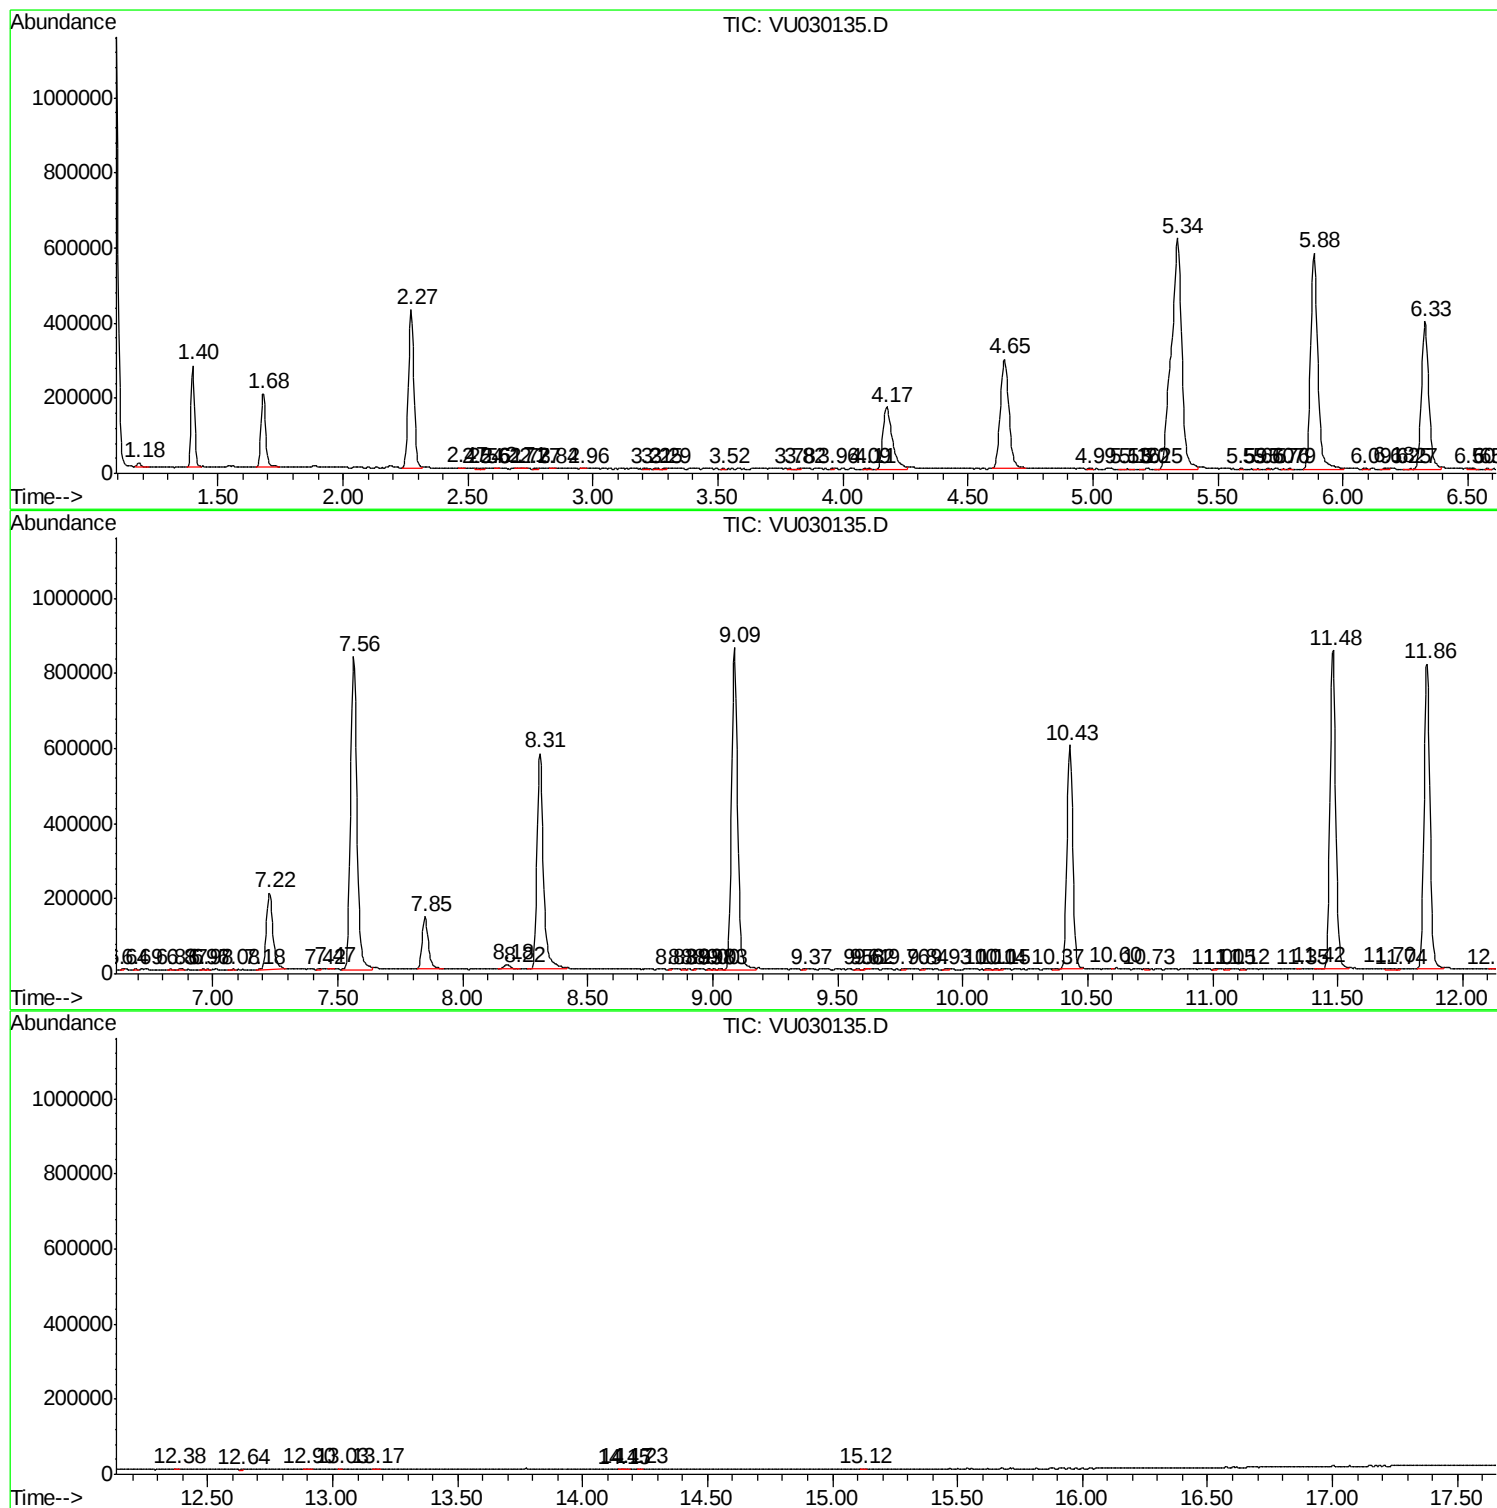

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031719\
Data File : VU030135.D
Acq On : 16 Mar 2019 11:20
Operator : JC/SP
Sample : VU0317WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK35

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031719\
Data File : VU030135.D
Acq On : 16 Mar 2019 11:20
Operator : JC/SP
Sample : VU0317WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK35

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc