

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031719\
 Data File : VU030138.D
 Acq On : 16 Mar 2019 12:33
 Operator : JC/SP
 Sample : K1936-22
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	38	rVB2	10687	10718	0.68%	0.082%
2	1.399	88	96	111	rBV	249686	252611	16.08%	1.941%
3	1.682	175	184	198	rBV	174228	221420	14.09%	1.701%
4	2.151	327	330	334	rBV	1875	1539	0.10%	0.012%
5	2.273	356	368	382	rBV	383863	589041	37.49%	4.526%
6	2.379	397	401	406	rVB	1827	1454	0.09%	0.011%
7	2.473	428	430	433	rVB2	1588	865	0.06%	0.007%
8	2.495	433	437	440	rBV	1987	1898	0.12%	0.015%
9	2.746	512	515	520	rBV2	1407	1555	0.10%	0.012%
10	2.952	574	579	581	rBV2	1263	1337	0.09%	0.010%
11	3.003	590	595	599	rBV	1162	1289	0.08%	0.010%
12	3.164	638	645	648	rBV2	1725	2345	0.15%	0.018%
13	3.321	692	694	700	rVB	1474	1503	0.10%	0.012%
14	3.485	740	745	747	rBV2	805	885	0.06%	0.007%
15	3.537	756	761	763	rBV	1235	1231	0.08%	0.009%
16	3.566	767	770	773	rBV	1247	998	0.06%	0.008%
17	3.675	801	804	810	rVB	1257	887	0.06%	0.007%
18	3.823	844	850	854	rBV	1256	1688	0.11%	0.013%
19	3.881	862	868	870	rBV	1318	1196	0.08%	0.009%
20	4.010	903	908	911	rBV	1172	1238	0.08%	0.010%
21	4.026	911	913	920	rVV	1467	1330	0.08%	0.010%
22	4.103	935	937	943	rVB	1353	1318	0.08%	0.010%
23	4.174	948	959	985	rBV	137937	363387	23.13%	2.792%
24	4.534	1067	1071	1073	rBV2	1408	1201	0.08%	0.009%
25	4.646	1089	1106	1126	rBV2	260175	615320	39.16%	4.728%
26	4.862	1169	1173	1174	rBV2	1448	891	0.06%	0.007%
27	4.878	1175	1178	1184	rVV	2632	2889	0.18%	0.022%
28	4.903	1184	1186	1190	rVB	1990	1171	0.07%	0.009%
29	4.929	1190	1194	1201	rBV	1097	1616	0.10%	0.012%
30	4.997	1212	1215	1222	rVB	1695	1936	0.12%	0.015%
31	5.032	1222	1226	1230	rVB	1345	1025	0.07%	0.008%
32	5.138	1256	1259	1262	rBV	1449	1306	0.08%	0.010%
33	5.206	1275	1280	1283	rBV	1374	1377	0.09%	0.011%
34	5.337	1299	1321	1345	rBV2	541525	1571288	100.00%	12.074%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031719\
 Data File : VU030138.D
 Acq On : 16 Mar 2019 12:33
 Operator : JC/SP
 Sample : K1936-22
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

35	5.559	1387	1390	1394	rVB	1646	1106	0.07%	0.008%
36	5.582	1394	1397	1400	rBV	1431	985	0.06%	0.008%
37	5.643	1413	1416	1424	rBV2	1277	1632	0.10%	0.013%
38	5.691	1428	1431	1435	rVB2	1466	955	0.06%	0.007%
39	5.714	1435	1438	1441	rVB2	1347	926	0.06%	0.007%
40	5.884	1475	1491	1525	rBV	553336	1130139	71.92%	8.684%
41	6.231	1597	1599	1606	rVB	1076	955	0.06%	0.007%
42	6.283	1611	1615	1616	rBV	1520	1072	0.07%	0.008%
43	6.328	1616	1629	1650	rBV	332323	675536	42.99%	5.191%
44	6.559	1698	1701	1706	rVB	1464	1141	0.07%	0.009%
45	6.588	1706	1710	1714	rBV	1050	1188	0.08%	0.009%
46	6.794	1770	1774	1780	rBV	1466	2016	0.13%	0.015%
47	6.945	1818	1821	1824	rVB	1730	1078	0.07%	0.008%
48	6.964	1824	1827	1831	rBV	1241	1013	0.06%	0.008%
49	7.045	1849	1852	1855	rBV	1920	1312	0.08%	0.010%
50	7.225	1897	1908	1932	rBV	191205	361834	23.03%	2.780%
51	7.472	1981	1985	1989	rBV2	2662	3037	0.19%	0.023%
52	7.562	2000	2013	2037	rBV	732883	1308058	83.25%	10.051%
53	7.849	2091	2102	2123	rVV	132515	237236	15.10%	1.823%
54	7.977	2139	2142	2147	rBV	1538	1402	0.09%	0.011%
55	8.122	2183	2187	2191	rBV2	2275	2325	0.15%	0.018%
56	8.177	2196	2204	2215	rVV3	9973	17870	1.14%	0.137%
57	8.228	2215	2220	2226	rBV2	1958	2865	0.18%	0.022%
58	8.308	2234	2245	2272	rBV	485157	860073	54.74%	6.609%
59	8.588	2326	2332	2335	rVB	1423	1310	0.08%	0.010%
60	8.627	2341	2344	2350	rBV2	1391	1095	0.07%	0.008%
61	8.701	2363	2367	2369	rBV	1271	917	0.06%	0.007%
62	8.861	2413	2417	2421	rBV	919	867	0.06%	0.007%
63	8.890	2421	2426	2430	rVB	1271	1150	0.07%	0.009%
64	8.942	2439	2442	2444	rBV	1445	1125	0.07%	0.009%
65	9.000	2455	2460	2463	rBV	1980	1714	0.11%	0.013%
66	9.042	2470	2473	2475	rBV	1690	867	0.06%	0.007%
67	9.087	2475	2487	2514	rVV	833413	1379806	87.81%	10.602%
68	9.415	2586	2589	2593	rVB	2398	1671	0.11%	0.013%
69	9.511	2615	2619	2623	rBV	1272	1165	0.07%	0.009%
70	9.537	2623	2627	2629	rBV	1550	1055	0.07%	0.008%
71	9.582	2634	2641	2644	rBV	1632	2290	0.15%	0.018%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031719\
 Data File : VU030138.D
 Acq On : 16 Mar 2019 12:33
 Operator : JC/SP
 Sample : K1936-22
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

72	9.630	2652	2656	2660	rBV	1238	1206	0.08%	0.009%
73	9.694	2672	2676	2681	rVB	1381	1073	0.07%	0.008%
74	9.984	2761	2766	2769	rBV	1524	1285	0.08%	0.010%
75	10.019	2773	2777	2779	rBV	1345	993	0.06%	0.008%
76	10.080	2793	2796	2801	rVB	1516	1150	0.07%	0.009%
77	10.125	2806	2810	2817	rVV2	1562	1884	0.12%	0.014%
78	10.389	2884	2892	2893	rBV	1528	1577	0.10%	0.012%
79	10.427	2893	2904	2926	rVB	510763	828394	52.72%	6.365%
80	10.604	2953	2959	2964	rBV5	3052	3695	0.24%	0.028%
81	10.797	3016	3019	3022	rVB	2243	1375	0.09%	0.011%
82	10.816	3022	3025	3028	rBV	1376	1198	0.08%	0.009%
83	10.887	3044	3047	3052	rVV	1426	1072	0.07%	0.008%
84	10.926	3056	3059	3064	rVB	1506	1124	0.07%	0.009%
85	11.064	3099	3102	3106	rVB	1295	908	0.06%	0.007%
86	11.086	3106	3109	3112	rBV	1108	1023	0.07%	0.008%
87	11.189	3139	3141	3149	rVB	947	1002	0.06%	0.008%
88	11.385	3198	3202	3203	rBV2	1294	874	0.06%	0.007%
89	11.482	3220	3232	3260	rBV	824689	1308131	83.25%	10.052%
90	11.720	3301	3306	3309	rBV	1489	1317	0.08%	0.010%
91	11.858	3337	3349	3377	rBV	708588	1168185	74.35%	8.976%
92	12.215	3457	3460	3463	rBV2	1833	1418	0.09%	0.011%
93	12.691	3604	3608	3615	rBV	1844	2068	0.13%	0.016%
94	13.006	3701	3706	3709	rBV2	1856	1650	0.11%	0.013%
95	13.771	3936	3944	3946	rBV2	1547	2156	0.14%	0.017%
96	14.151	4058	4062	4065	rBV2	1932	1898	0.12%	0.015%
97	14.620	4205	4208	4212	rVB	2487	1596	0.10%	0.012%
98	14.755	4246	4250	4251	rBV	1439	1032	0.07%	0.008%
99	15.479	4473	4475	4480	rVB2	1506	937	0.06%	0.007%
100	15.527	4486	4490	4493	rBV3	1614	1478	0.09%	0.011%


Sum of corrected areas: 13014238

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU031719\
Data File : VU030138.D
Acq On : 16 Mar 2019 12:33
Operator : JC/SP
Sample : K1936-22
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

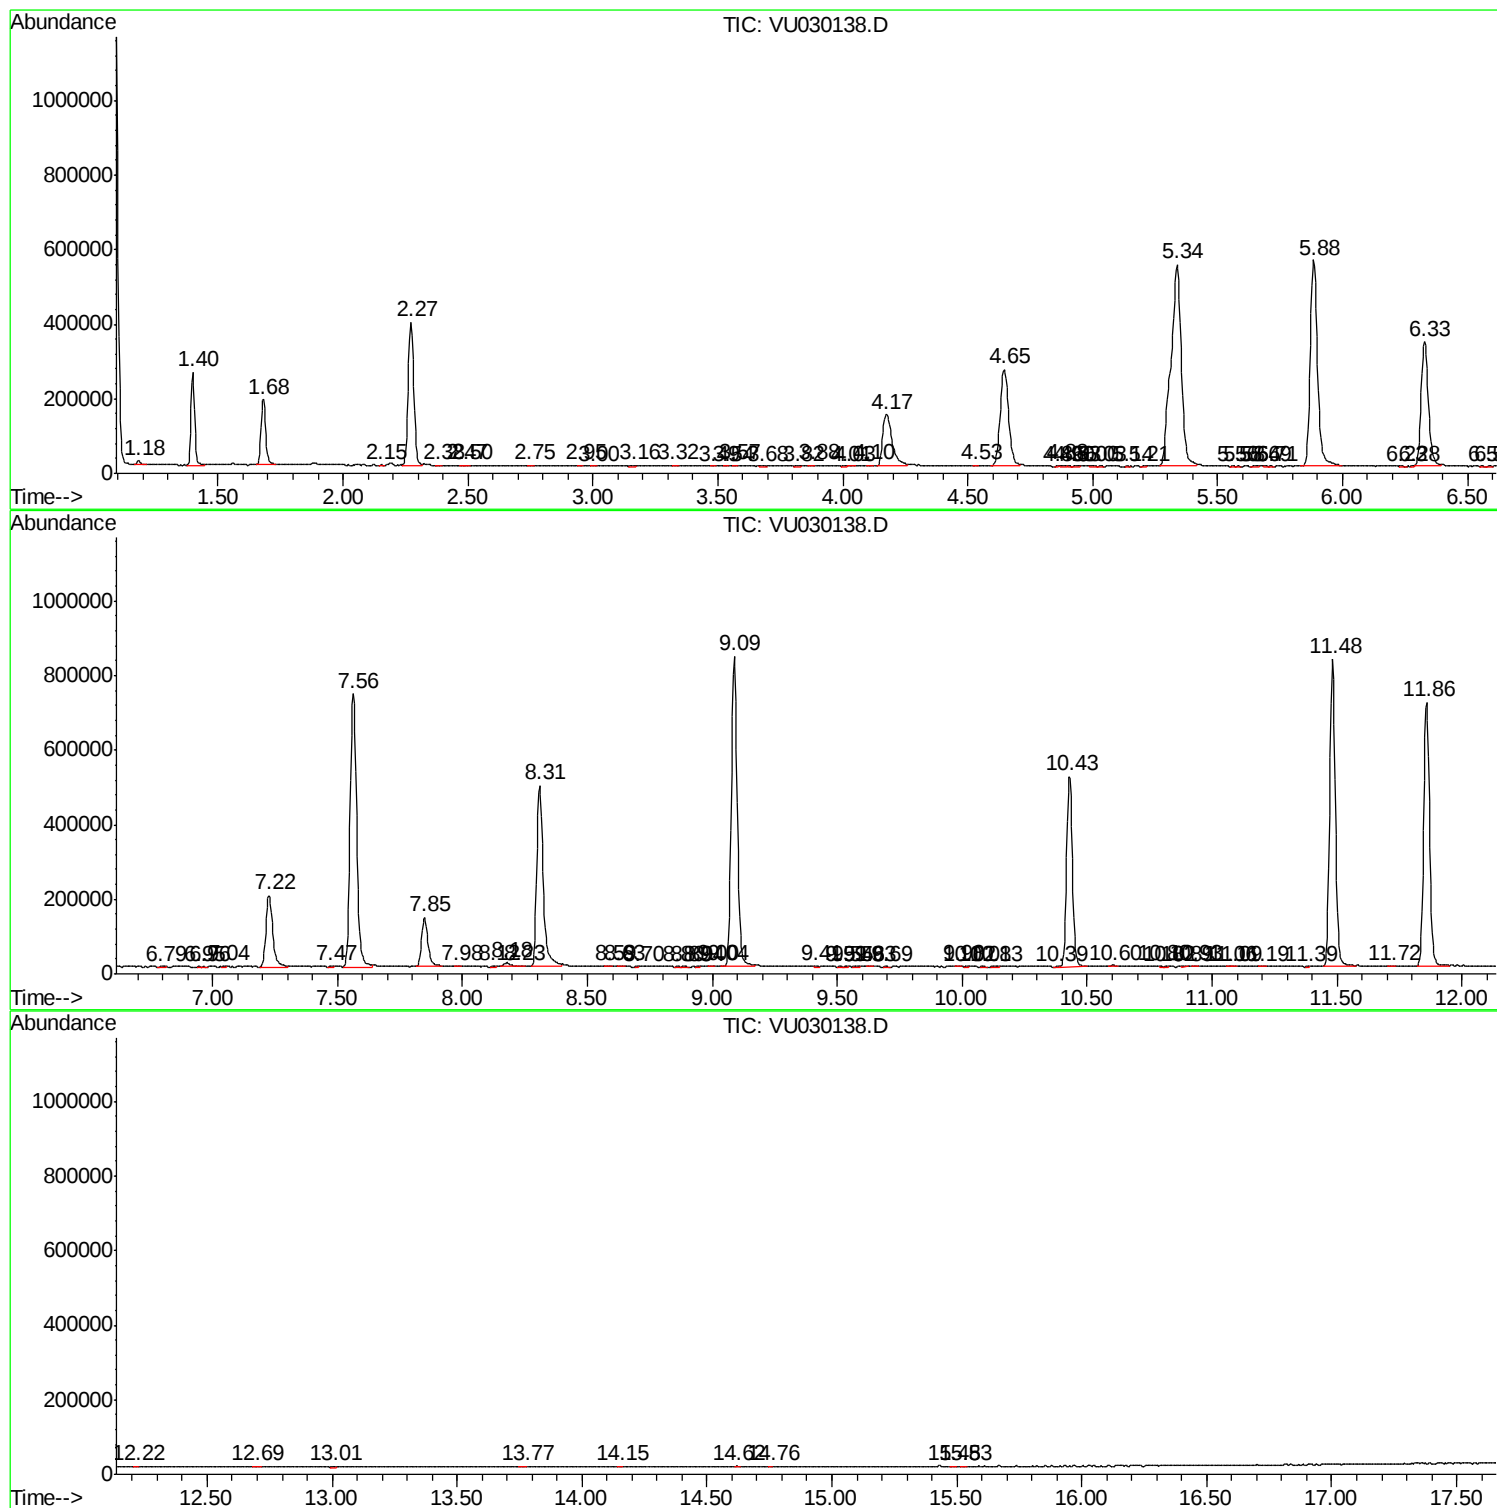

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031719\
Data File : VU030138.D
Acq On : 16 Mar 2019 12:33
Operator : JC/SP
Sample : K1936-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031719\
Data File : VU030138.D
Acq On : 16 Mar 2019 12:33
Operator : JC/SP
Sample : K1936-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK02

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc