

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031719\
 Data File : VU030142.D
 Acq On : 16 Mar 2019 14:04
 Operator : JC/SP
 Sample : K1949-15 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1B4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	35	rBV	11383	10633	0.10%	0.044%
2	1.399	89	96	108	rBV	237572	235230	2.28%	0.980%
3	1.678	175	183	202	rVB	179092	226869	2.20%	0.945%
4	2.270	357	367	384	rBV	384602	589679	5.71%	2.456%
5	2.556	453	456	460	rBV	1046	828	0.01%	0.003%
6	2.813	534	536	540	rVB	1292	790	0.01%	0.003%
7	3.061	610	613	615	rBV	957	765	0.01%	0.003%
8	3.096	621	624	629	rBV	1470	1219	0.01%	0.005%
9	3.177	646	649	652	rVB	1388	899	0.01%	0.004%
10	3.434	726	729	731	rBV	1752	1250	0.01%	0.005%
11	3.608	779	783	786	rBV	1294	1337	0.01%	0.006%
12	3.746	823	826	829	rBV	888	720	0.01%	0.003%
13	3.865	860	863	867	rBV	1102	1002	0.01%	0.004%
14	4.132	941	946	948	rBV	1776	1717	0.02%	0.007%
15	4.173	948	959	995	rVV	168368	489296	4.74%	2.038%
16	4.534	1067	1071	1074	rBV2	1664	1208	0.01%	0.005%
17	4.646	1084	1106	1125	rBV	282420	672456	6.51%	2.800%
18	4.865	1171	1174	1178	rBV3	1199	872	0.01%	0.004%
19	4.894	1178	1183	1187	rVV3	1138	1294	0.01%	0.005%
20	4.980	1206	1210	1212	rBV	1086	863	0.01%	0.004%
21	5.048	1224	1231	1238	rVB	1582	1896	0.02%	0.008%
22	5.083	1238	1242	1245	rBV2	687	712	0.01%	0.003%
23	5.228	1282	1287	1292	rVV	2174	2474	0.02%	0.010%
24	5.251	1292	1294	1298	rVV	1109	880	0.01%	0.004%
25	5.337	1298	1321	1358	rVV2	571596	1695872	16.41%	7.062%
26	5.489	1364	1368	1373	rVB	2237	1786	0.02%	0.007%
27	5.694	1428	1432	1435	rVB	759	671	0.01%	0.003%
28	5.771	1453	1456	1461	rVB	1479	1264	0.01%	0.005%
29	5.797	1461	1464	1467	rBV	929	605	0.01%	0.003%
30	5.884	1477	1491	1527	rBV	502898	1026132	9.93%	4.273%
31	6.067	1546	1548	1553	rVB	1167	962	0.01%	0.004%
32	6.160	1573	1577	1578	rBV	1042	642	0.01%	0.003%
33	6.193	1578	1587	1596	rVB6	9412	18391	0.18%	0.077%
34	6.328	1614	1629	1653	rBV	367352	759047	7.35%	3.161%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031719\
 Data File : VU030142.D
 Acq On : 16 Mar 2019 14:04
 Operator : JC/SP
 Sample : K1949-15 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1B4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

35	6.453	1666	1668	1671	rBV3	981	728	0.01%	0.003%
36	6.505	1681	1684	1687	rBV	1051	682	0.01%	0.003%
37	6.595	1708	1712	1716	rVB	1142	644	0.01%	0.003%
38	6.771	1764	1767	1772	rVB2	805	661	0.01%	0.003%
39	6.797	1772	1775	1778	rBV	1230	851	0.01%	0.004%
40	6.887	1798	1803	1808	rVB3	1999	2468	0.02%	0.010%
41	7.016	1840	1843	1847	rBV	1177	963	0.01%	0.004%
42	7.141	1880	1882	1886	rVB	1287	847	0.01%	0.004%
43	7.170	1886	1891	1894	rVB	878	750	0.01%	0.003%
44	7.225	1894	1908	1928	rBV	206954	381695	3.69%	1.589%
45	7.334	1939	1942	1946	rVB	1395	933	0.01%	0.004%
46	7.353	1946	1948	1950	rBV	1424	753	0.01%	0.003%
47	7.389	1956	1959	1962	rBV2	1070	835	0.01%	0.003%
48	7.472	1980	1985	1988	rBV2	994	887	0.01%	0.004%
49	7.562	2000	2013	2034	rVV	760604	1348555	13.05%	5.616%
50	7.849	2091	2102	2122	rBV	144079	258365	2.50%	1.076%
51	7.996	2143	2148	2152	rBV	2144	2672	0.03%	0.011%
52	8.061	2165	2168	2172	rBV2	1502	1439	0.01%	0.006%
53	8.115	2181	2185	2191	rVB2	1815	1795	0.02%	0.007%
54	8.225	2191	2219	2236	rBV	6042975	10332642	100.00%	43.027%
55	8.308	2236	2245	2283	rVB	590024	1110313	10.75%	4.624%
56	8.521	2308	2311	2314	rBV2	1603	1114	0.01%	0.005%
57	8.659	2352	2354	2357	rBV	1316	852	0.01%	0.004%
58	8.694	2363	2365	2368	rBV2	1046	773	0.01%	0.003%
59	8.771	2385	2389	2395	rBV	1265	1497	0.01%	0.006%
60	8.951	2442	2445	2450	rBV2	1757	1487	0.01%	0.006%
61	8.990	2452	2457	2460	rBV2	1718	1453	0.01%	0.006%
62	9.086	2474	2487	2510	rBV	764257	1277439	12.36%	5.320%
63	9.360	2567	2572	2575	rBV	1867	2223	0.02%	0.009%
64	9.385	2578	2580	2586	rVB2	2598	1874	0.02%	0.008%
65	9.443	2594	2598	2603	rBV3	1657	1629	0.02%	0.007%
66	9.469	2603	2606	2609	rVB	1606	880	0.01%	0.004%
67	9.495	2609	2614	2618	rVB	777	732	0.01%	0.003%
68	9.678	2668	2671	2674	rBV	1400	962	0.01%	0.004%
69	9.697	2674	2677	2679	rBV	1257	906	0.01%	0.004%
70	9.746	2684	2692	2695	rBV	1597	2554	0.02%	0.011%
71	10.012	2771	2775	2779	rBV	1872	1549	0.01%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031719\
 Data File : VU030142.D
 Acq On : 16 Mar 2019 14:04
 Operator : JC/SP
 Sample : K1949-15 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1B4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

72	10.154	2816	2819	2822	rBV	1451	1113	0.01%	0.005%
73	10.266	2851	2854	2860	rBV	1387	1744	0.02%	0.007%
74	10.334	2869	2875	2879	rVB	2101	2242	0.02%	0.009%
75	10.427	2893	2904	2922	rBV	584296	942720	9.12%	3.926%
76	10.604	2950	2959	2973	rVB3	14960	26640	0.26%	0.111%
77	10.684	2980	2984	2989	rBV	2048	2110	0.02%	0.009%
78	10.987	3075	3078	3081	rBV	925	664	0.01%	0.003%
79	11.080	3104	3107	3113	rVB	2222	2317	0.02%	0.010%
80	11.109	3113	3116	3119	rBV	1500	1410	0.01%	0.006%
81	11.183	3135	3139	3145	rVB	2629	2971	0.03%	0.012%
82	11.225	3145	3152	3154	rBV2	1442	1780	0.02%	0.007%
83	11.292	3164	3173	3175	rBV2	1299	1741	0.02%	0.007%
84	11.414	3204	3211	3213	rBV4	1987	2474	0.02%	0.010%
85	11.482	3219	3232	3254	rBV	747342	1232727	11.93%	5.133%
86	11.691	3290	3297	3302	rBV2	1728	2267	0.02%	0.009%
87	11.858	3337	3349	3377	rBV	762983	1270806	12.30%	5.292%
88	12.475	3537	3541	3551	rVB	6171	8276	0.08%	0.034%
89	12.594	3575	3578	3581	rBV	935	833	0.01%	0.003%
90	12.726	3616	3619	3622	rVB2	1556	990	0.01%	0.004%
91	12.752	3622	3627	3629	rBV	1048	1055	0.01%	0.004%
92	12.897	3669	3672	3679	rBV2	1672	1720	0.02%	0.007%
93	13.138	3744	3747	3750	rVB	1464	919	0.01%	0.004%
94	13.160	3750	3754	3756	rBV2	1055	895	0.01%	0.004%
95	13.196	3762	3765	3767	rBV2	1161	801	0.01%	0.003%
96	13.398	3823	3828	3830	rBV2	1300	1354	0.01%	0.006%
97	13.434	3836	3839	3842	rBV	1941	1483	0.01%	0.006%
98	13.533	3866	3870	3871	rBV	1119	820	0.01%	0.003%
99	13.922	3988	3991	3993	rBV	1032	643	0.01%	0.003%
100	14.655	4216	4219	4221	rBV	1477	987	0.01%	0.004%


Sum of corrected areas: 24014165

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU031719\
Data File : VU030142.D
Acq On : 16 Mar 2019 14:04
Operator : JC/SP
Sample : K1949-15 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1B4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

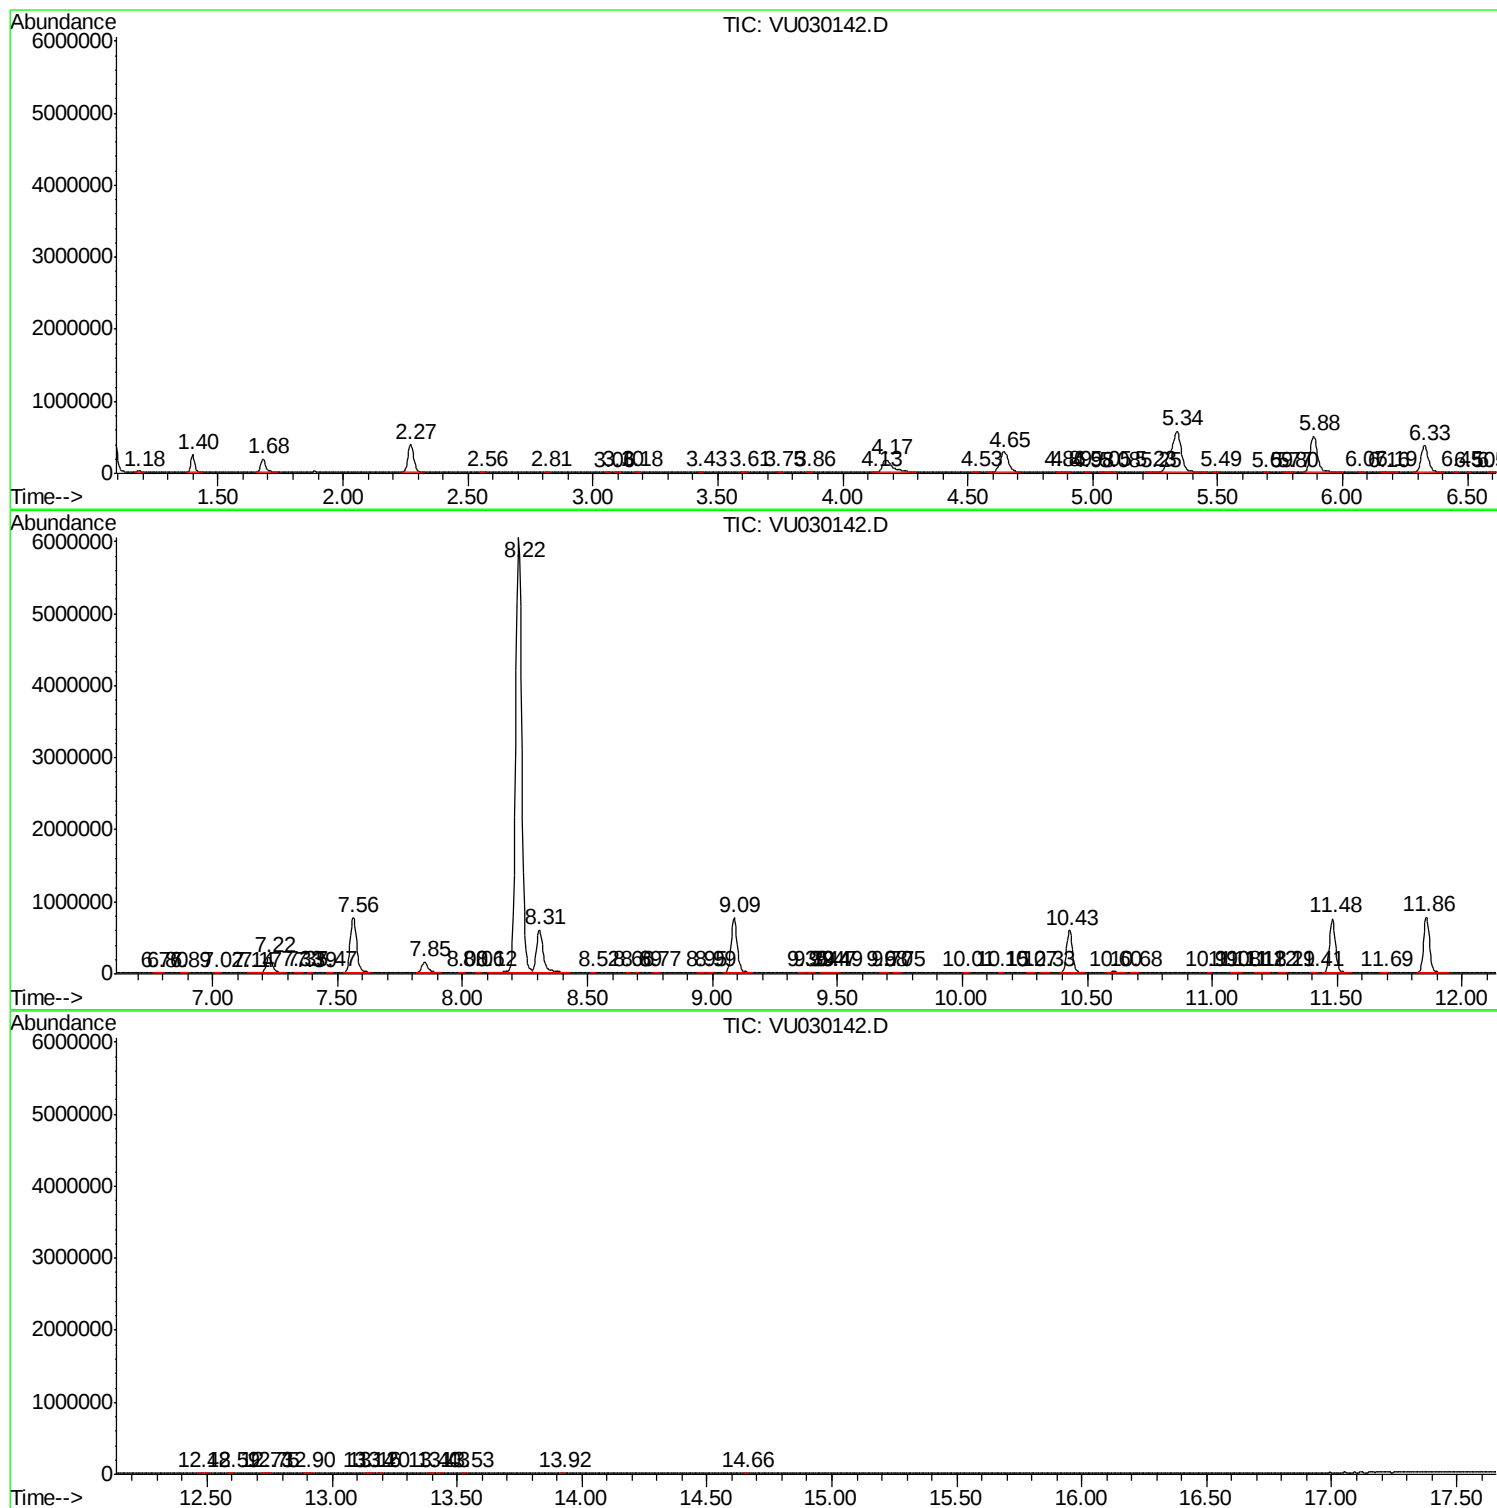

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031719\
Data File : VU030142.D
Acq On : 16 Mar 2019 14:04
Operator : JC/SP
Sample : K1949-15 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1B4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031719\
Data File : VU030142.D
Acq On : 16 Mar 2019 14:04
Operator : JC/SP
Sample : K1949-15 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1B4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc