

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031719\
 Data File : VU030145.D
 Acq On : 16 Mar 2019 15:13
 Operator : JC/SP
 Sample : K1949-19 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1H1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	36	rVB2	9920	8962	0.08%	0.036%
2	1.399	89	96	111	rVB	236482	235279	2.15%	0.953%
3	1.678	175	183	200	rBV	175449	227182	2.08%	0.920%
4	2.270	356	367	380	rBV	377940	584014	5.34%	2.366%
5	2.444	414	421	429	rBV	2807	4428	0.04%	0.018%
6	2.518	440	444	446	rBV	1376	1112	0.01%	0.005%
7	3.112	624	629	632	rBV2	1307	1427	0.01%	0.006%
8	3.257	669	674	678	rBV	1496	1604	0.01%	0.006%
9	4.173	947	959	990	rBV	178629	509070	4.66%	2.062%
10	4.575	1080	1084	1088	rBV	1903	2131	0.02%	0.009%
11	4.646	1088	1106	1128	rVV	281310	669741	6.13%	2.713%
12	4.948	1196	1200	1202	rBV	1257	1094	0.01%	0.004%
13	5.058	1230	1234	1241	rVB	1229	1523	0.01%	0.006%
14	5.209	1277	1281	1286	rBV	1143	1170	0.01%	0.005%
15	5.337	1299	1321	1344	rVV2	565405	1664571	15.22%	6.743%
16	5.759	1448	1452	1457	rBV2	1538	1582	0.01%	0.006%
17	5.884	1477	1491	1517	rBV	507787	1031344	9.43%	4.178%
18	6.186	1575	1585	1600	rBV5	10393	23779	0.22%	0.096%
19	6.328	1615	1629	1648	rBV	374559	750750	6.87%	3.041%
20	6.585	1706	1709	1715	rVB	1340	1028	0.01%	0.004%
21	6.672	1731	1736	1743	rBV	2238	2519	0.02%	0.010%
22	6.759	1756	1763	1768	rVB2	2259	2623	0.02%	0.011%
23	6.810	1768	1779	1783	rBV	1939	3795	0.03%	0.015%
24	6.923	1812	1814	1821	rVB	1933	1721	0.02%	0.007%
25	7.109	1867	1872	1881	rVB	2394	3569	0.03%	0.014%
26	7.170	1887	1891	1893	rBV	1421	1196	0.01%	0.005%
27	7.225	1897	1908	1932	rVV	203065	373764	3.42%	1.514%
28	7.341	1941	1944	1949	rVB2	1584	1352	0.01%	0.005%
29	7.389	1955	1959	1961	rBV3	1468	1153	0.01%	0.005%
30	7.562	2000	2013	2035	rBV	764687	1353811	12.38%	5.484%
31	7.752	2069	2072	2080	rVB2	1668	2001	0.02%	0.008%
32	7.800	2080	2087	2090	rBV	1304	1361	0.01%	0.006%
33	7.849	2090	2102	2122	rBV	144493	255858	2.34%	1.036%
34	8.225	2186	2219	2236	rBV	6467832	10933870	100.00%	44.292%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031719\
 Data File : VU030145.D
 Acq On : 16 Mar 2019 15:13
 Operator : JC/SP
 Sample : K1949-19 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1H1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

35	8.308	2236	2245	2278	rVB	622629	1144182	10.46%	4.635%
36	8.717	2368	2372	2376	rBV	1662	1248	0.01%	0.005%
37	8.746	2376	2381	2386	rBV	1438	1399	0.01%	0.006%
38	8.855	2411	2415	2418	rBV	1681	1340	0.01%	0.005%
39	8.894	2421	2427	2429	rBV	1210	1214	0.01%	0.005%
40	8.987	2451	2456	2459	rBV	1139	1265	0.01%	0.005%
41	9.086	2475	2487	2511	rBV	760584	1289746	11.80%	5.225%
42	9.373	2574	2576	2582	rVB2	1431	1140	0.01%	0.005%
43	9.607	2645	2649	2655	rBV	1461	1517	0.01%	0.006%
44	9.713	2678	2682	2687	rVB	1655	1428	0.01%	0.006%
45	9.787	2701	2705	2707	rBV3	1581	1250	0.01%	0.005%
46	10.170	2821	2824	2828	rVB2	1530	1064	0.01%	0.004%
47	10.196	2828	2832	2836	rBV2	768	1016	0.01%	0.004%
48	10.260	2848	2852	2858	rVB2	1119	1282	0.01%	0.005%
49	10.292	2858	2862	2869	rVB	939	1131	0.01%	0.005%
50	10.369	2881	2886	2891	rVB2	1183	1565	0.01%	0.006%
51	10.427	2891	2904	2922	rBV	595177	971093	8.88%	3.934%
52	10.543	2935	2940	2943	rVB	1737	1466	0.01%	0.006%
53	10.578	2948	2951	2953	rVV	1585	1231	0.01%	0.005%
54	10.601	2953	2958	2972	rVB6	5351	9868	0.09%	0.040%
55	10.659	2972	2976	2981	rBV	1682	1527	0.01%	0.006%
56	10.881	3041	3045	3050	rBV	1650	1612	0.01%	0.007%
57	10.935	3055	3062	3067	rVB2	1464	2148	0.02%	0.009%
58	10.961	3067	3070	3072	rBV	1997	1443	0.01%	0.006%
59	11.003	3080	3083	3090	rVB2	1607	2127	0.02%	0.009%
60	11.045	3090	3096	3098	rBV	1435	1355	0.01%	0.005%
61	11.064	3098	3102	3104	rVV2	1098	1047	0.01%	0.004%
62	11.144	3125	3127	3131	rVV	1267	1017	0.01%	0.004%
63	11.270	3162	3166	3168	rBV	1360	1109	0.01%	0.004%
64	11.347	3187	3190	3200	rBV	1357	2222	0.02%	0.009%
65	11.395	3200	3205	3207	rBV	1123	1171	0.01%	0.005%
66	11.482	3220	3232	3257	rVV	763966	1234950	11.29%	5.003%
67	11.858	3336	3349	3371	rVV	768307	1276155	11.67%	5.170%
68	12.051	3405	3409	3412	rBV2	2201	1710	0.02%	0.007%
69	12.125	3429	3432	3436	rVB	1393	1092	0.01%	0.004%
70	12.324	3489	3494	3500	rBV2	1505	2366	0.02%	0.010%
71	12.479	3534	3542	3553	rBV3	4342	7809	0.07%	0.032%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031719\
 Data File : VU030145.D
 Acq On : 16 Mar 2019 15:13
 Operator : JC/SP
 Sample : K1949-19 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1H1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

72	12.559	3563	3567	3574	rBV	1349	1653	0.02%	0.007%
73	12.684	3603	3606	3613	rVB2	1292	1180	0.01%	0.005%
74	12.720	3613	3617	3620	rBV	1439	1173	0.01%	0.005%
75	12.826	3647	3650	3655	rVB2	1467	1261	0.01%	0.005%
76	12.967	3689	3694	3698	rBV2	1140	1290	0.01%	0.005%
77	13.064	3717	3724	3728	rVB	1516	2148	0.02%	0.009%
78	13.106	3734	3737	3743	rBV	1869	2342	0.02%	0.009%
79	13.376	3817	3821	3827	rVB	2130	2101	0.02%	0.009%
80	13.417	3827	3834	3837	rBV	1835	2347	0.02%	0.010%
81	13.553	3873	3876	3880	rBV3	1310	1099	0.01%	0.004%
82	13.729	3926	3931	3934	rBV	1971	1846	0.02%	0.007%
83	14.167	4063	4067	4072	rBV	1291	1503	0.01%	0.006%
84	14.279	4094	4102	4106	rBV4	3264	5290	0.05%	0.021%
85	14.556	4183	4188	4190	rBV	1087	1114	0.01%	0.005%
86	14.597	4198	4201	4206	rVB	1245	1135	0.01%	0.005%
87	14.633	4206	4212	4214	rBV2	1114	1101	0.01%	0.004%
88	14.749	4243	4248	4252	rBV3	1302	1383	0.01%	0.006%
89	15.060	4340	4345	4347	rBV	1497	1365	0.01%	0.006%
90	15.112	4358	4361	4364	rBV	1796	1336	0.01%	0.005%
91	15.167	4374	4378	4385	rVB	2774	2989	0.03%	0.012%
92	15.221	4385	4395	4400	rBV2	1959	3305	0.03%	0.013%
93	15.247	4400	4403	4405	rBV3	1568	1078	0.01%	0.004%
94	15.321	4423	4426	4429	rVV2	1417	1025	0.01%	0.004%
95	15.340	4429	4432	4438	rVB	1026	1118	0.01%	0.005%
96	15.369	4438	4441	4447	rBV3	1655	1582	0.01%	0.006%
97	15.549	4494	4497	4501	rVB2	1461	1011	0.01%	0.004%
98	15.659	4527	4531	4537	rVB3	2034	2205	0.02%	0.009%
99	15.687	4537	4540	4542	rBV	1457	1103	0.01%	0.004%
100	15.758	4558	4562	4565	rBV2	1348	1308	0.01%	0.005%


Sum of corrected areas: 24686080

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU031719\
Data File : VU030145.D
Acq On : 16 Mar 2019 15:13
Operator : JC/SP
Sample : K1949-19 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1H1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

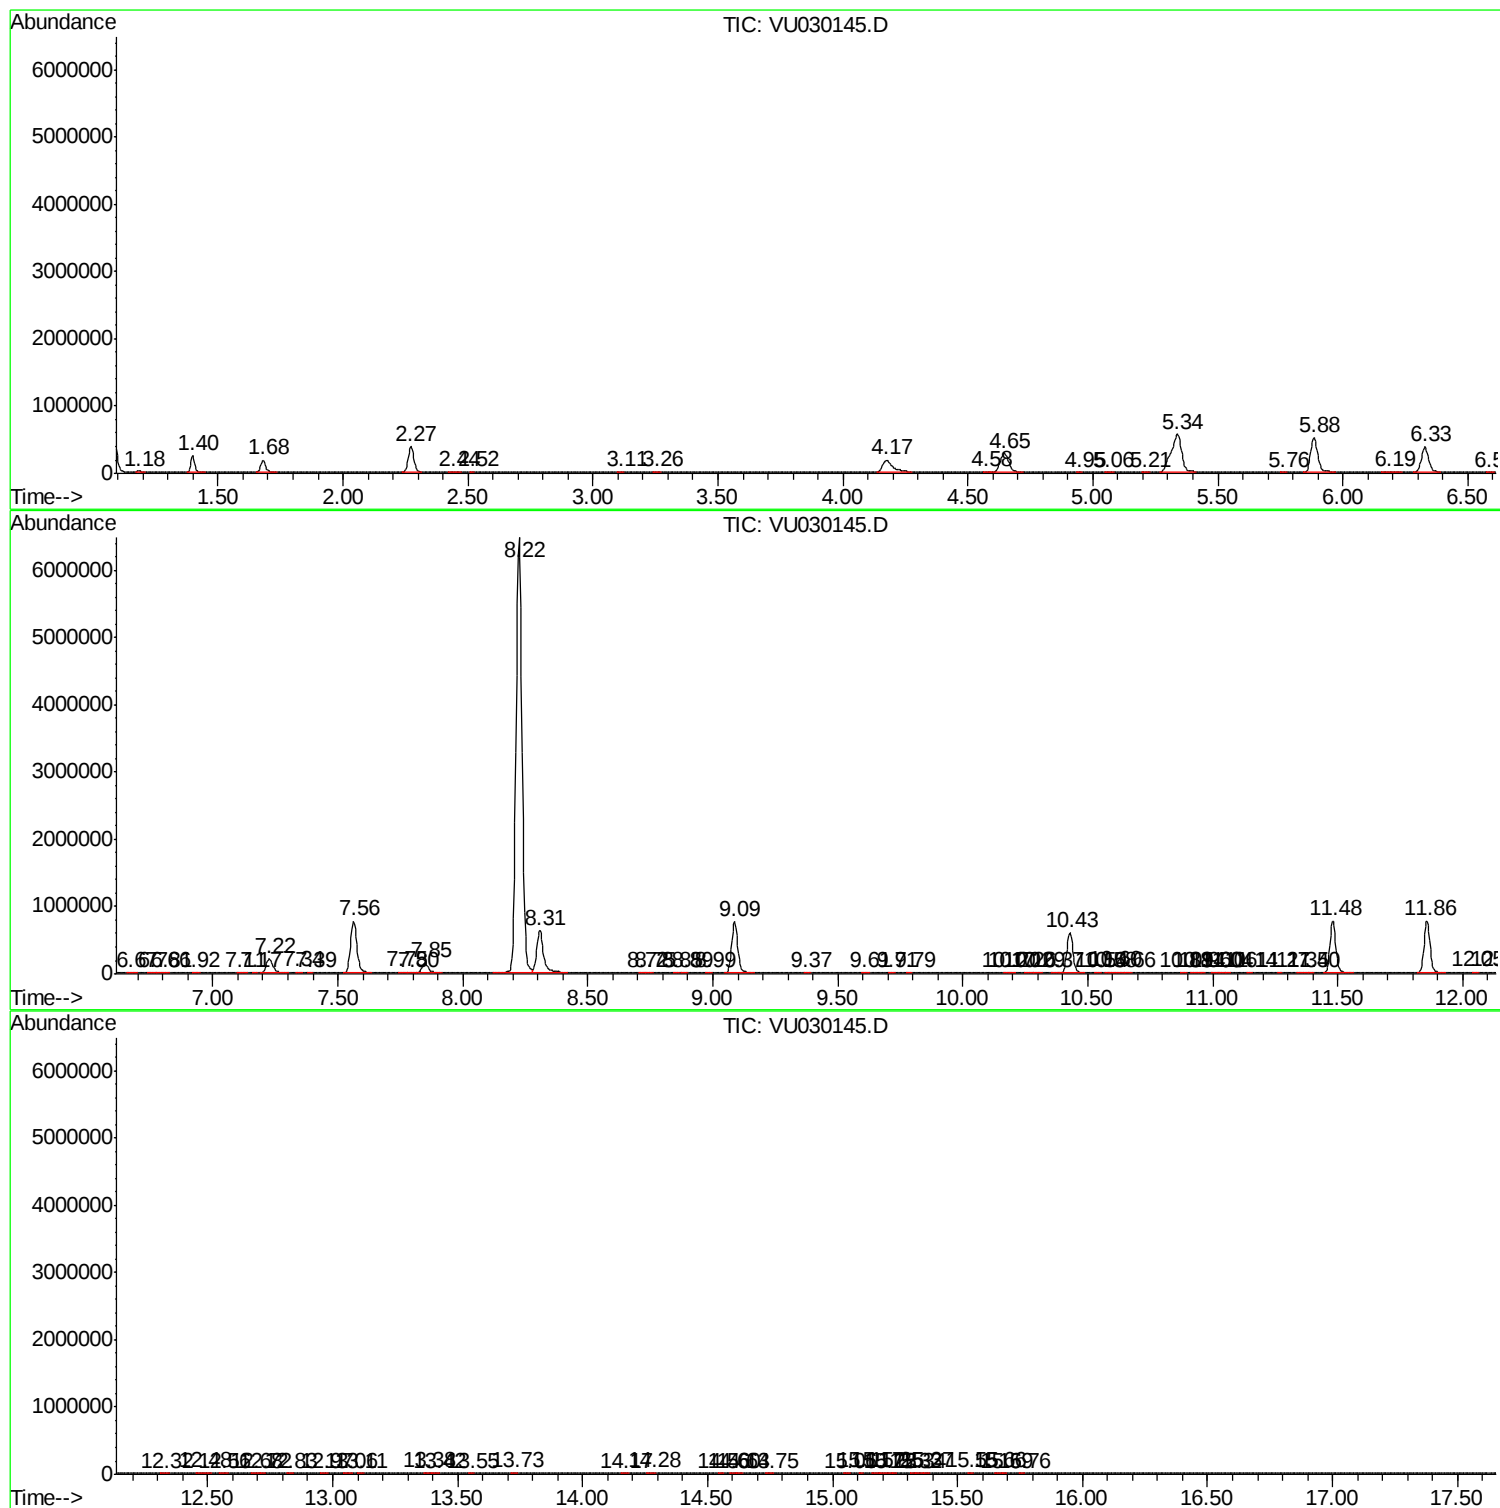

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031719\
Data File : VU030145.D
Acq On : 16 Mar 2019 15:13
Operator : JC/SP
Sample : K1949-19 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1H1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031719\
Data File : VU030145.D
Acq On : 16 Mar 2019 15:13
Operator : JC/SP
Sample : K1949-19 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1H1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc