

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031719\
 Data File : VU030148.D
 Acq On : 16 Mar 2019 16:32
 Operator : JC/SP
 Sample : K1939-17DL 10X
 Misc : 5.35/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF0Y0DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.399	89	96	109	rBV	213486	218229	13.45%	1.498%
2	1.666	171	179	189	rBV	164949	208678	12.86%	1.432%
3	2.267	356	366	381	rBV	360643	538273	33.18%	3.694%
4	2.739	509	513	517	rBV3	1671	1820	0.11%	0.012%
5	2.781	522	526	528	rBV	1035	724	0.04%	0.005%
6	2.823	535	539	541	rBV	1850	1541	0.09%	0.011%
7	2.939	571	575	578	rBV	868	757	0.05%	0.005%
8	3.038	604	606	609	rVB	866	432	0.03%	0.003%
9	3.235	663	667	670	rBV	1267	1147	0.07%	0.008%
10	3.305	683	689	690	rBV	1439	1396	0.09%	0.010%
11	3.341	697	700	705	rBV	1312	1371	0.08%	0.009%
12	3.366	705	708	711	rVV	1123	849	0.05%	0.006%
13	3.437	727	730	731	rBV	559	310	0.02%	0.002%
14	3.469	735	740	744	rVV	1473	1625	0.10%	0.011%
15	3.501	748	750	755	rVV2	765	626	0.04%	0.004%
16	3.534	757	760	764	rVB	912	666	0.04%	0.005%
17	3.701	809	812	816	rBV	993	895	0.06%	0.006%
18	3.739	821	824	827	rBV	1093	798	0.05%	0.005%
19	3.755	827	829	832	rVB2	553	263	0.02%	0.002%
20	3.788	835	839	844	rVB	877	850	0.05%	0.006%
21	3.823	844	850	851	rBV	1085	1000	0.06%	0.007%
22	3.884	866	869	871	rBV	945	680	0.04%	0.005%
23	3.926	879	882	885	rBV	889	517	0.03%	0.004%
24	3.948	885	889	895	rBV	1102	1210	0.07%	0.008%
25	3.993	899	903	905	rBV	748	622	0.04%	0.004%
26	4.038	912	917	920	rBV	1891	1636	0.10%	0.011%
27	4.093	932	934	935	rBV2	422	199	0.01%	0.001%
28	4.109	936	939	945	rVB	992	903	0.06%	0.006%
29	4.173	947	959	966	rBV	170188	381339	23.51%	2.617%
30	4.575	1081	1084	1087	rBV2	1235	923	0.06%	0.006%
31	4.643	1089	1105	1128	rVV	271060	649324	40.03%	4.457%
32	5.064	1231	1236	1239	rBV3	918	1020	0.06%	0.007%
33	5.167	1266	1268	1270	rBV2	743	435	0.03%	0.003%
34	5.193	1274	1276	1278	rBV	345	170	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031719\
 Data File : VU030148.D
 Acq On : 16 Mar 2019 16:32
 Operator : JC/SP
 Sample : K1939-17DL 10X
 Misc : 5.35/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF0Y0DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

35	5.209	1278	1281	1285	rBV	835	697	0.04%	0.005%
36	5.337	1296	1321	1350	rBV2	551882	1622249	100.00%	11.134%
37	5.601	1398	1403	1405	rBV	1427	1287	0.08%	0.009%
38	5.662	1419	1422	1426	rBV2	491	380	0.02%	0.003%
39	5.685	1426	1429	1433	rBV2	1022	751	0.05%	0.005%
40	5.704	1433	1435	1438	rBV	1153	856	0.05%	0.006%
41	5.765	1451	1454	1461	rVB3	1321	1321	0.08%	0.009%
42	5.804	1461	1466	1471	rBV2	1454	1889	0.12%	0.013%
43	5.884	1477	1491	1516	rBV	623015	1243050	76.63%	8.532%
44	6.148	1566	1573	1575	rBV2	1766	2094	0.13%	0.014%
45	6.328	1611	1629	1653	rBV	358068	735946	45.37%	5.051%
46	6.572	1701	1705	1707	rBV	1167	913	0.06%	0.006%
47	6.865	1793	1796	1798	rBV	1866	1276	0.08%	0.009%
48	7.225	1894	1908	1930	rBV	202938	377402	23.26%	2.590%
49	7.562	2001	2013	2035	rBV	747478	1293832	79.76%	8.880%
50	7.849	2091	2102	2121	rBV	140648	248319	15.31%	1.704%
51	8.000	2146	2149	2151	rBV	1363	993	0.06%	0.007%
52	8.225	2209	2219	2234	rVB	367536	621402	38.30%	4.265%
53	8.308	2235	2245	2272	rVV	602054	1018668	62.79%	6.992%
54	8.723	2370	2374	2380	rBV	1715	1675	0.10%	0.011%
55	8.823	2402	2405	2408	rBV	1754	1187	0.07%	0.008%
56	8.865	2416	2418	2420	rBV	751	370	0.02%	0.003%
57	9.086	2475	2487	2507	rBV	939418	1557684	96.02%	10.691%
58	9.537	2624	2627	2631	rVB	1419	960	0.06%	0.007%
59	9.559	2631	2634	2637	rBV	895	669	0.04%	0.005%
60	9.807	2706	2711	2714	rBV3	1392	1672	0.10%	0.011%
61	9.897	2735	2739	2742	rBV	1304	1082	0.07%	0.007%
62	10.160	2816	2821	2827	rBV	1636	2070	0.13%	0.014%
63	10.427	2893	2904	2926	rBV	605565	967960	59.67%	6.644%
64	10.566	2943	2947	2951	rBV2	1372	1386	0.09%	0.010%
65	10.604	2952	2959	2972	rVV3	3920	8114	0.50%	0.056%
66	10.704	2987	2990	2996	rVB3	1832	1701	0.10%	0.012%
67	10.739	2996	3001	3003	rBV	1541	1463	0.09%	0.010%
68	10.839	3028	3032	3036	rBV	1675	1800	0.11%	0.012%
69	11.000	3079	3082	3086	rVB2	1552	1173	0.07%	0.008%
70	11.028	3087	3091	3093	rBV	1349	936	0.06%	0.006%
71	11.395	3202	3205	3206	rBV	978	477	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031719\
Data File : VU030148.D
Acq On : 16 Mar 2019 16:32
Operator : JC/SP
Sample : K1939-17DL 10X
Misc : 5.35/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0Y0DL

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Title : VOC Analysis

72	11.482	3220	3232	3251	rBV	947298	1513147	93.27%	10.386%
73	11.858	3336	3349	3373	rBV	790728	1296738	79.93%	8.900%
74	12.356	3500	3504	3506	rBV3	892	669	0.04%	0.005%
75	12.437	3525	3529	3530	rBV	729	480	0.03%	0.003%
76	12.588	3574	3576	3580	rBV	1215	884	0.05%	0.006%
77	12.678	3602	3604	3607	rBV	927	550	0.03%	0.004%
78	12.762	3627	3630	3631	rBV	880	548	0.03%	0.004%
79	12.945	3684	3687	3692	rBV2	1605	1642	0.10%	0.011%
80	13.501	3857	3860	3862	rBV	1088	792	0.05%	0.005%
81	13.768	3940	3943	3947	rBV	2029	1561	0.10%	0.011%
82	13.913	3983	3988	3993	rBV	2177	2502	0.15%	0.017%
83	14.694	4228	4231	4234	rBV	1650	1098	0.07%	0.008%
84	15.315	4420	4424	4428	rBV2	1619	2037	0.13%	0.014%


Sum of corrected areas: 14569580

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU031719\
Data File : VU030148.D
Acq On : 16 Mar 2019 16:32
Operator : JC/SP
Sample : K1939-17DL 10X
Misc : 5.35/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0Y0DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

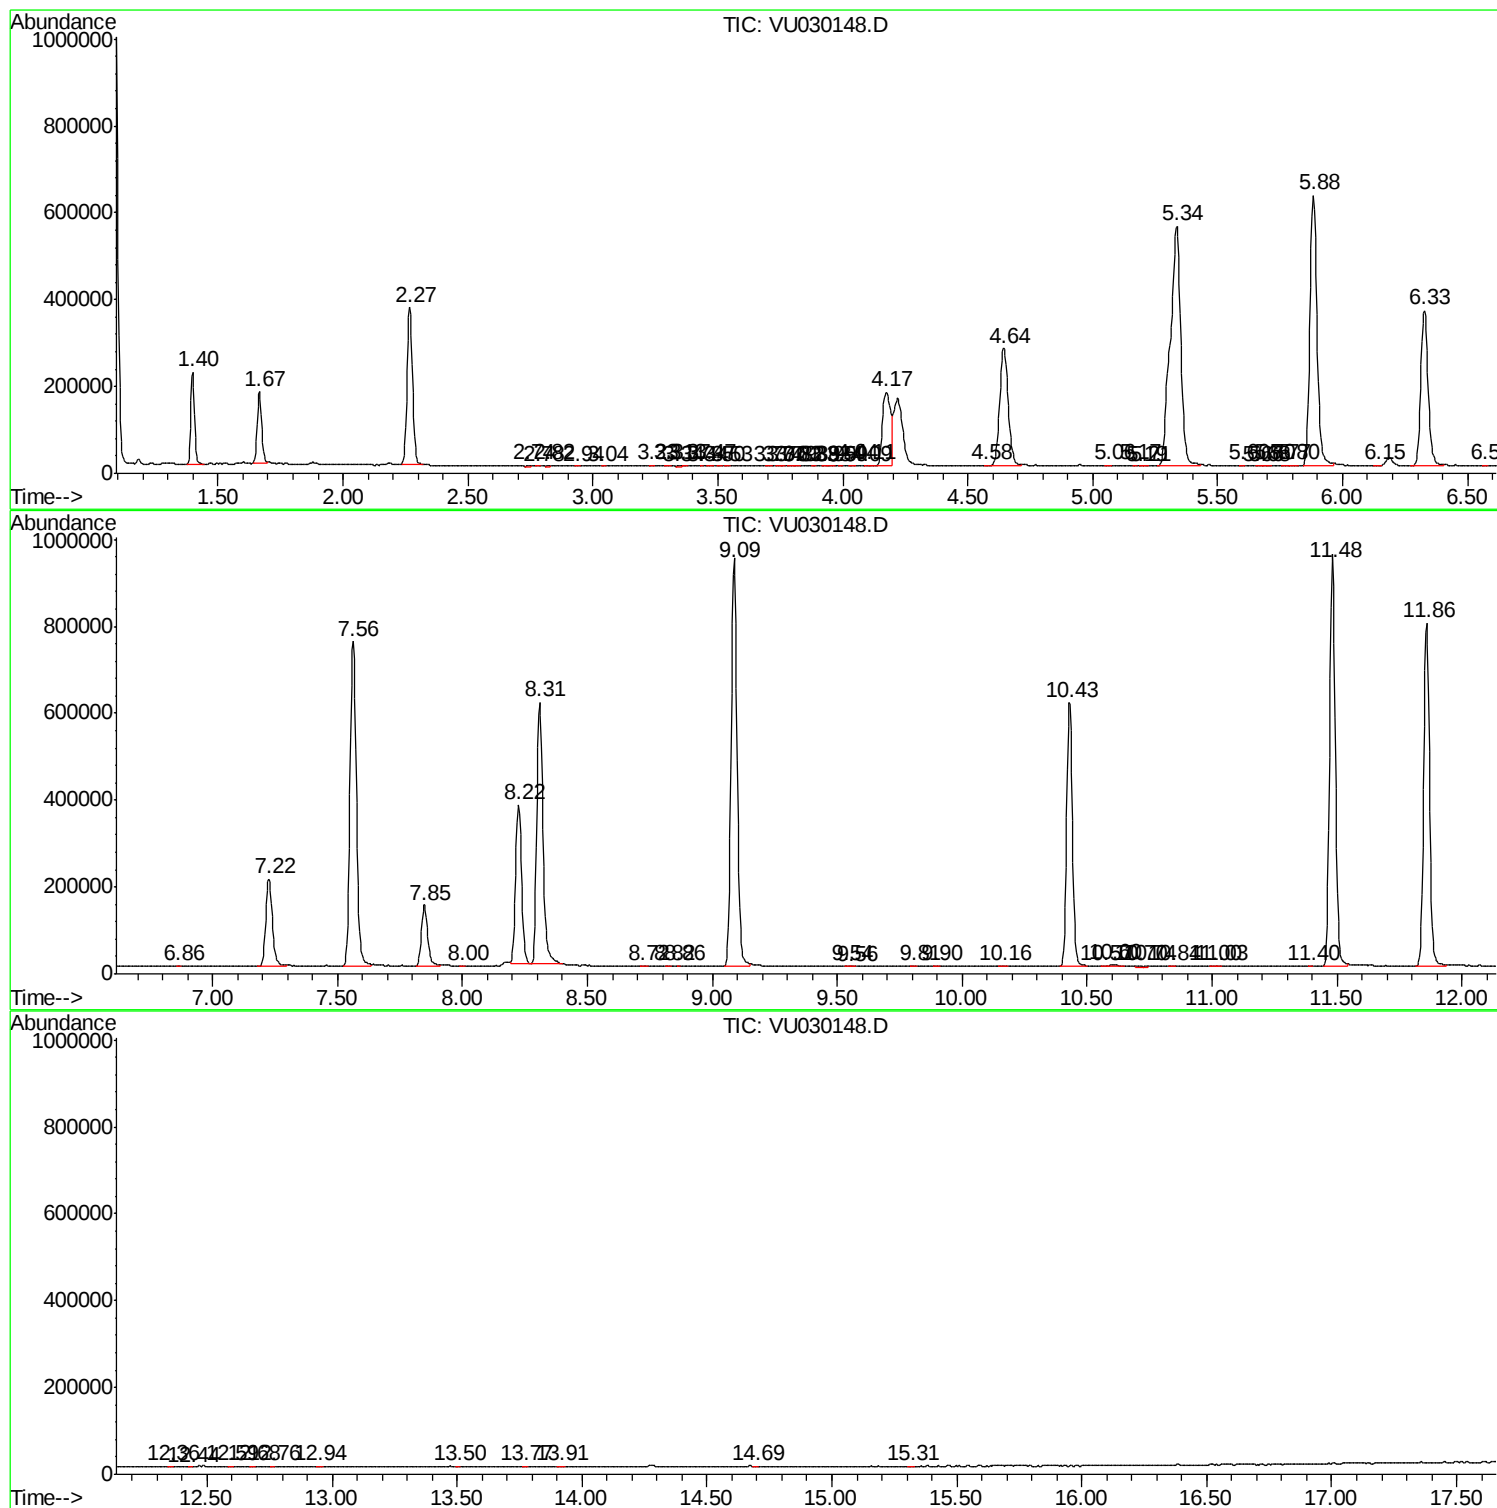

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031719\
Data File : VU030148.D
Acq On : 16 Mar 2019 16:32
Operator : JC/SP
Sample : K1939-17DL 10X
Misc : 5.35/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0Y0DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031719\
Data File : VU030148.D
Acq On : 16 Mar 2019 16:32
Operator : JC/SP
Sample : K1939-17DL 10X
Misc : 5.35/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0Y0DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc