

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031719\
 Data File : VU030156.D
 Acq On : 16 Mar 2019 19:35
 Operator : JC/SP
 Sample : K1936-13
 Misc : 6.05g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF0X1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.392	88	94	111	rVB	166945	215749	5.71%	1.143%
2	1.640	166	171	185	rBV	89597	118421	3.14%	0.628%
3	2.228	344	354	370	rBV	350532	543386	14.39%	2.880%
4	2.498	435	438	441	rBV	1322	1057	0.03%	0.006%
5	2.801	530	532	534	rBV	862	405	0.01%	0.002%
6	2.823	534	539	543	rBV2	2484	2838	0.08%	0.015%
7	3.016	595	599	601	rBV2	1101	806	0.02%	0.004%
8	3.267	673	677	678	rBV	1082	667	0.02%	0.004%
9	3.434	725	729	733	rBV	1300	1446	0.04%	0.008%
10	3.768	829	833	841	rBV	1511	1585	0.04%	0.008%
11	3.842	853	856	858	rBV	1138	806	0.02%	0.004%
12	3.894	869	872	873	rBV	1240	699	0.02%	0.004%
13	4.141	946	949	952	rBV	1621	1051	0.03%	0.006%
14	4.193	952	965	1000	rBV2	139931	493328	13.06%	2.615%
15	4.530	1064	1070	1074	rBV2	1487	1935	0.05%	0.010%
16	4.640	1088	1104	1131	rBV	265928	652774	17.29%	3.460%
17	5.219	1280	1284	1287	rVB	1774	1380	0.04%	0.007%
18	5.238	1287	1290	1292	rBV	708	453	0.01%	0.002%
19	5.328	1296	1318	1345	rBV2	587055	1651687	43.74%	8.754%
20	5.534	1376	1382	1383	rBV	1385	1438	0.04%	0.008%
21	5.588	1396	1399	1401	rBV	1018	725	0.02%	0.004%
22	5.878	1475	1489	1515	rBV	614418	1300530	34.44%	6.893%
23	6.071	1545	1549	1552	rBV	1696	1032	0.03%	0.005%
24	6.180	1571	1583	1597	rBV2	83696	172583	4.57%	0.915%
25	6.325	1614	1628	1650	rBV	349259	738734	19.56%	3.915%
26	6.505	1681	1684	1687	rVB	1731	1085	0.03%	0.006%
27	6.521	1687	1689	1690	rBV	812	315	0.01%	0.002%
28	6.678	1736	1738	1741	rBV	610	317	0.01%	0.002%
29	6.698	1741	1744	1748	rBV2	1097	722	0.02%	0.004%
30	6.720	1748	1751	1752	rVV	804	445	0.01%	0.002%
31	6.746	1756	1759	1761	rBV	905	487	0.01%	0.003%
32	6.817	1779	1781	1784	rVB	729	366	0.01%	0.002%
33	6.836	1784	1787	1792	rVB	843	694	0.02%	0.004%
34	6.897	1792	1806	1813	rBV5	3492	8305	0.22%	0.044%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031719\
 Data File : VU030156.D
 Acq On : 16 Mar 2019 19:35
 Operator : JC/SP
 Sample : K1936-13
 Misc : 6.05µ/5.0mL/100µL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF0X1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

35	6.964	1825	1827	1829	rBV	661	414	0.01%	0.002%
36	7.009	1838	1841	1844	rBV	858	572	0.02%	0.003%
37	7.029	1844	1847	1849	rBV2	1001	626	0.02%	0.003%
38	7.087	1862	1865	1868	rBV2	746	424	0.01%	0.002%
39	7.122	1872	1876	1877	rBV	474	263	0.01%	0.001%
40	7.138	1877	1881	1883	rBV	1174	776	0.02%	0.004%
41	7.183	1891	1895	1897	rBV	837	653	0.02%	0.003%
42	7.225	1897	1908	1932	rVV	184126	367848	9.74%	1.950%
43	7.395	1956	1961	1968	rBV	2169	2705	0.07%	0.014%
44	7.431	1970	1972	1974	rBV	1070	513	0.01%	0.003%
45	7.447	1974	1977	1982	rVV	1894	1517	0.04%	0.008%
46	7.489	1988	1990	1994	rVB2	1404	860	0.02%	0.005%
47	7.511	1994	1997	1999	rBV	710	502	0.01%	0.003%
48	7.559	2000	2012	2034	rBV	728183	1334139	35.33%	7.071%
49	7.849	2089	2102	2124	rBV2	126927	258876	6.86%	1.372%
50	8.003	2148	2150	2155	rBV	933	703	0.02%	0.004%
51	8.222	2194	2218	2238	rBV	2179610	3775997	100.00%	20.012%
52	8.325	2239	2250	2276	rVB	577541	1135864	30.08%	6.020%
53	8.733	2374	2377	2379	rBV2	851	445	0.01%	0.002%
54	8.749	2379	2382	2385	rVB3	1038	648	0.02%	0.003%
55	8.775	2386	2390	2393	rBV2	975	811	0.02%	0.004%
56	8.903	2425	2430	2433	rVB2	1493	1492	0.04%	0.008%
57	8.923	2433	2436	2440	rBV	1281	1177	0.03%	0.006%
58	8.974	2449	2452	2456	rBV	1018	1042	0.03%	0.006%
59	9.090	2476	2488	2516	rVB	919377	1664358	44.08%	8.821%
60	9.289	2548	2550	2552	rBV2	1083	664	0.02%	0.004%
61	9.344	2564	2567	2568	rBV	1041	506	0.01%	0.003%
62	9.395	2579	2583	2590	rBV3	1104	1114	0.03%	0.006%
63	9.530	2622	2625	2628	rBV2	991	637	0.02%	0.003%
64	9.572	2635	2638	2640	rBV	762	374	0.01%	0.002%
65	9.640	2655	2659	2662	rBV2	789	764	0.02%	0.004%
66	9.672	2667	2669	2673	rVB	921	615	0.02%	0.003%
67	9.749	2691	2693	2697	rVB2	1219	840	0.02%	0.004%
68	9.771	2697	2700	2704	rBV	1571	1114	0.03%	0.006%
69	9.804	2706	2710	2712	rVV2	1876	1363	0.04%	0.007%
70	9.816	2712	2714	2720	rVB2	1344	1118	0.03%	0.006%
71	9.845	2720	2723	2724	rBV2	259	134	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031719\
 Data File : VU030156.D
 Acq On : 16 Mar 2019 19:35
 Operator : JC/SP
 Sample : K1936-13
 Misc : 6.05g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF0X1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

72	9.903	2738	2741	2745	rBV2	1270	1052	0.03%	0.006%
73	10.038	2779	2783	2786	rBV2	1085	962	0.03%	0.005%
74	10.132	2807	2812	2814	rBV2	696	657	0.02%	0.003%
75	10.286	2857	2860	2867	rVB	2023	2130	0.06%	0.011%
76	10.321	2867	2871	2875	rBV	2061	1858	0.05%	0.010%
77	10.434	2892	2906	2933	rBV	693615	1111643	29.44%	5.892%
78	10.720	2992	2995	2997	rBV	767	483	0.01%	0.003%
79	10.797	3015	3019	3021	rBV2	1658	1436	0.04%	0.008%
80	10.858	3034	3038	3041	rBV	1037	919	0.02%	0.005%
81	10.906	3049	3053	3057	rBV	1332	1310	0.03%	0.007%
82	11.061	3092	3101	3102	rBV2	1750	1933	0.05%	0.010%
83	11.128	3119	3122	3126	rBV	795	800	0.02%	0.004%
84	11.202	3140	3145	3149	rBV	1823	2137	0.06%	0.011%
85	11.260	3160	3163	3166	rBV3	1297	783	0.02%	0.004%
86	11.340	3185	3188	3190	rBV2	1113	820	0.02%	0.004%
87	11.482	3220	3232	3252	rBV	1131677	1790777	47.43%	9.491%
88	11.858	3337	3349	3371	rBV	899018	1463896	38.77%	7.758%
89	13.048	3715	3719	3722	rBV	1502	1124	0.03%	0.006%
90	13.768	3938	3943	3946	rBV	1456	1491	0.04%	0.008%
91	13.819	3956	3959	3961	rBV2	1321	751	0.02%	0.004%
92	13.836	3961	3964	3967	rVB	1596	885	0.02%	0.005%


Sum of corrected areas: 18868566

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU031719\
Data File : VU030156.D
Acq On : 16 Mar 2019 19:35
Operator : JC/SP
Sample : K1936-13
Misc : 6.05g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0X1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

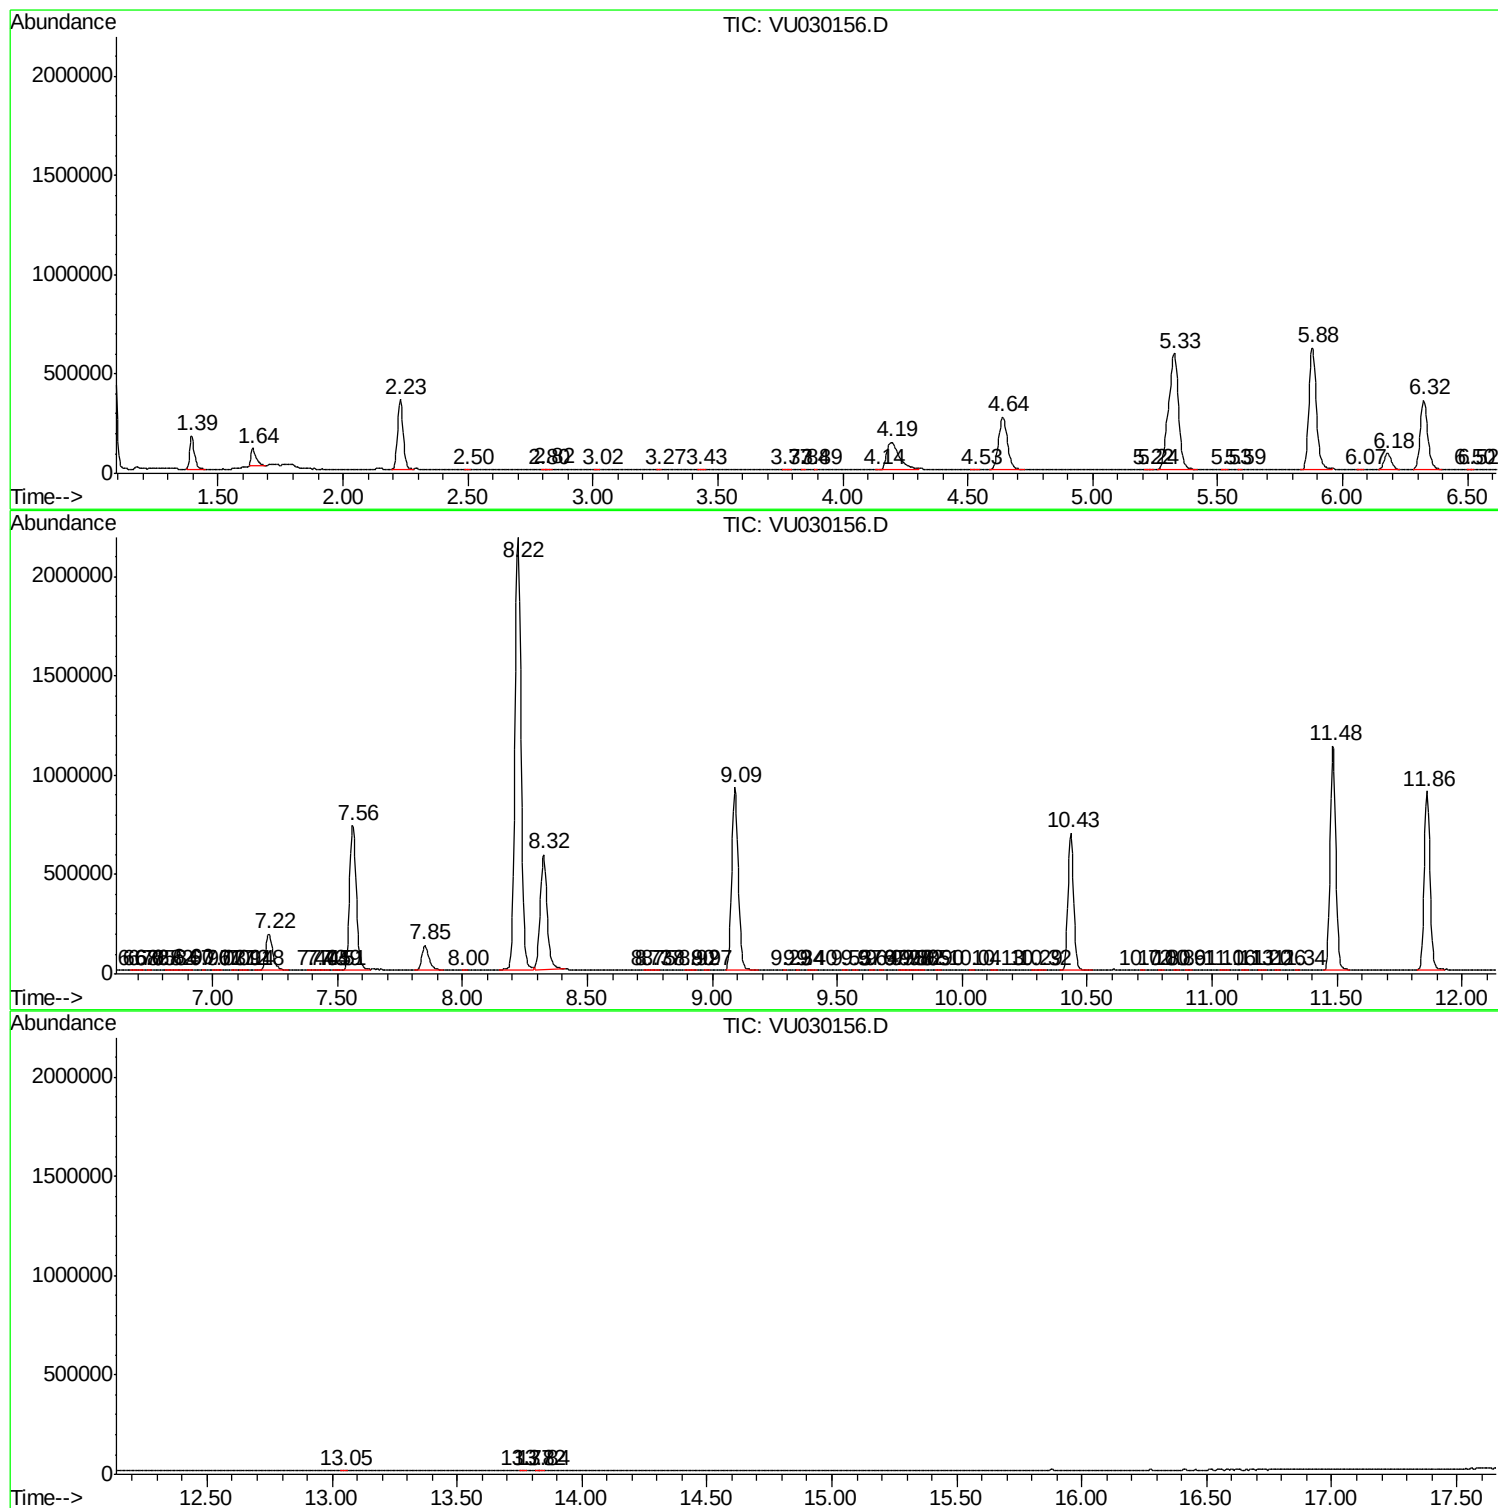

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031719\
Data File : VU030156.D
Acq On : 16 Mar 2019 19:35
Operator : JC/SP
Sample : K1936-13
Misc : 6.05g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0X1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031719\
Data File : VU030156.D
Acq On : 16 Mar 2019 19:35
Operator : JC/SP
Sample : K1936-13
Misc : 6.05g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0X1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc