
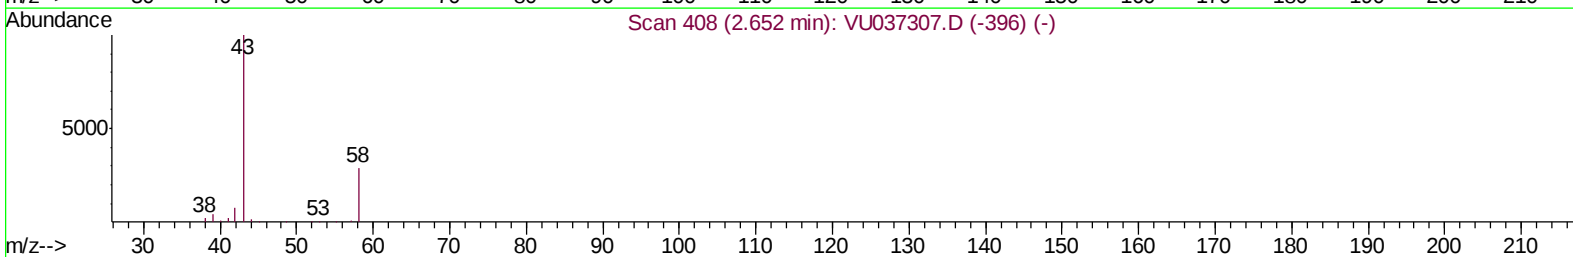
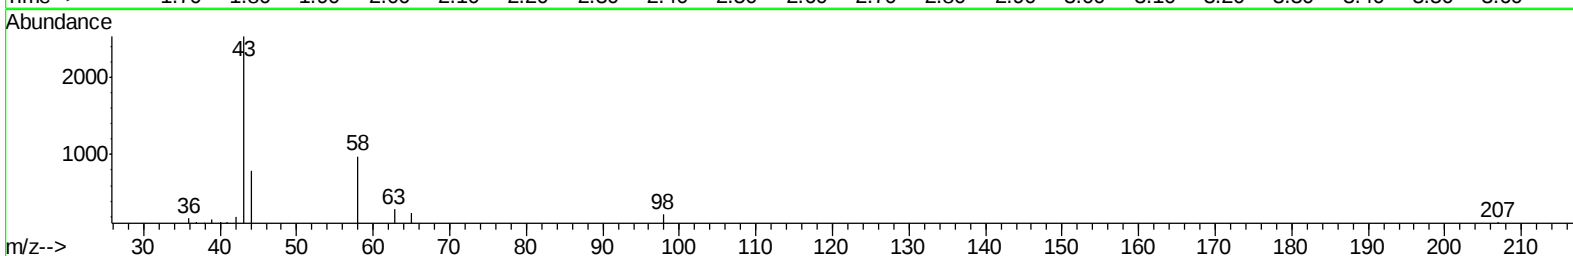


Data File : VU037321.D
Acq On : 17 Mar 2020 16:52
Operator : JC/MD
Sample : L1494-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Mar 18 02:40:11 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 18 02:36:04 2020
Response via : Initial Calibration

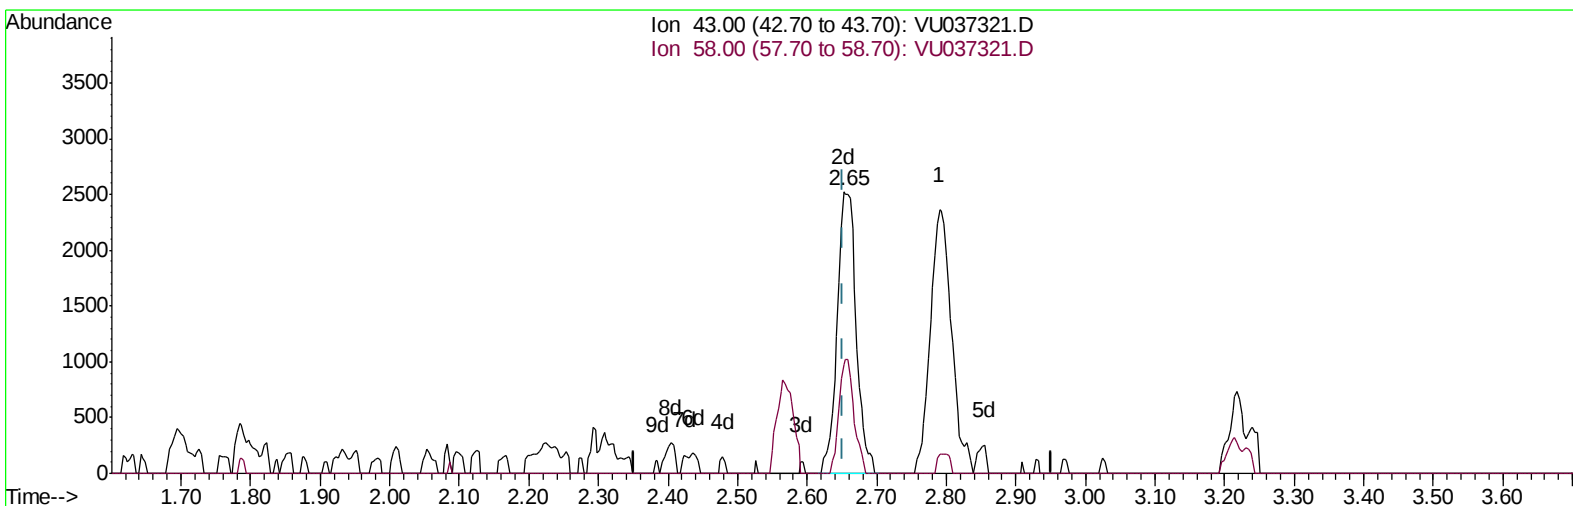

TIC: VU037321.D

(13) Acetone (T)

2.652min (+0.000) 1.98ug/L m

response 4795

Ion	Exp%	Act%
43.00	100	100
58.00	28.60	2.69
0.00	0.00	0.00
0.00	0.00	0.00