
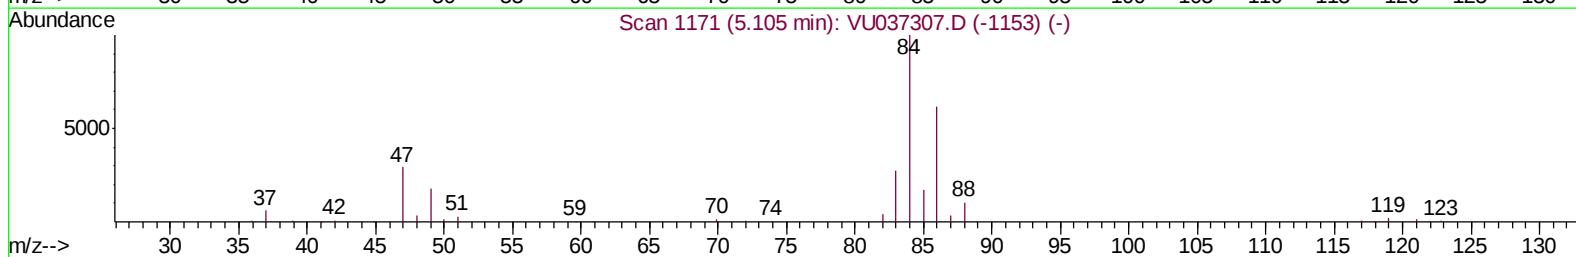
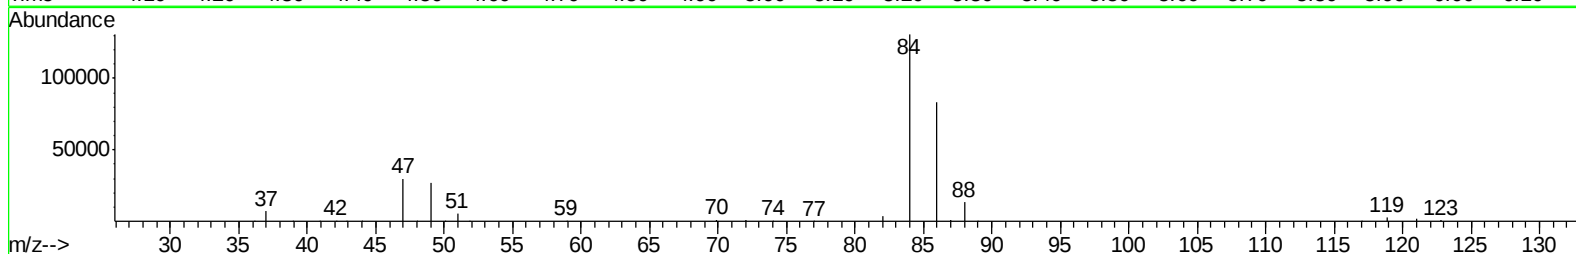


Data File : VU037325.D
Acq On : 17 Mar 2020 18:23
Operator : JC/MD
Sample : L1494-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Mar 18 02:40:47 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 18 02:36:04 2020
Response via : Initial Calibration

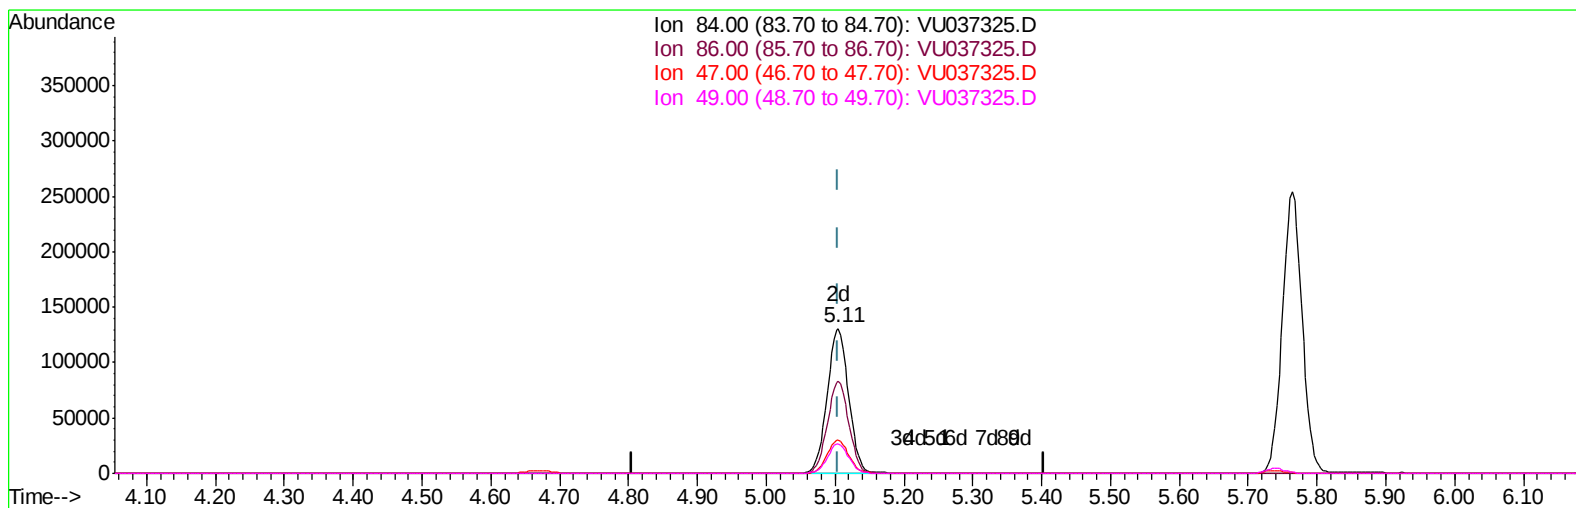

TIC: VU037325.D

(24) Chloroform-d (S)

5.105min (0.000) 45.99ug/L m

response 282960

Ion	Exp%	Act%
84.00	100	100
86.00	62.70	0.02#
47.00	50.00	0.02#
49.00	29.90	0.01#