

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031720\
Quantitation Report (Qedit)


Data File : VU037309.D
Acq On : 17 Mar 2020 12:19
Operator : JC/MD
Sample : L1901-06DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0NC9DL

Manual Integrations
APPROVED

apatel
3/18/2020 12:02:52 PM

Quant Time: Mar 18 02:38:25 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 18 02:36:04 2020
Response via : Initial Calibration

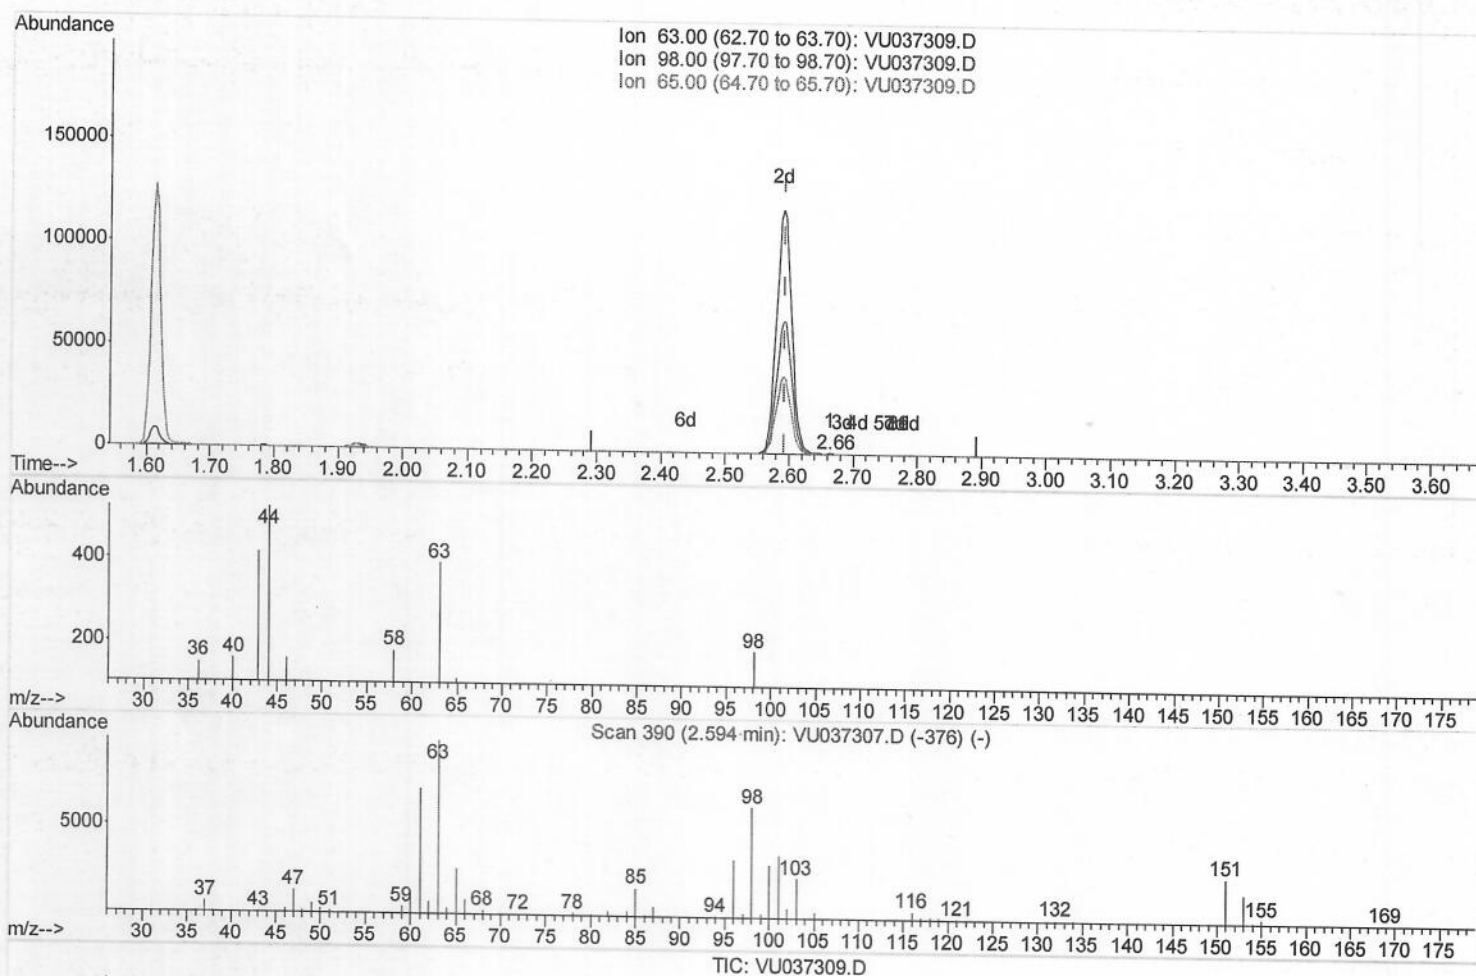

(11) 1,1-Dichloroethene-d2 (S)

2.665min (+0.071) 0.05ug/L

response 324

Ion	Exp%	Act%
63.00	100	100
98.00	63.10	58.02
65.00	23.70	30.25
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031720\
Quantitation Report (Qedit)


Data File : VU037309.D
Acq On : 17 Mar 2020 12:19
Operator : JC/MD
Sample : L1901-06DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0NC9DL

Manual Integrations
APPROVED

apatel
3/18/2020 12:02:52 PM

Quant Time: Mar 18 02:38:25 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 18 02:36:04 2020
Response via : Initial Calibration

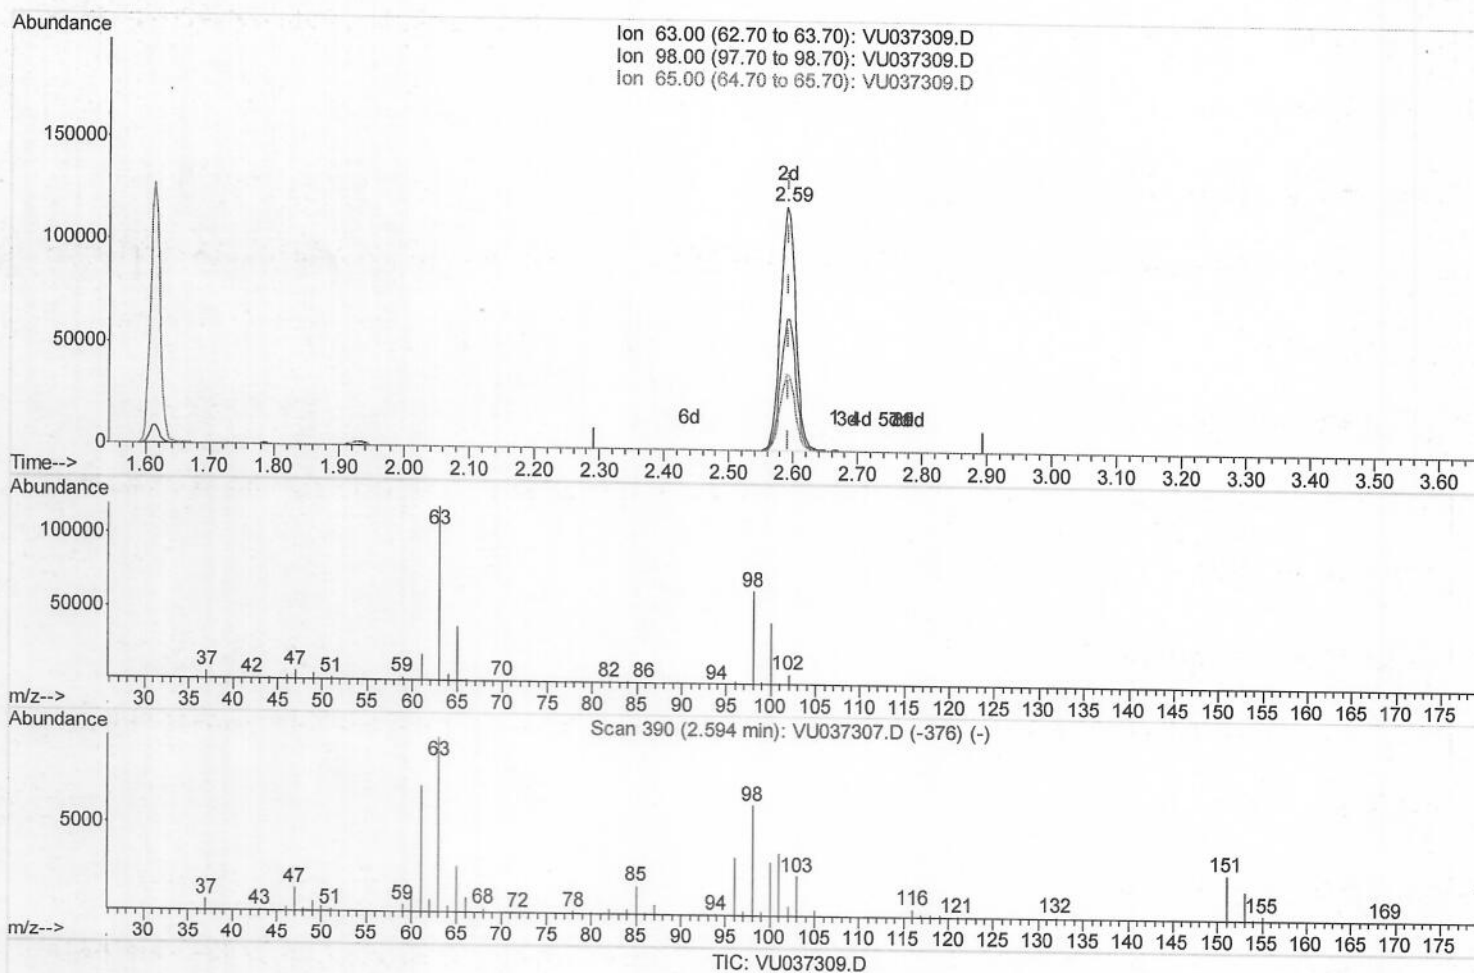

(11) 1,1-Dichloroethene-d2 (S)

2.591min (-0.003) 31.12ug/L m

response 195817

Ion	Exp%	Act%
63.00	100	100
98.00	63.10	0.10#
65.00	23.70	0.05#
0.00	0.00	0.00

MD
03/23/2020

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031720\
 Quantitation Report (QT Reviewed)

Data File : VU037309.D
 Acq On : 17 Mar 2020 12:19
 Operator : JC/MD
 Sample : L1901-06DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0NC9DL

Manual Integrations
 APPROVED

apatel
 3/18/2020 12:02:52 PM

Quant Time: Mar 18 03:02:00 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 18 02:36:04 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	443116	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	427043	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	174463	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	133773	39.01	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	78.02%		
7) Chloroethane-d5	1.93	69	123234	44.57	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	89.14%		
11) 1,1-Dichloroethene-d2	2.59	63	195817m	31.12	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	62.24%		
21) 2-Butanone-d5	4.67	46	243737	89.81	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	89.81%		
24) Chloroform-d	5.11	84	292430	44.35	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.70%		
26) 1,2-Dichloroethane-d4	5.74	65	217924	45.15	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.30%		
32) Benzene-d6	5.76	84	545123	46.37	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.74%		
36) 1,2-Dichloropropane-d6	6.73	67	180357	46.87	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	93.74%		
41) Toluene-d8	7.93	98	510360	45.41	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	90.82%		
43) trans-1,3-Dichloropropene-	8.20	79	93106	44.45	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	88.90%		
47) 2-Hexanone-d5	8.66	63	172656	86.66	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	86.66%		
57) 1,1,2,2-Tetrachloroethane-	10.78	84	260264	43.66	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	87.32%		
64) 1,2-Dichlorobenzene-d4	12.21	152	184302	50.93	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	101.86%		

MD
 03/23/2020

Target Compounds

					Qvalue	
12) 1,1-Dichloroethene	2.60	96	5389	2.061	ug/L #	1
20) cis-1,2-Dichloroethene	4.71	96	4864	1.468	ug/L	91
30) 1,1,1-Trichloroethane	5.36	97	6974	1.230	ug/L #	81
34) Trichloroethene	6.57	95	70834	21.656	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031720\
Quantitation Report (QT Reviewed)
Data File : VU037309.D
Acq On : 17 Mar 2020 12:19
Operator : JC/MD
Sample : L1901-06DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0NC9DL

Quant Time: Mar 18 03:02:00 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 18 02:36:04 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

apatel
3/18/2020 12:02:52 PM

