


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU031720\
 Data File : VU037306.D
 Acq On : 17 Mar 2020 10:20
 Operator : JC/MD
 Sample : BFB31
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB31

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
 Title : VOC Analysis
 Last Update : Wed Mar 18 12:18:01 2020

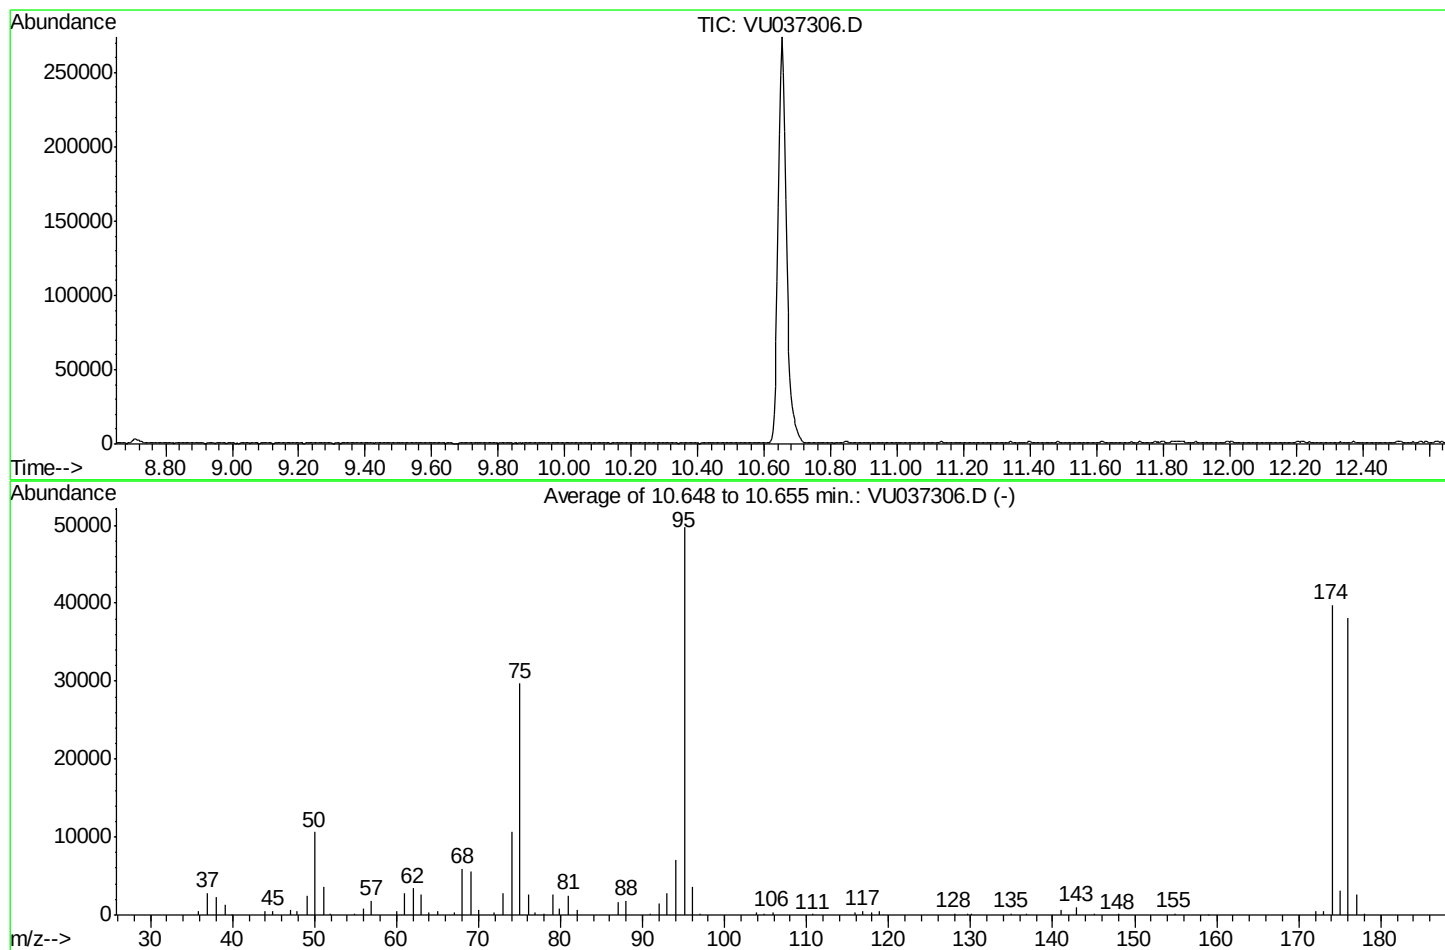

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	10664	PASS
75	95	30	80	59.7	29696	PASS
95	95	100	100	100.0	49741	PASS
96	95	5	9	7.2	3592	PASS
173	174	0.00	2	1.4	561	PASS
174	95	50	120	80.1	39818	PASS
175	174	5	9	7.9	3153	PASS
176	174	95	101	95.8	38136	PASS
177	176	5	9	7.1	2713	PASS

m/z	Abundance
35.90	510.0
37.00	2625.0
38.00	2091.0
39.10	1286.0
39.80	188.0
44.00	930.0
44.90	618.0
47.10	646.0
47.90	414.0
49.00	2412.0
50.00	9996.0
51.10	3312.0
51.90	181.0
55.00	187.0
56.00	944.0
56.90	1475.0
60.10	614.0
61.00	2530.0
62.10	3253.0
63.00	2376.0
63.90	297.0
65.00	435.0
67.00	297.0
68.00	5712.0
69.00	5216.0
70.00	645.0
72.00	417.0
73.00	2677.0
74.10	10363.0
75.00	28232.0
76.00	2513.0
76.90	333.0
77.90	181.0
79.00	2539.0
79.90	724.0
81.00	2281.0
82.00	582.0
87.10	1578.0
88.00	1853.0
90.90	188.0
92.00	1677.0
93.00	2693.0
94.10	6742.0
95.10	47384.0
96.10	3453.0
103.90	259.0
104.70	113.0
105.90	420.0
110.80	135.0
115.90	281.0
117.00	556.0
117.90	296.0
118.90	455.0
128.00	199.0
130.00	166.0
135.00	173.0
136.90	121.0
141.00	696.0
142.90	1032.0
145.00	171.0
154.90	142.0
172.00	500.0
173.00	556.0
174.00	36232.0
175.00	2823.0
176.00	34552.0
177.10	2624.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

m/z	Abundance
35.90	569.0
37.00	2935.0
38.00	2359.0
39.10	1409.0
39.90	245.0
43.90	1005.0
44.90	568.0
47.00	724.0
47.90	459.0
49.10	2454.0
50.00	10945.0
51.00	3756.0
51.90	108.0
54.90	250.0
56.00	943.0
56.90	1917.0
60.10	597.0
61.00	2789.0
62.00	3554.0
63.00	2678.0
64.00	357.0
65.00	501.0
67.00	302.0
68.00	6078.0
69.00	5648.0
70.00	660.0
72.00	406.0
73.00	2844.0
74.10	11018.0
75.00	30856.0
76.00	2698.0
76.90	330.0
78.00	247.0
79.00	2862.0
79.90	888.0
81.00	2628.0
81.90	719.0
87.00	1777.0
88.00	1887.0
90.90	215.0
92.00	1487.0
93.00	2946.0
94.10	7229.0
95.10	50976.0
96.10	3748.0
97.00	142.0
103.80	306.0
104.70	150.0
105.80	398.0
110.80	133.0
115.80	260.0
116.90	565.0
117.80	309.0
118.90	484.0
128.00	200.0
129.60	123.0
130.10	138.0
135.00	222.0
136.70	104.0
141.00	708.0
142.90	976.0
145.00	190.0
148.00	112.0
154.90	198.0
158.90	132.0
172.00	611.0
173.00	579.0
174.10	40888.0
175.10	3191.0
176.00	39016.0
177.10	2763.0
178.00	141.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

m/z	Abundance
35.90	590.0
37.00	3066.0
38.00	2669.0
39.00	1348.0
39.90	252.0
43.90	995.0
44.90	401.0
47.00	729.0
47.90	420.0
49.00	2301.0
50.00	11052.0
51.00	3809.0
54.90	236.0
56.00	815.0
57.00	2044.0
60.10	515.0
61.00	2904.0
62.00	3490.0
63.00	2703.0
64.00	348.0
65.00	548.0
67.00	206.0
68.00	6008.0
69.00	5802.0
70.00	569.0
71.90	358.0
73.00	2780.0
74.10	10587.0
75.10	30000.0
76.10	2561.0
76.90	362.0
78.00	298.0
79.00	2659.0
79.90	918.0
81.00	2683.0
81.90	736.0
87.00	1778.0
88.00	1780.0
90.90	268.0
91.90	1405.0
93.00	2896.0
94.00	7120.0
95.10	50864.0
96.10	3575.0
97.00	133.0
103.80	326.0
104.80	131.0
105.80	364.0
110.80	116.0
115.80	258.0
116.80	496.0
117.90	322.0
118.90	438.0
128.00	214.0
129.70	199.0
135.00	215.0
136.60	133.0
141.00	741.0
143.00	1038.0
145.00	190.0
148.00	165.0
154.90	211.0
158.90	117.0
172.00	609.0
173.00	550.0
174.10	42336.0
175.10	3445.0
176.10	40840.0
177.00	2753.0
178.00	125.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

Scan 2883 (10.610 min): VU037306.D
BFB31

m/z	Abundance
39.90	153.0
44.00	522.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31