

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031721\
 Data File : VU042692.D
 Acq On : 17 Mar 2021 16:38
 Operator : SY/MD
 Sample : VU0317WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0317WBL01

Quant Time: Mar 18 07:30:05 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U031721DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Mar 18 07:25:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.124	96	16143	1.00	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.642	95	5600	0.78	ug/l	0.00
Spiked Amount 1.000			Recovery	=	78.00%	
68) 1,2-Dichlorobenzene-d4	12.201	152	6261	0.82	ug/l	0.00
Spiked Amount 1.000			Recovery	=	82.00%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031721\
Data File : VU042692.D
Acq On : 17 Mar 2021 16:38
Operator : SY/MD
Sample : VU0317WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0317WBL01

Quant Time: Mar 18 07:30:05 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U031721DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Mar 18 07:25:09 2021
Response via : Initial Calibration

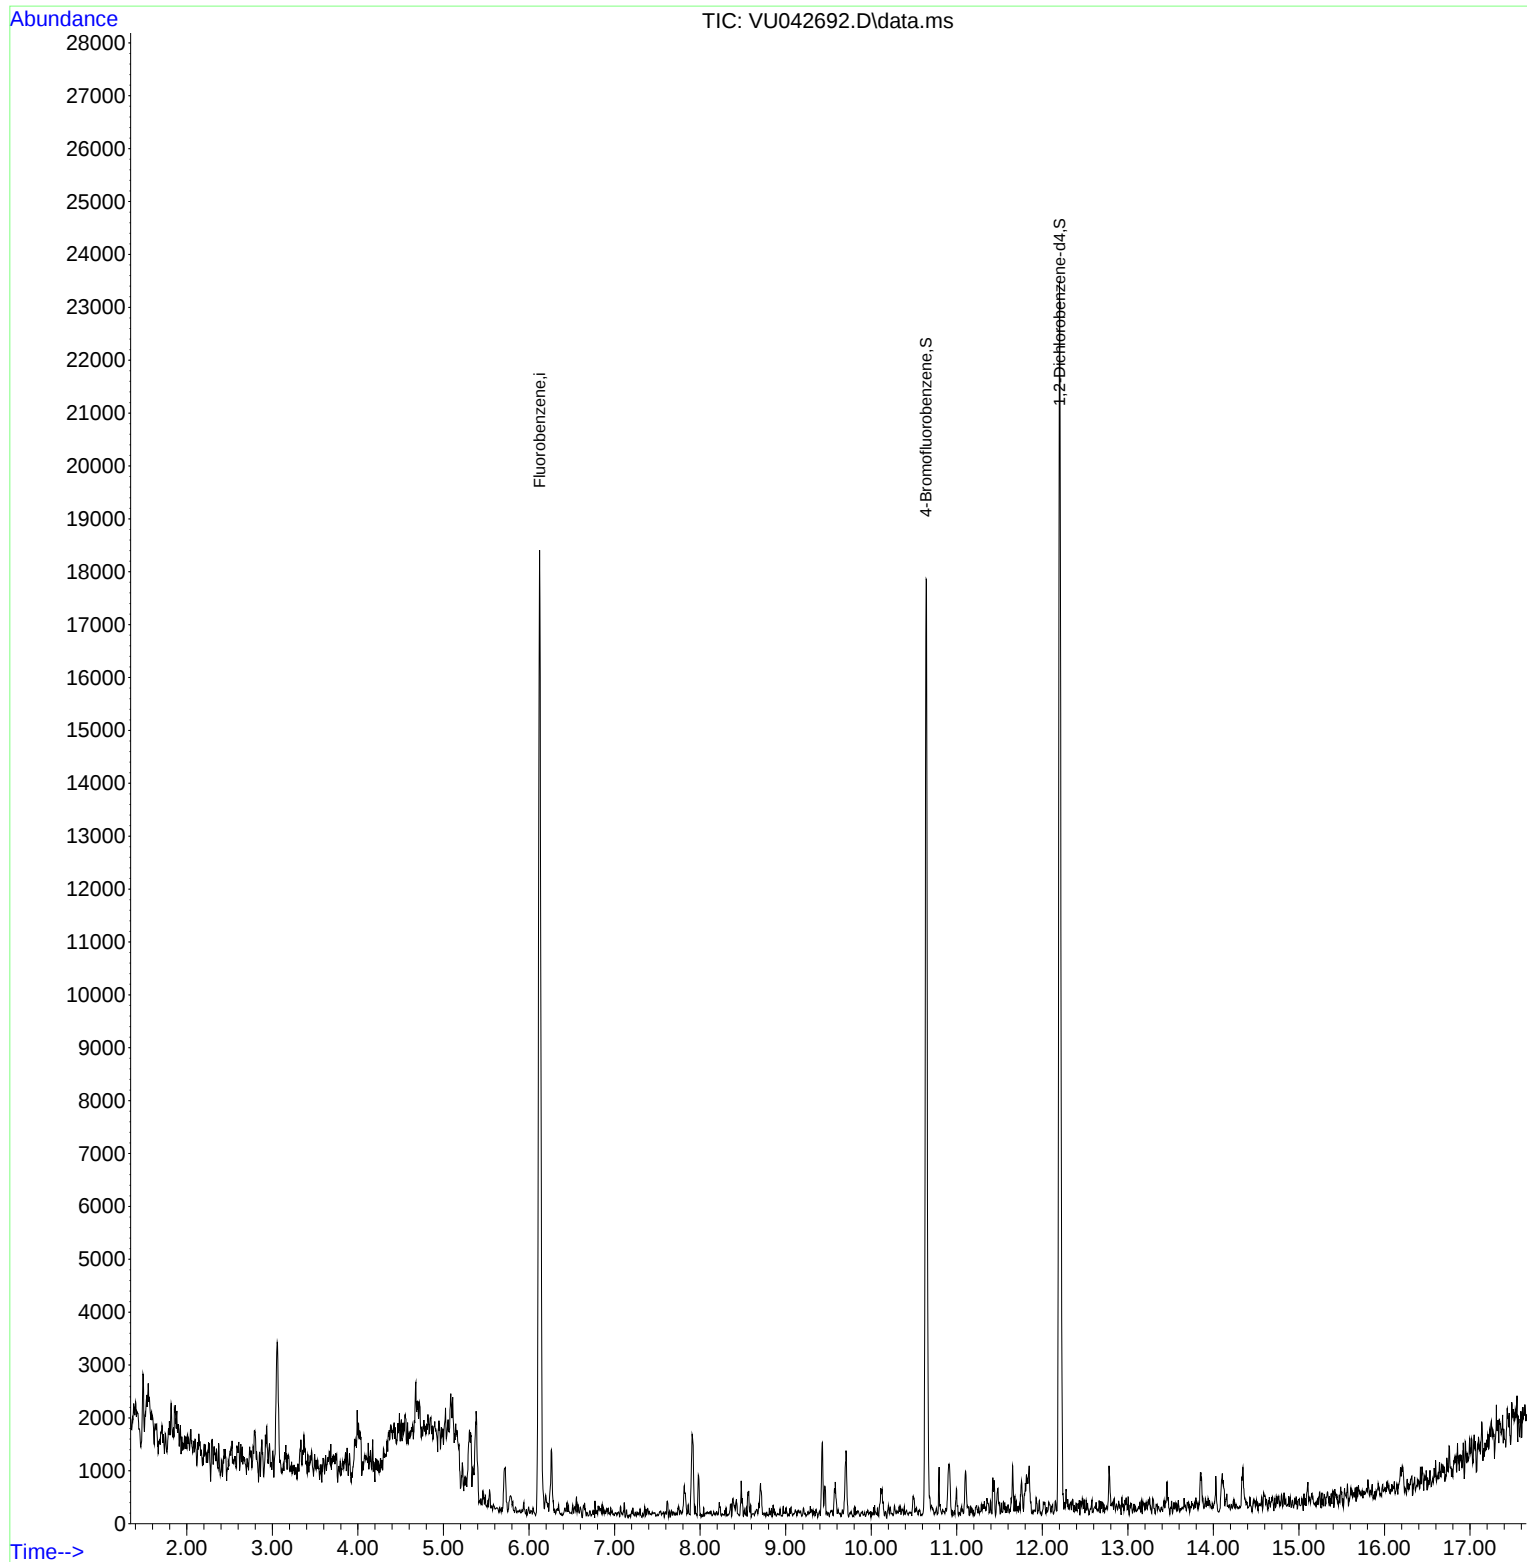




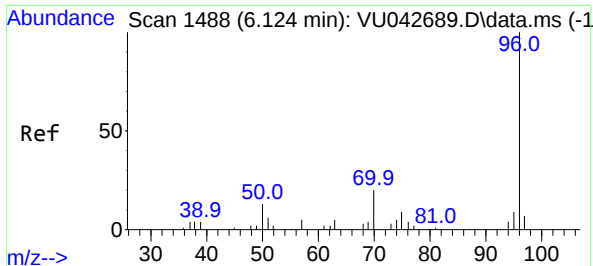


#1
Fluorobenzene
Concen: 1.00 ug/l
RT: 6.124 min Scan# 1488
Delta R.T. 0.000 min
Lab File: VU042692.D
Acq: 17 Mar 2021 16:38

Instrument :
MSVOA_U
ClientSampleId :
VU0317WBL01

Tgt Ion: 96 Resp: 16143




Ion	Ratio	Lower	Upper
96	100		
70	20.7	17.2	25.8
95	8.8	8.0	12.0
97	6.5	0.0	0.0

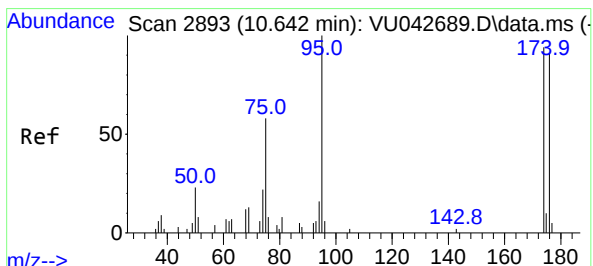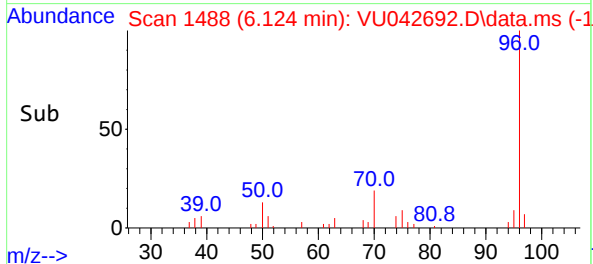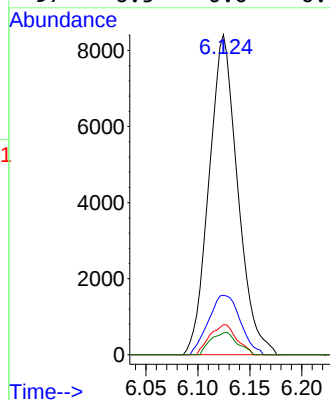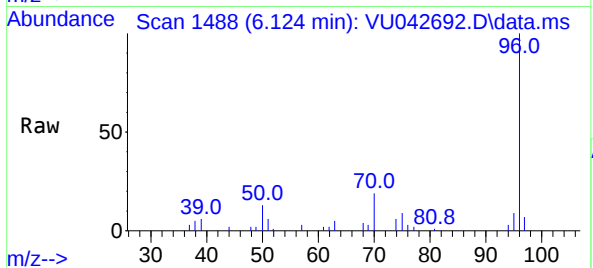


#57
4-Bromofluorobenzene
Concen: 0.78 ug/l
RT: 10.642 min Scan# 2893
Delta R.T. 0.000 min
Lab File: VU042692.D
Acq: 17 Mar 2021 16:38

Tgt Ion: 95 Resp: 5600

Ion	Ratio	Lower	Upper
95	100		
174	93.4	73.8	110.6
176	82.1	71.4	107.0

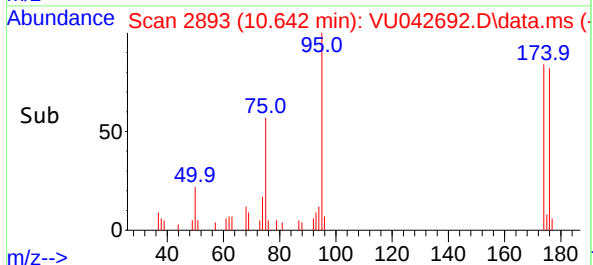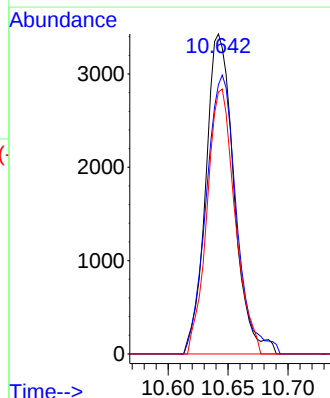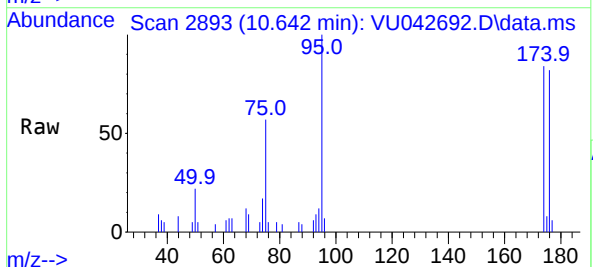

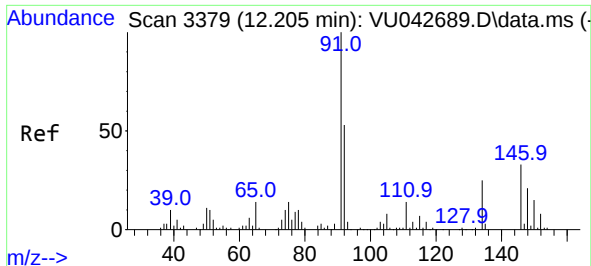

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.82 ug/l
 RT: 12.201 min Scan# 3378
 Delta R.T. -0.004 min
 Lab File: VU042692.D
 Acq: 17 Mar 2021 16:38

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0317WBL01

Tgt Ion:	152	Resp:	6261
Ion	Ratio	Lower	Upper
152	100		
115	61.7	0.0	271.0
150	147.6	0.0	633.0

