

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
 Data File : VU053262.D
 Acq On : 17 Mar 2023 13:16
 Operator : JC/MD
 Sample : 01929-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE6

Quant Time: Mar 18 01:51:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 18 01:49:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	132787	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	122366	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	56335	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	55411	45.232	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	90.460%
7) Chloroethane-d5	1.909	69	46602	47.030	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	94.060%
11) 1,1-Dichloroethene-d2	2.562	63	73653	34.707	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.420%
21) 2-Butanone-d5	4.610	46	74505	131.130	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	131.130%#
24) Chloroform-d	5.057	84	94917	47.042	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.080%
26) 1,2-Dichloroethane-d4	5.694	65	65135	51.980	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.960%
32) Benzene-d6	5.723	84	205191	51.699	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.400%
36) 1,2-Dichloropropane-d6	6.684	67	67664	52.822	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	105.640%
41) Toluene-d8	7.893	98	183132	49.559	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.120%
43) trans-1,3-Dichloroprop...	8.173	79	31425	49.722	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	99.440%
47) 2-Hexanone-d5	8.626	63	56672	141.511	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	141.510%#
56) 1,1,2,2-Tetrachloroeth...	10.751	84	93844	56.553	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	113.100%
66) 1,2-Dichlorobenzene-d4	12.189	152	58775	53.882	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.760%
Target Compounds						
13) Acetone	2.617	43	4291	6.631	ug/L	Qvalue 76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
Data File : VU053262.D
Acq On : 17 Mar 2023 13:16
Operator : JC/MD
Sample : 01929-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE6

Quant Time: Mar 18 01:51:24 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 18 01:49:30 2023
Response via : Initial Calibration

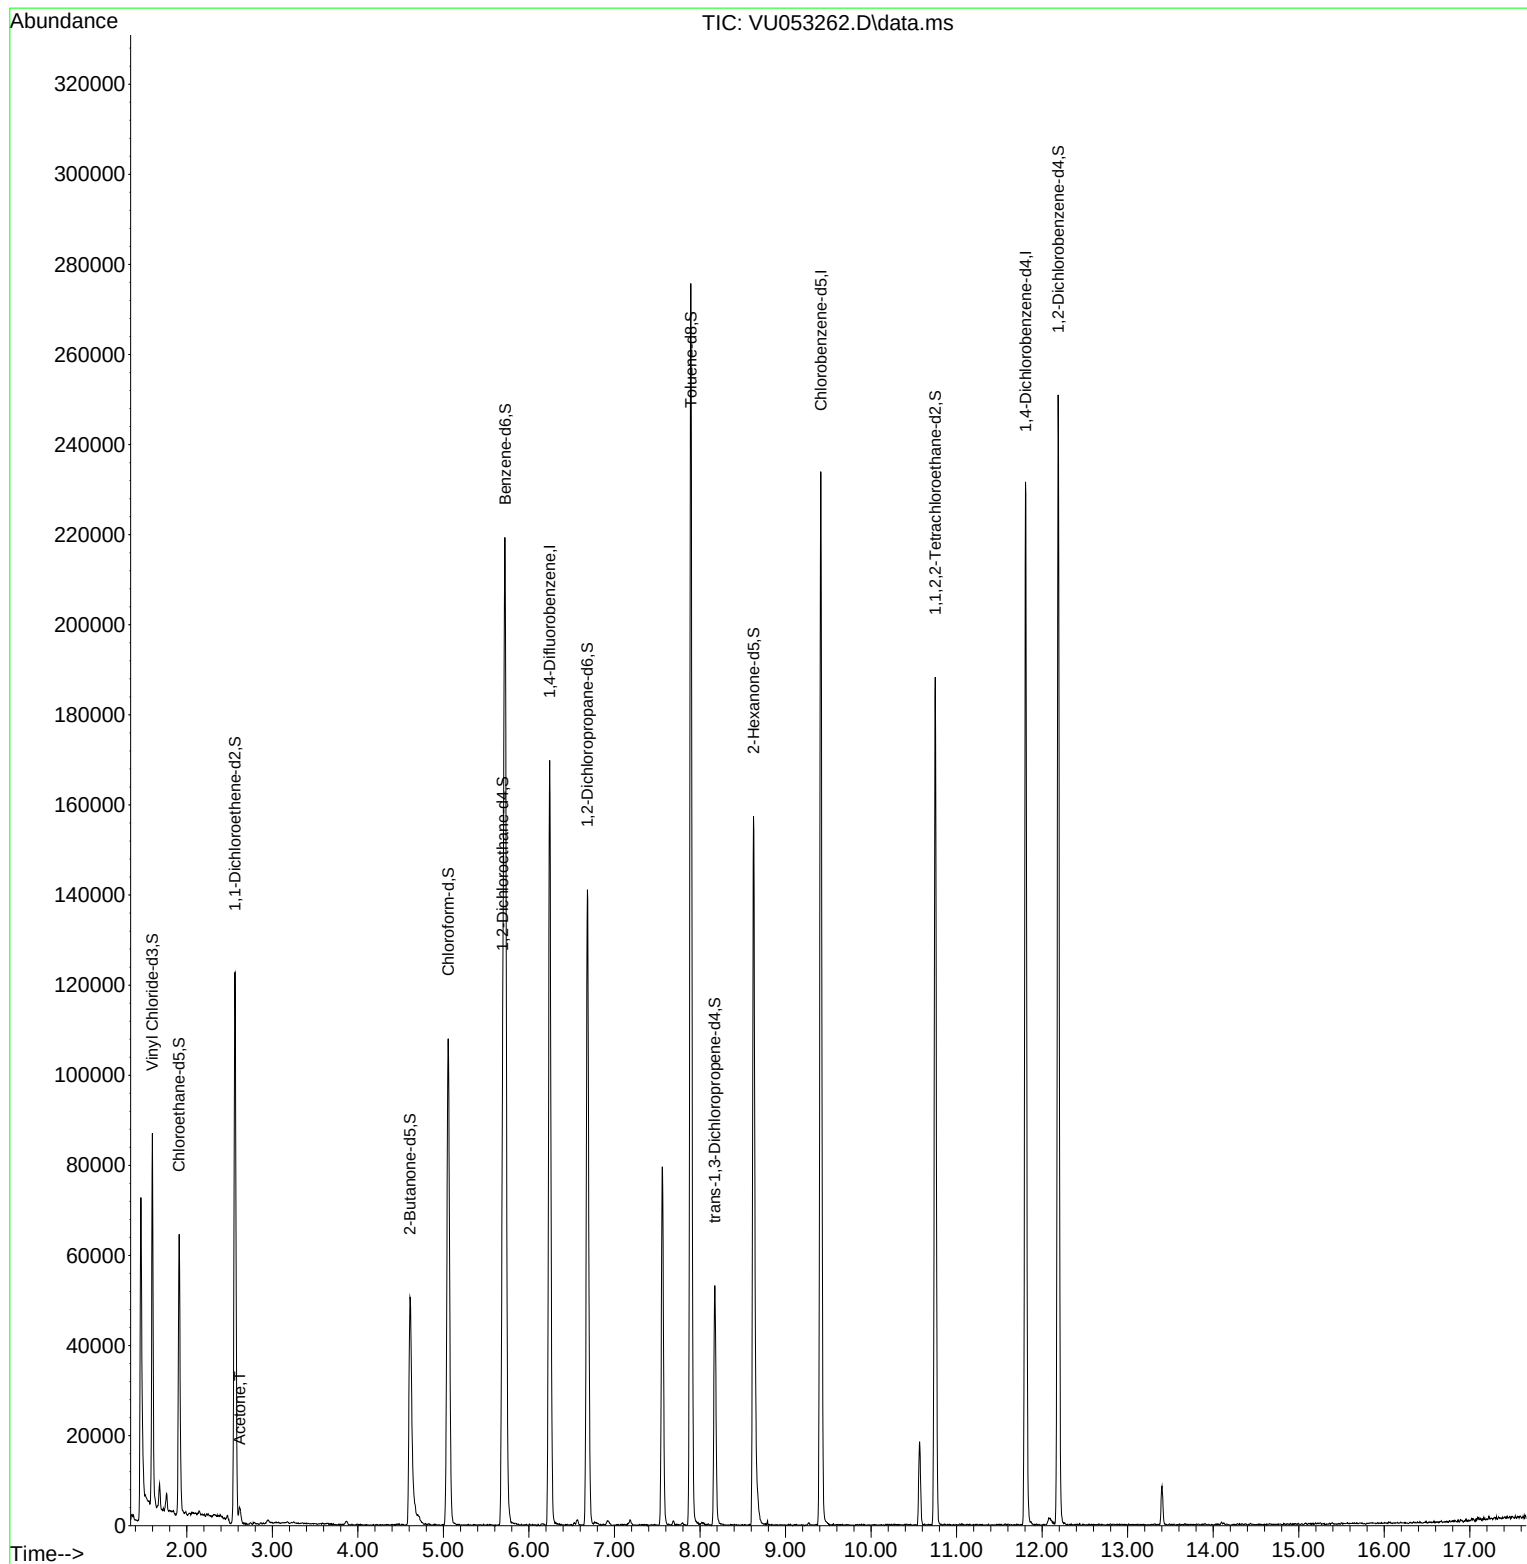

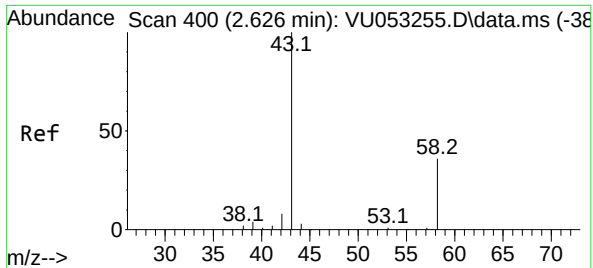

#13
 Acetone
 Concen: 6.631 ug/L
 RT: 2.617 min Scan# 397
 Delta R.T. -0.010 min
 Lab File: VU053262.D
 Acq: 17 Mar 2023 13:16

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE6

Tgt Ion: 43 Resp: 4291
 Ion Ratio Lower Upper
 43 100
 58 22.9 0.0 75.0

