

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
 Data File : VU053256.D
 Acq On : 17 Mar 2023 10:53
 Operator : JC/MD
 Sample : VU0317WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK052

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053256.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rVB	99606	112163	15.74%	2.208%
2	1.909	169	177	191	rBV	78105	104594	14.68%	2.059%
3	2.565	369	381	398	rBV	151947	244919	34.38%	4.821%
4	2.912	487	489	491	rBV	308	141	0.02%	0.003%
5	3.041	523	529	539	rVB5	1075	1721	0.24%	0.034%
6	3.176	564	571	573	rBV2	732	813	0.11%	0.016%
7	3.912	799	800	803	rBV	147	60	0.01%	0.001%
8	3.977	817	820	825	rVB2	209	157	0.02%	0.003%
9	4.002	825	828	830	rBV2	185	120	0.02%	0.002%
10	4.112	860	862	864	rVB	167	66	0.01%	0.001%
11	4.327	926	929	931	rBV	138	61	0.01%	0.001%
12	4.340	931	933	936	rBV2	162	99	0.01%	0.002%
13	4.613	1007	1018	1047	rBV	51731	129728	18.21%	2.554%
14	4.851	1090	1092	1094	rBV	134	58	0.01%	0.001%
15	4.867	1094	1097	1101	rVB	210	155	0.02%	0.003%
16	4.916	1109	1112	1116	rBV	196	218	0.03%	0.004%
17	5.057	1140	1156	1179	rBV	129422	283552	39.80%	5.582%
18	5.234	1208	1211	1213	rBV	170	95	0.01%	0.002%
19	5.292	1227	1229	1231	rBV	136	76	0.01%	0.001%
20	5.719	1341	1362	1385	rBV2	262965	712410	100.00%	14.024%
21	6.038	1458	1461	1466	rBV2	324	379	0.05%	0.007%
22	6.144	1489	1494	1497	rBV2	209	248	0.03%	0.005%
23	6.243	1512	1525	1546	rBV	197405	369280	51.84%	7.270%
24	6.481	1596	1599	1600	rBV	196	89	0.01%	0.002%
25	6.526	1609	1613	1617	rBV3	722	756	0.11%	0.015%
26	6.597	1631	1635	1637	rBV	155	153	0.02%	0.003%
27	6.684	1649	1662	1682	rBV	163449	319988	44.92%	6.299%
28	6.764	1686	1687	1690	rVV2	363	196	0.03%	0.004%
29	6.803	1693	1699	1703	rBV4	409	398	0.06%	0.008%
30	6.880	1720	1723	1725	rBV	172	95	0.01%	0.002%
31	6.912	1732	1733	1734	rBV	218	66	0.01%	0.001%
32	6.964	1748	1749	1754	rVB	298	217	0.03%	0.004%
33	6.993	1755	1758	1761	rBV	175	171	0.02%	0.003%
34	7.047	1773	1775	1777	rVB	268	142	0.02%	0.003%
35	7.067	1777	1781	1784	rBV	245	253	0.04%	0.005%
36	7.179	1810	1816	1817	rBV3	1037	767	0.11%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
 Data File : VU053256.D
 Acq On : 17 Mar 2023 10:53
 Operator : JC/MD
 Sample : VU0317WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK052

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	7.269	1840	1844	1846	rBV	201	169	0.02%	0.003%
38	7.333	1862	1864	1866	rVB	164	64	0.01%	0.001%
39	7.420	1886	1891	1892	rBV	168	162	0.02%	0.003%
40	7.562	1922	1935	1956	rBV	97138	167191	23.47%	3.291%
41	7.690	1969	1975	1978	rBV5	699	837	0.12%	0.016%
42	7.742	1986	1991	1998	rVB2	327	508	0.07%	0.010%
43	7.777	1998	2002	2003	rBV	304	199	0.03%	0.004%
44	7.822	2014	2016	2019	rBV2	283	205	0.03%	0.004%
45	7.893	2022	2038	2057	rBV	327962	562527	78.96%	11.074%
46	8.095	2099	2101	2103	rVB	276	109	0.02%	0.002%
47	8.128	2103	2111	2114	rBV2	383	538	0.08%	0.011%
48	8.176	2114	2126	2141	rVV	66231	110427	15.50%	2.174%
49	8.266	2151	2154	2160	rBV2	308	277	0.04%	0.005%
50	8.304	2163	2166	2167	rBV	172	116	0.02%	0.002%
51	8.382	2187	2190	2195	rBV	174	130	0.02%	0.003%
52	8.456	2207	2213	2215	rBV	206	257	0.04%	0.005%
53	8.536	2235	2238	2240	rBV	153	130	0.02%	0.003%
54	8.626	2251	2266	2293	rBV2	154152	283439	39.79%	5.580%
55	8.764	2306	2309	2312	rVB	316	178	0.02%	0.004%
56	8.816	2323	2325	2328	rVB2	285	203	0.03%	0.004%
57	8.841	2331	2333	2336	rVV	189	104	0.01%	0.002%
58	9.050	2395	2398	2400	rVB2	189	106	0.01%	0.002%
59	9.079	2404	2407	2408	rBV2	168	76	0.01%	0.001%
60	9.253	2459	2461	2466	rVB	161	55	0.01%	0.001%
61	9.414	2498	2511	2536	rBV	268540	442241	62.08%	8.706%
62	9.558	2552	2556	2557	rVB2	228	131	0.02%	0.003%
63	9.571	2557	2560	2563	rBV	241	172	0.02%	0.003%
64	9.648	2582	2584	2588	rBV	144	84	0.01%	0.002%
65	9.693	2595	2598	2601	rVB	414	270	0.04%	0.005%
66	9.729	2605	2609	2612	rBV	232	236	0.03%	0.005%
67	9.883	2654	2657	2659	rBV	165	92	0.01%	0.002%
68	10.002	2692	2694	2697	rBV	152	71	0.01%	0.001%
69	10.070	2713	2715	2716	rBV	126	54	0.01%	0.001%
70	10.099	2720	2724	2728	rBV2	318	375	0.05%	0.007%
71	10.372	2807	2809	2812	rVB	195	97	0.01%	0.002%
72	10.636	2885	2891	2896	rVB3	819	997	0.14%	0.020%
73	10.658	2896	2898	2902	rBV	95	76	0.01%	0.001%
74	10.751	2915	2927	2945	rBV	209989	330915	46.45%	6.514%
75	10.883	2966	2968	2972	rBV2	224	138	0.02%	0.003%
76	10.941	2983	2986	2988	rBV	193	150	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
 Data File : VU053256.D
 Acq On : 17 Mar 2023 10:53
 Operator : JC/MD
 Sample : VU0317WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK052

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	11.230	3075	3076	3082	rVB	185	63	0.01%	0.001%
78	11.468	3145	3150	3151	rBV2	717	625	0.09%	0.012%
79	11.510	3161	3163	3167	rBV	207	85	0.01%	0.002%
80	11.558	3175	3178	3181	rBV	177	86	0.01%	0.002%
81	11.693	3219	3220	3224	rVB	192	55	0.01%	0.001%
82	11.742	3231	3235	3237	rBV	441	330	0.05%	0.006%
83	11.806	3244	3255	3272	rBV	265617	416418	58.45%	8.197%
84	12.073	3335	3338	3341	rVB	250	120	0.02%	0.002%
85	12.108	3347	3349	3356	rVB	237	138	0.02%	0.003%
86	12.189	3362	3374	3393	rBV	286746	462378	64.90%	9.102%
87	12.298	3405	3408	3413	rVB	243	173	0.02%	0.003%
88	12.343	3419	3422	3424	rVB	152	63	0.01%	0.001%
89	12.873	3584	3587	3589	rBV	241	142	0.02%	0.003%
90	13.214	3690	3693	3694	rBV2	402	234	0.03%	0.005%
91	13.250	3702	3704	3708	rBV2	199	132	0.02%	0.003%
92	13.844	3885	3889	3895	rVB4	2053	1769	0.25%	0.035%
93	14.089	3957	3965	3975	rBV2	3280	5137	0.72%	0.101%
94	14.269	4019	4021	4023	rBV	164	65	0.01%	0.001%
95	14.333	4033	4041	4048	rVB3	2008	2439	0.34%	0.048%
96	14.471	4082	4084	4086	rBV	186	75	0.01%	0.001%
97	15.002	4244	4249	4253	rBV3	398	383	0.05%	0.008%
98	15.060	4265	4267	4271	rVB	261	131	0.02%	0.003%
99	15.079	4271	4273	4274	rBV	196	105	0.01%	0.002%
100	15.134	4287	4290	4292	rBV	243	174	0.02%	0.003%




Sum of corrected areas: 5079830

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
Data File : VU053256.D
Acq On : 17 Mar 2023 10:53
Operator : JC/MD
Sample : VU0317WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK052

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

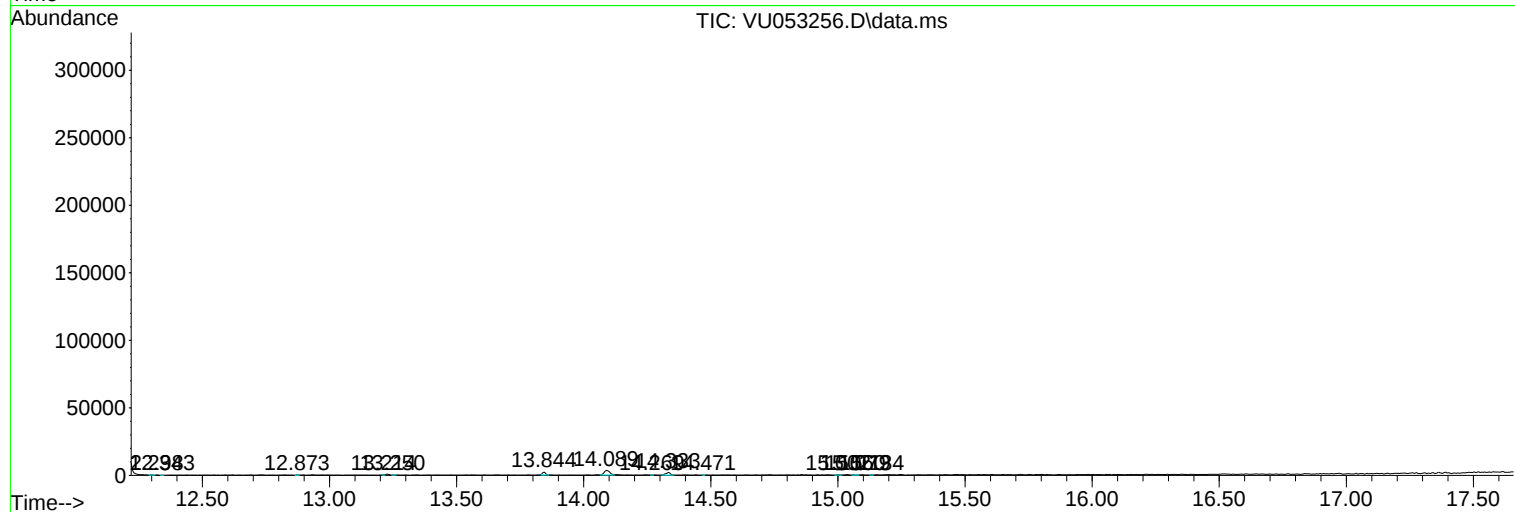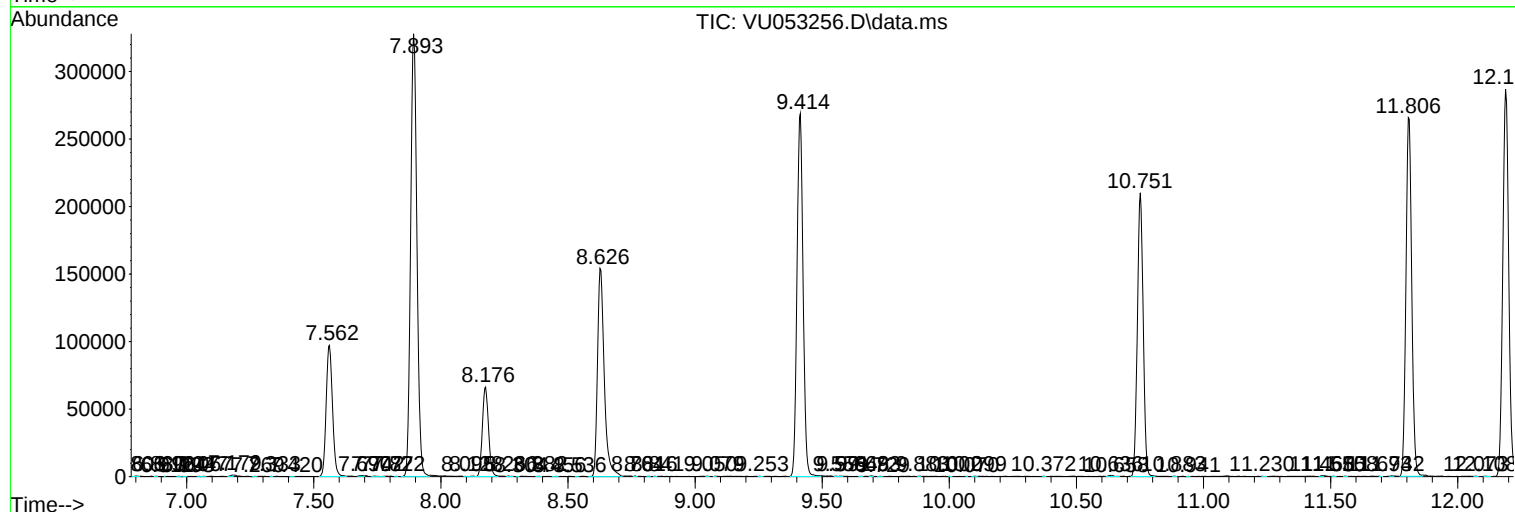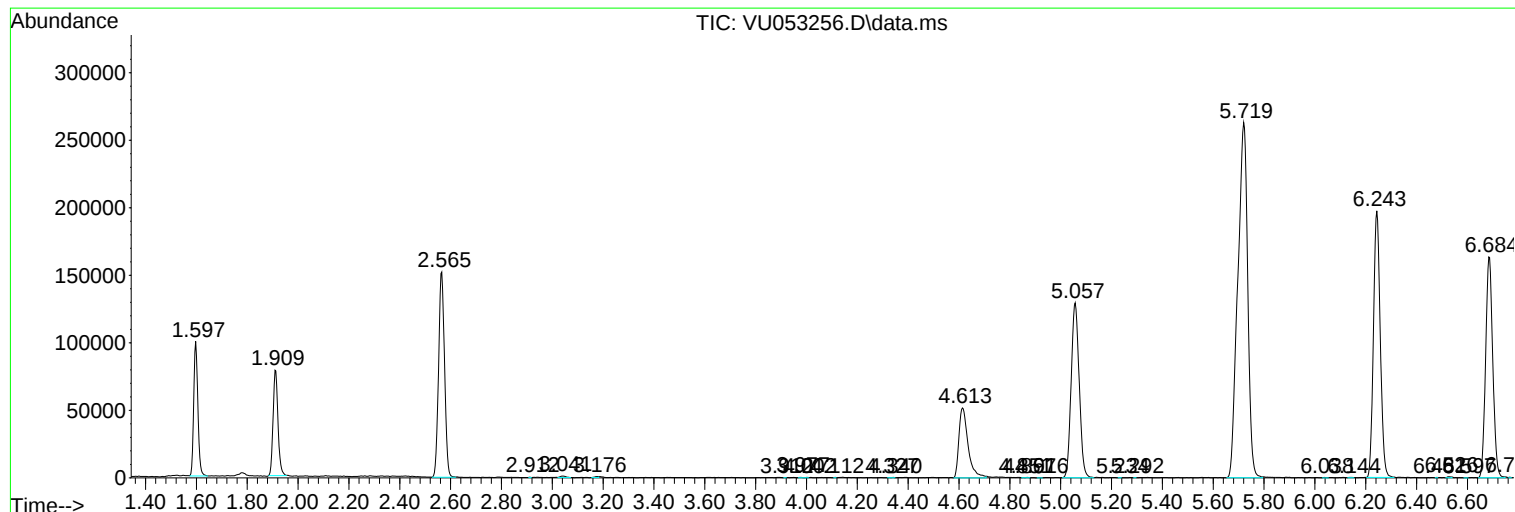

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
Data File : VU053256.D
Acq On : 17 Mar 2023 10:53
Operator : JC/MD
Sample : VU0317WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK052

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
Data File : VU053256.D
Acq On : 17 Mar 2023 10:53
Operator : JC/MD
Sample : VU0317WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK052

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------