

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
 Data File : VU053257.D
 Acq On : 17 Mar 2023 11:18
 Operator : JC/MD
 Sample : 01929-17DL 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFF0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053257.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	99	rVB	100975	120215	17.26%	2.165%
2	1.913	169	178	195	rBV	74780	101044	14.51%	1.820%
3	2.565	369	381	396	rVB	149719	240192	34.48%	4.326%
4	2.842	464	467	469	rBV2	234	141	0.02%	0.003%
5	3.491	666	669	671	rBV	157	71	0.01%	0.001%
6	3.710	734	737	742	rVB2	207	160	0.02%	0.003%
7	3.970	815	818	820	rVB	183	74	0.01%	0.001%
8	4.093	853	856	860	rVB	335	242	0.03%	0.004%
9	4.109	860	861	862	rBV	148	45	0.01%	0.001%
10	4.192	882	887	890	rBV2	267	280	0.04%	0.005%
11	4.308	920	923	925	rBV	171	152	0.02%	0.003%
12	4.318	925	926	927	rVV	111	30	0.00%	0.001%
13	4.485	973	978	980	rBV	232	237	0.03%	0.004%
14	4.527	990	991	992	rBV	119	34	0.00%	0.001%
15	4.617	1007	1019	1023	rBV2	52906	96107	13.80%	1.731%
16	4.871	1096	1098	1100	rBV	175	88	0.01%	0.002%
17	4.935	1115	1118	1122	rBV	170	105	0.02%	0.002%
18	5.057	1140	1156	1179	rBV	127920	278664	40.00%	5.019%
19	5.279	1222	1225	1227	rBV	164	129	0.02%	0.002%
20	5.343	1242	1245	1249	rBV	173	115	0.02%	0.002%
21	5.388	1257	1259	1261	rVB	198	98	0.01%	0.002%
22	5.469	1282	1284	1288	rBV	139	63	0.01%	0.001%
23	5.494	1289	1292	1296	rVB2	213	141	0.02%	0.003%
24	5.510	1296	1297	1299	rBV	112	43	0.01%	0.001%
25	5.719	1342	1362	1382	rBV2	260276	696595	100.00%	12.546%
26	5.887	1410	1414	1417	rVB2	362	223	0.03%	0.004%
27	5.941	1429	1431	1433	rBV	163	115	0.02%	0.002%
28	6.073	1470	1472	1473	rBV	153	46	0.01%	0.001%
29	6.244	1512	1525	1545	rBV	199317	379448	54.47%	6.834%
30	6.420	1578	1580	1585	rVB	215	128	0.02%	0.002%
31	6.536	1603	1616	1640	rBV	286771	534102	76.67%	9.620%
32	6.623	1640	1643	1648	rVB4	790	591	0.08%	0.011%
33	6.684	1649	1662	1686	rBV	162612	314200	45.11%	5.659%
34	6.793	1691	1696	1701	rBV2	334	364	0.05%	0.007%
35	6.816	1701	1703	1710	rVB	238	157	0.02%	0.003%
36	7.009	1761	1763	1766	rVB	216	116	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
 Data File : VU053257.D
 Acq On : 17 Mar 2023 11:18
 Operator : JC/MD
 Sample : 01929-17DL 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFF0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	7.089	1786	1788	1792	rVB2	171	97	0.01%	0.002%
38	7.108	1792	1794	1797	rBV	170	121	0.02%	0.002%
39	7.144	1803	1805	1806	rBV	244	123	0.02%	0.002%
40	7.182	1811	1817	1828	rVB4	1090	1872	0.27%	0.034%
41	7.340	1864	1866	1867	rBV	133	35	0.01%	0.001%
42	7.391	1879	1882	1887	rBV2	225	159	0.02%	0.003%
43	7.440	1892	1897	1903	rVB	321	377	0.05%	0.007%
44	7.475	1904	1908	1910	rBB	165	130	0.02%	0.002%
45	7.491	1911	1913	1914	rBV	137	75	0.01%	0.001%
46	7.562	1923	1935	1953	rBV	93106	160951	23.11%	2.899%
47	7.668	1966	1968	1969	rBV	167	86	0.01%	0.002%
48	7.780	2001	2003	2005	rBV	128	51	0.01%	0.001%
49	7.893	2025	2038	2058	rBV	329502	555635	79.76%	10.007%
50	8.073	2091	2094	2096	rBV2	332	200	0.03%	0.004%
51	8.086	2096	2098	2100	rBV	214	108	0.02%	0.002%
52	8.125	2108	2110	2114	rBV	191	199	0.03%	0.004%
53	8.176	2114	2126	2147	rVV	64951	108613	15.59%	1.956%
54	8.327	2170	2173	2176	rBV	266	242	0.03%	0.004%
55	8.446	2208	2210	2213	rVB2	100	26	0.00%	0.000%
56	8.465	2214	2216	2221	rVB2	229	136	0.02%	0.002%
57	8.501	2225	2227	2229	rBV	145	59	0.01%	0.001%
58	8.629	2256	2267	2295	rBV2	147265	275308	39.52%	4.959%
59	9.205	2441	2446	2451	rBV	265	249	0.04%	0.004%
60	9.279	2466	2469	2474	rBV2	209	203	0.03%	0.004%
61	9.359	2488	2494	2496	rBV2	164	152	0.02%	0.003%
62	9.414	2499	2511	2530	rBV	276567	452670	64.98%	8.153%
63	9.568	2556	2559	2561	rBV	265	135	0.02%	0.002%
64	9.729	2607	2609	2611	rVB	164	49	0.01%	0.001%
65	9.858	2646	2649	2656	rVB2	230	226	0.03%	0.004%
66	10.147	2737	2739	2740	rBV2	136	34	0.00%	0.001%
67	10.301	2784	2787	2790	rBV2	171	120	0.02%	0.002%
68	10.337	2797	2798	2802	rBV	133	57	0.01%	0.001%
69	10.356	2802	2804	2806	rBV	197	102	0.01%	0.002%
70	10.478	2839	2842	2847	rBV2	236	157	0.02%	0.003%
71	10.751	2914	2927	2952	rVB	204826	321272	46.12%	5.786%
72	10.838	2952	2954	2964	rBV2	200	229	0.03%	0.004%
73	11.015	3006	3009	3015	rVB2	260	202	0.03%	0.004%
74	11.083	3028	3030	3036	rVB2	320	211	0.03%	0.004%
75	11.163	3053	3055	3056	rBV2	147	41	0.01%	0.001%
76	11.224	3072	3074	3076	rBV	189	110	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
 Data File : VU053257.D
 Acq On : 17 Mar 2023 11:18
 Operator : JC/MD
 Sample : 01929-17DL 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFF0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	11.314	3100	3102	3105	rVB	183	83	0.01%	0.001%
78	11.468	3146	3150	3156	rBV2	341	334	0.05%	0.006%
79	11.526	3165	3168	3170	rVB	231	151	0.02%	0.003%
80	11.597	3188	3190	3193	rBV	160	89	0.01%	0.002%
81	11.742	3232	3235	3239	rBV2	310	263	0.04%	0.005%
82	11.809	3244	3256	3282	rVV	274955	437087	62.75%	7.872%
83	11.964	3302	3304	3306	rBV2	130	78	0.01%	0.001%
84	12.189	3362	3374	3397	rBV	285213	467297	67.08%	8.416%
85	12.947	3608	3610	3612	rBV	229	145	0.02%	0.003%
86	13.285	3713	3715	3718	rBV2	185	134	0.02%	0.002%
87	14.028	3943	3946	3947	rBV	215	131	0.02%	0.002%
88	14.365	4049	4051	4053	rBV	263	134	0.02%	0.002%
89	14.433	4068	4072	4075	rBV2	255	216	0.03%	0.004%
90	14.510	4095	4096	4099	rBV	208	118	0.02%	0.002%
91	14.629	4130	4133	4135	rBV2	253	216	0.03%	0.004%
92	14.999	4247	4248	4251	rBV	202	146	0.02%	0.003%
93	15.398	4369	4372	4374	rBV2	306	220	0.03%	0.004%




Sum of corrected areas: 5552219

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
Data File : VU053257.D
Acq On : 17 Mar 2023 11:18
Operator : JC/MD
Sample : 01929-17DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFF0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

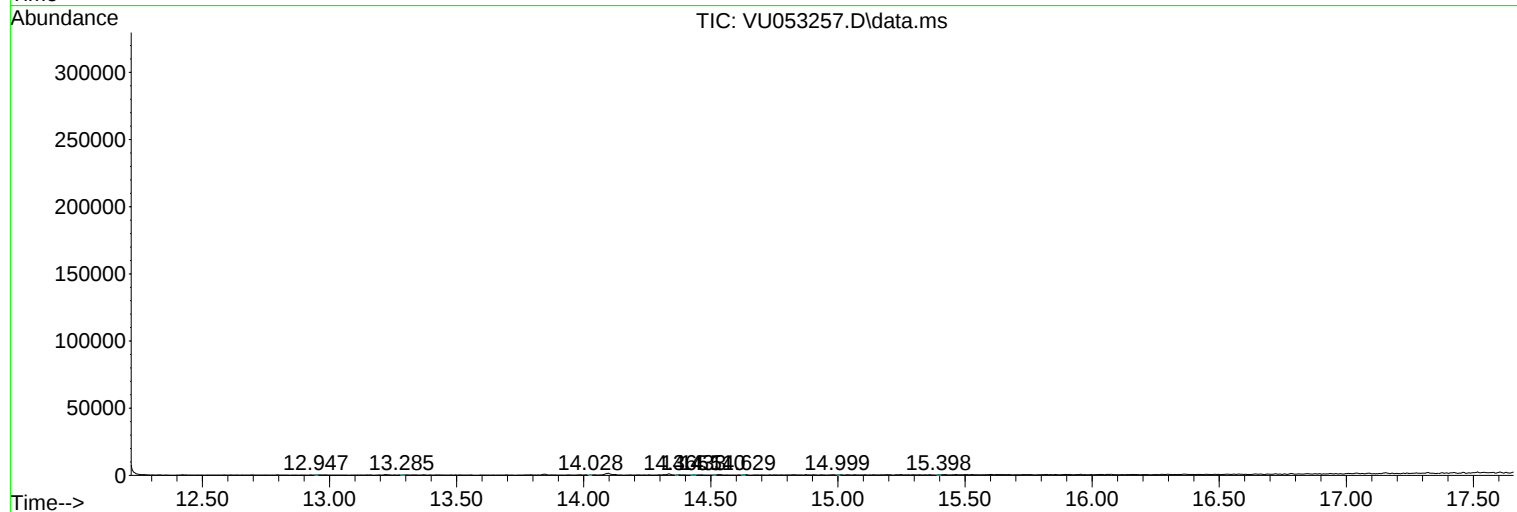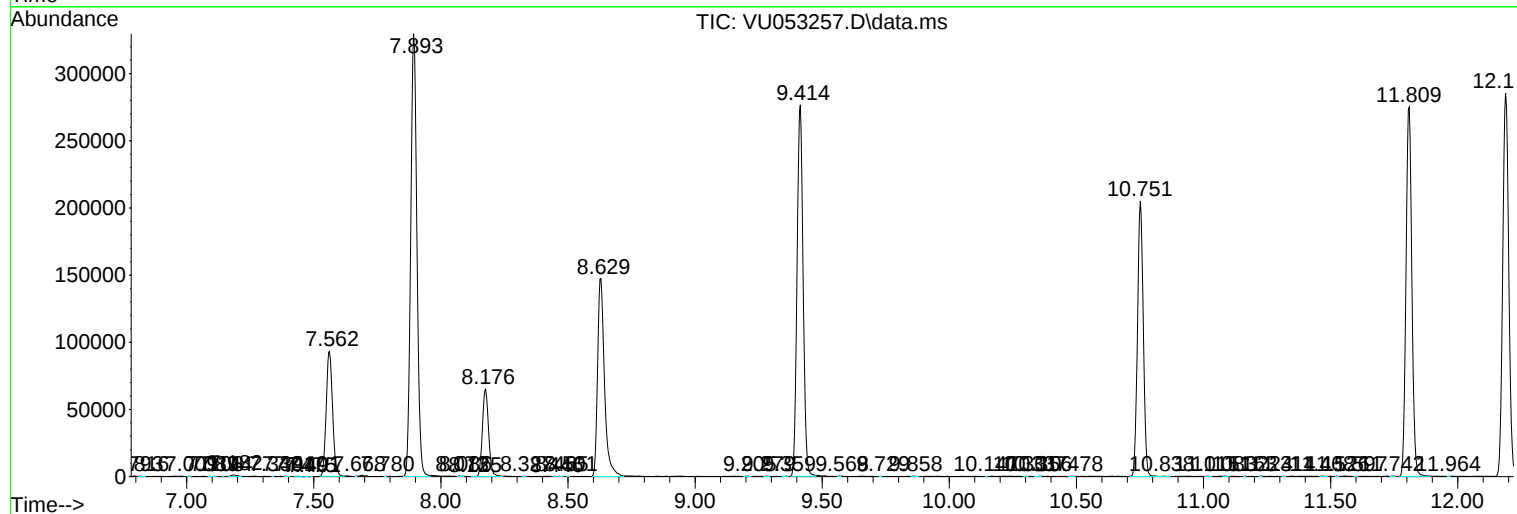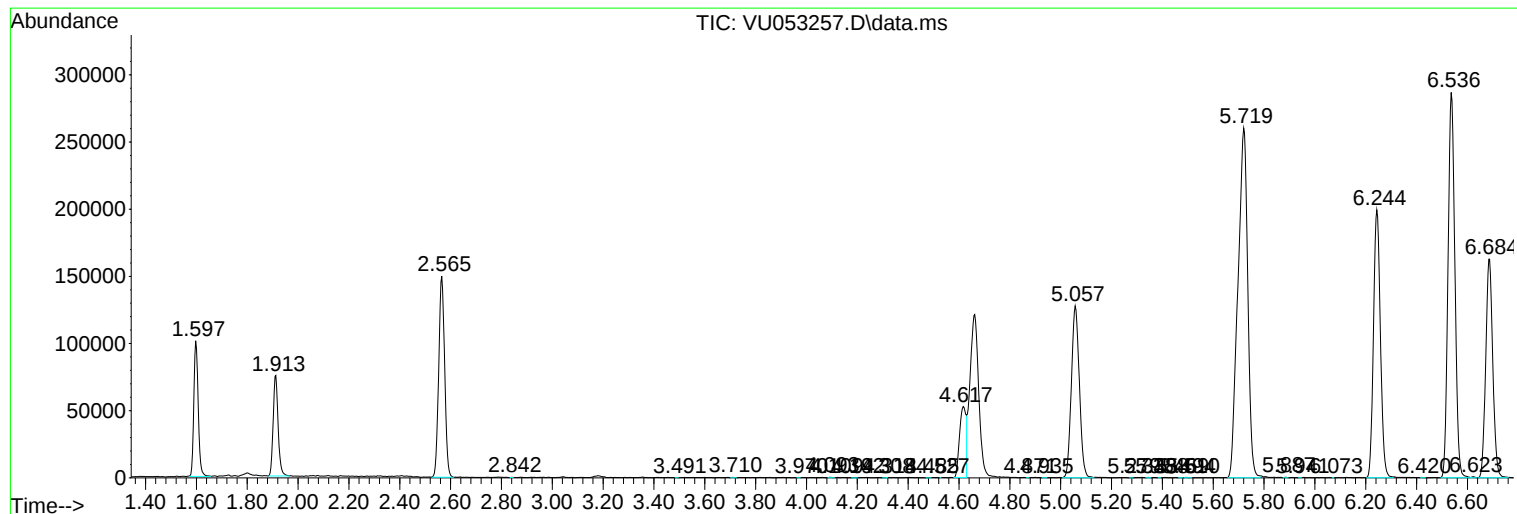

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
Data File : VU053257.D
Acq On : 17 Mar 2023 11:18
Operator : JC/MD
Sample : 01929-17DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFF0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
Data File : VU053257.D
Acq On : 17 Mar 2023 11:18
Operator : JC/MD
Sample : 01929-17DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFF0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------