

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
 Data File : VU053258.D
 Acq On : 17 Mar 2023 11:41
 Operator : JC/MD
 Sample : 01929-16DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M

Title : VOC Analysis

Signal : TIC: VU053258.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	98	rVB2	164252	204747	30.40%	4.128%
2	1.909	169	177	193	rBV	74200	100183	14.88%	2.020%
3	2.565	369	381	397	rVB	142849	233546	34.68%	4.709%
4	2.954	499	502	503	rBV	176	81	0.01%	0.002%
5	3.003	515	517	523	rBV	197	152	0.02%	0.003%
6	3.028	523	525	526	rBV	270	138	0.02%	0.003%
7	3.353	619	626	631	rVB3	849	1065	0.16%	0.021%
8	3.430	647	650	654	rVV	197	131	0.02%	0.003%
9	3.450	654	656	660	rVB	225	112	0.02%	0.002%
10	4.179	881	883	887	rVB2	173	106	0.02%	0.002%
11	4.289	914	917	921	rBV2	186	132	0.02%	0.003%
12	4.321	925	927	930	rVB	148	65	0.01%	0.001%
13	4.347	933	935	938	rVB	168	110	0.02%	0.002%
14	4.363	938	940	942	rBV2	177	124	0.02%	0.003%
15	4.472	971	974	975	rBV2	165	78	0.01%	0.002%
16	4.614	1005	1018	1020	rBV2	56646	79830	11.85%	1.609%
17	4.922	1112	1114	1118	rVB	190	90	0.01%	0.002%
18	5.057	1139	1156	1183	rBV2	122644	269588	40.03%	5.435%
19	5.173	1190	1192	1195	rVB2	238	114	0.02%	0.002%
20	5.192	1195	1198	1202	rBV2	168	135	0.02%	0.003%
21	5.298	1229	1231	1232	rBV2	139	66	0.01%	0.001%
22	5.536	1301	1305	1308	rBV2	215	194	0.03%	0.004%
23	5.646	1337	1339	1341	rBV	140	96	0.01%	0.002%
24	5.720	1341	1362	1389	rVV2	251710	673460	100.00%	13.578%
25	6.244	1511	1525	1548	rBV	196097	368321	54.69%	7.426%
26	6.427	1578	1582	1585	rBV2	365	246	0.04%	0.005%
27	6.443	1585	1587	1589	rBV2	161	111	0.02%	0.002%
28	6.536	1608	1616	1627	rVB6	3902	7147	1.06%	0.144%
29	6.597	1631	1635	1638	rVB	293	239	0.04%	0.005%
30	6.613	1638	1640	1643	rVB	283	158	0.02%	0.003%
31	6.630	1643	1645	1647	rBV	250	133	0.02%	0.003%
32	6.684	1648	1662	1685	rBV	159039	305149	45.31%	6.152%
33	6.797	1695	1697	1705	rVB4	448	461	0.07%	0.009%
34	6.880	1719	1723	1725	rBV2	166	108	0.02%	0.002%
35	6.903	1726	1730	1737	rVV2	247	299	0.04%	0.006%
36	7.054	1774	1777	1778	rBV	181	117	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
 Data File : VU053258.D
 Acq On : 17 Mar 2023 11:41
 Operator : JC/MD
 Sample : 01929-16DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	7.154	1805	1808	1809	rBV	170	116	0.02%	0.002%
38	7.173	1812	1814	1817	rBV2	584	449	0.07%	0.009%
39	7.273	1842	1845	1846	rBV	148	100	0.01%	0.002%
40	7.282	1846	1848	1853	rVV	260	200	0.03%	0.004%
41	7.311	1853	1857	1863	rVB2	426	429	0.06%	0.009%
42	7.343	1864	1867	1869	rBV	163	130	0.02%	0.003%
43	7.356	1869	1871	1875	rBV	169	89	0.01%	0.002%
44	7.420	1883	1891	1895	rBV2	288	487	0.07%	0.010%
45	7.504	1914	1917	1919	rVB2	181	101	0.01%	0.002%
46	7.562	1923	1935	1958	rVB2	88287	156742	23.27%	3.160%
47	7.668	1966	1968	1969	rBV	158	68	0.01%	0.001%
48	7.684	1969	1973	1980	rVB4	936	1143	0.17%	0.023%
49	7.732	1986	1988	1991	rBB	143	99	0.01%	0.002%
50	7.755	1992	1995	1998	rBV	168	178	0.03%	0.004%
51	7.893	2024	2038	2059	rBV	312757	536781	79.70%	10.822%
52	8.067	2090	2092	2098	rVB2	198	154	0.02%	0.003%
53	8.118	2106	2108	2109	rBV2	160	70	0.01%	0.001%
54	8.173	2115	2125	2139	rBV	63612	104054	15.45%	2.098%
55	8.292	2160	2162	2165	rVB	199	68	0.01%	0.001%
56	8.330	2173	2174	2175	rBV	209	63	0.01%	0.001%
57	8.385	2189	2191	2194	rVB	267	172	0.03%	0.003%
58	8.401	2194	2196	2197	rBV	233	89	0.01%	0.002%
59	8.591	2253	2255	2256	rBV	158	63	0.01%	0.001%
60	8.626	2256	2266	2293	rBV2	150114	277262	41.17%	5.590%
61	8.774	2309	2312	2313	rBV	203	120	0.02%	0.002%
62	8.803	2318	2321	2326	rVB	242	180	0.03%	0.004%
63	8.851	2334	2336	2342	rVB2	179	176	0.03%	0.004%
64	8.990	2376	2379	2380	rBV2	136	62	0.01%	0.001%
65	9.002	2380	2383	2384	rBV	195	90	0.01%	0.002%
66	9.096	2409	2412	2415	rBV2	173	122	0.02%	0.002%
67	9.350	2488	2491	2493	rBV	155	68	0.01%	0.001%
68	9.411	2498	2510	2532	rBV	263810	442724	65.74%	8.926%
69	9.523	2542	2545	2550	rVB3	369	290	0.04%	0.006%
70	9.565	2554	2558	2559	rBV2	170	129	0.02%	0.003%
71	9.636	2578	2580	2587	rVB	184	108	0.02%	0.002%
72	9.793	2627	2629	2632	rBV2	154	90	0.01%	0.002%
73	9.854	2642	2648	2651	rBV	177	249	0.04%	0.005%
74	9.896	2659	2661	2665	rBV2	228	157	0.02%	0.003%
75	10.105	2724	2726	2728	rBV	260	147	0.02%	0.003%
76	10.340	2795	2799	2800	rBV	198	119	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
 Data File : VU053258.D
 Acq On : 17 Mar 2023 11:41
 Operator : JC/MD
 Sample : 01929-16DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.481	2840	2843	2847	rBV	265	239	0.04%	0.005%
78	10.591	2874	2877	2880	rBV2	178	162	0.02%	0.003%
79	10.752	2915	2927	2950	rBV	200087	319533	47.45%	6.442%
80	10.954	2988	2990	2991	rBV	189	85	0.01%	0.002%
81	11.305	3098	3099	3102	rVB	191	97	0.01%	0.002%
82	11.497	3156	3159	3160	rBV	184	84	0.01%	0.002%
83	11.694	3218	3220	3222	rBV	186	75	0.01%	0.002%
84	11.806	3243	3255	3275	rBV	266175	420799	62.48%	8.484%
85	11.928	3291	3293	3295	rBV	191	73	0.01%	0.001%
86	12.189	3362	3374	3393	rBV	281014	444735	66.04%	8.967%
87	12.803	3563	3565	3567	rBV	193	73	0.01%	0.001%
88	13.224	3694	3696	3700	rBV	262	172	0.03%	0.003%
89	13.263	3705	3708	3710	rBV	163	101	0.01%	0.002%
90	13.378	3740	3744	3746	rBV	279	196	0.03%	0.004%
91	13.552	3796	3798	3800	rBV	217	94	0.01%	0.002%
92	13.674	3834	3836	3840	rBV	244	178	0.03%	0.004%
93	13.800	3872	3875	3878	rVB	245	157	0.02%	0.003%
94	13.816	3878	3880	3883	rBV	302	171	0.03%	0.003%
95	13.903	3904	3907	3913	rBV2	245	285	0.04%	0.006%
96	13.954	3920	3923	3926	rBV	204	140	0.02%	0.003%
97	14.028	3945	3946	3947	rBV	227	80	0.01%	0.002%
98	14.095	3960	3967	3975	rBV	782	1346	0.20%	0.027%
99	14.282	4023	4025	4027	rBV2	253	141	0.02%	0.003%
100	14.941	4227	4230	4232	rBV	227	166	0.02%	0.003%




Sum of corrected areas: 4959952

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
Data File : VU053258.D
Acq On : 17 Mar 2023 11:41
Operator : JC/MD
Sample : 01929-16DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

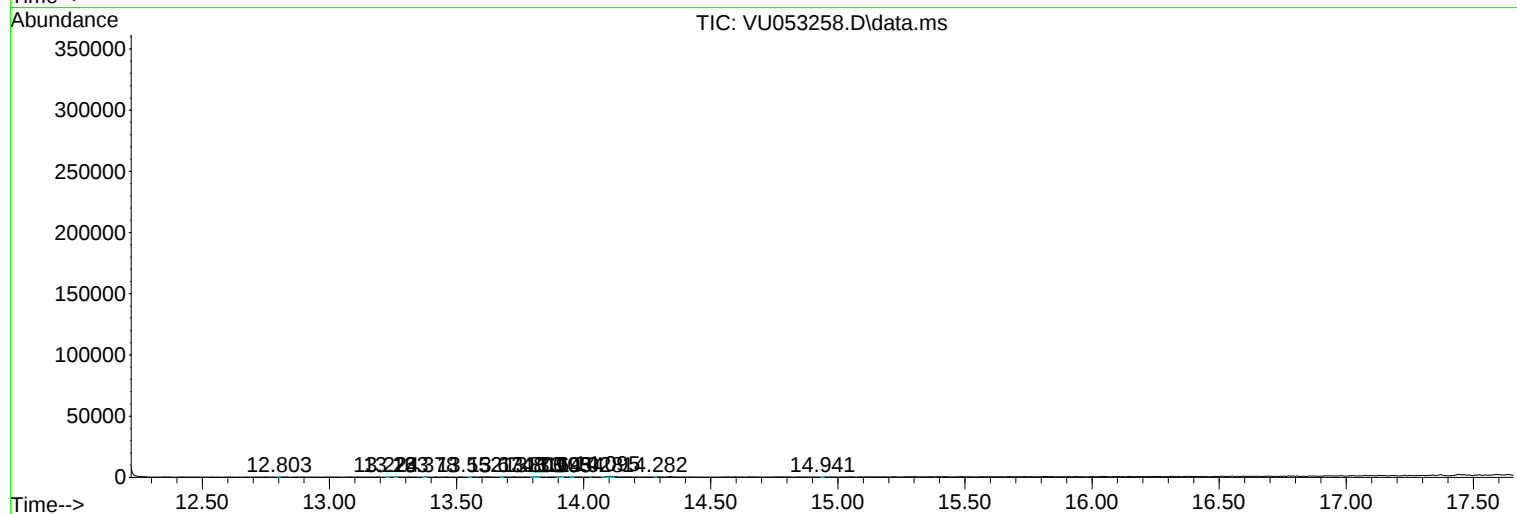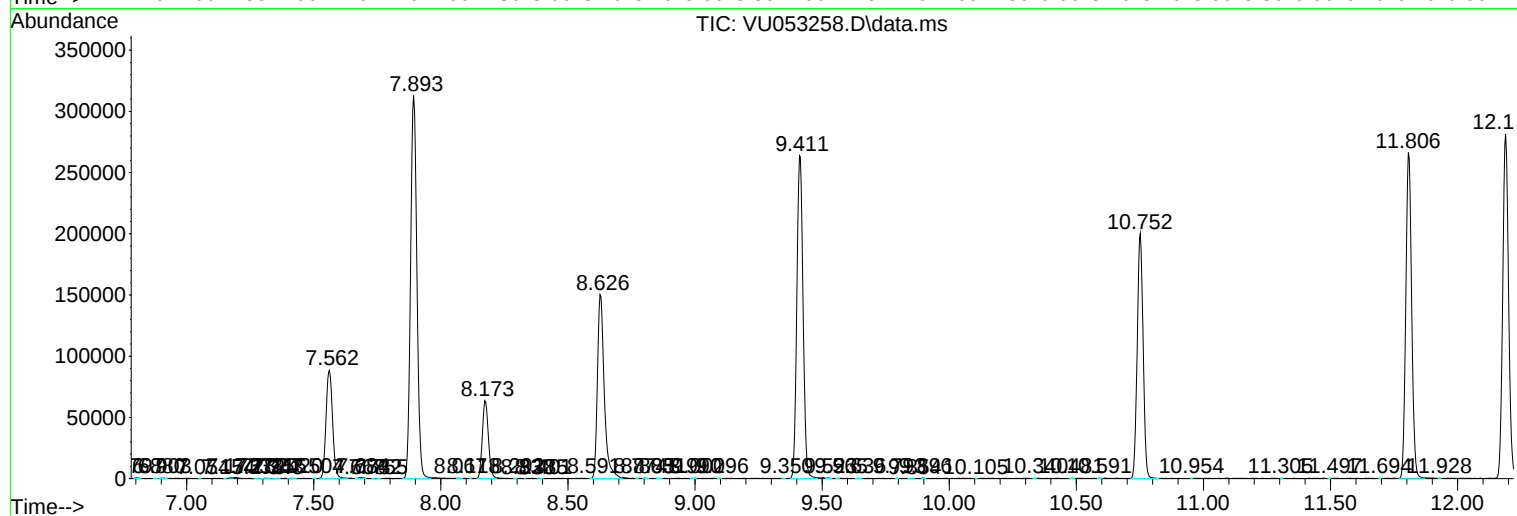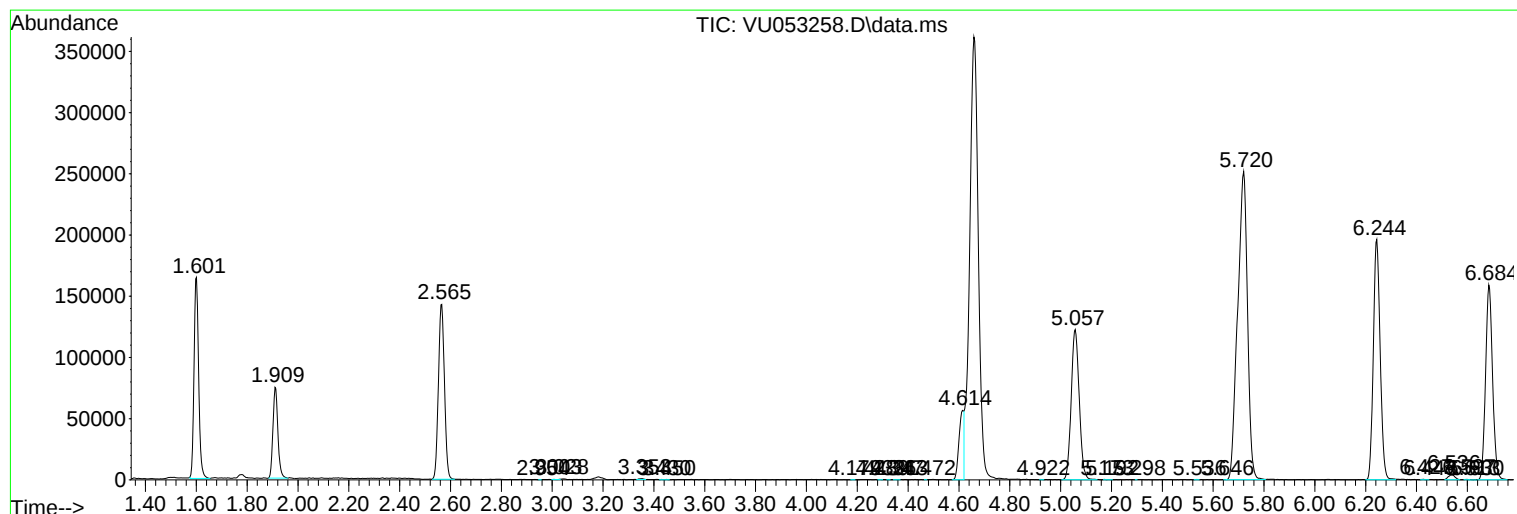

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
Data File : VU053258.D
Acq On : 17 Mar 2023 11:41
Operator : JC/MD
Sample : 01929-16DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
Data File : VU053258.D
Acq On : 17 Mar 2023 11:41
Operator : JC/MD
Sample : 01929-16DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------