

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
 Data File : VU053280.D
 Acq On : 17 Mar 2023 20:47
 Operator : JC/MD
 Sample : VU0317WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK053

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053280.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	98	rVB	90106	101261	15.87%	2.192%
2	1.909	169	177	198	rVB	67699	93502	14.65%	2.024%
3	2.562	369	380	398	rBV	130460	212768	33.34%	4.607%
4	3.041	521	529	538	rBV2	2991	5086	0.80%	0.110%
5	3.179	561	572	587	rVB	3294	7022	1.10%	0.152%
6	3.411	641	644	648	rVB	196	102	0.02%	0.002%
7	3.825	770	773	775	rVB2	239	139	0.02%	0.003%
8	3.954	809	813	815	rBV2	189	114	0.02%	0.002%
9	4.018	831	833	834	rBV2	144	41	0.01%	0.001%
10	4.034	835	838	845	rVB	264	208	0.03%	0.005%
11	4.247	901	904	905	rBV	158	73	0.01%	0.002%
12	4.276	909	913	916	rBV2	205	164	0.03%	0.004%
13	4.613	1006	1018	1040	rBV	49855	117542	18.42%	2.545%
14	4.883	1099	1102	1107	rBV2	385	305	0.05%	0.007%
15	4.999	1129	1138	1140	rBV	197	328	0.05%	0.007%
16	5.057	1140	1156	1178	rVV	114988	254740	39.92%	5.515%
17	5.198	1198	1200	1201	rBV	135	52	0.01%	0.001%
18	5.292	1228	1229	1230	rBV	111	24	0.00%	0.001%
19	5.369	1251	1253	1254	rBV	131	58	0.01%	0.001%
20	5.404	1262	1264	1269	rVB	255	178	0.03%	0.004%
21	5.436	1270	1274	1276	rBV	214	202	0.03%	0.004%
22	5.485	1287	1289	1290	rBV	138	38	0.01%	0.001%
23	5.523	1298	1301	1303	rBV	160	71	0.01%	0.002%
24	5.719	1342	1362	1386	rBV2	234740	638119	100.00%	13.816%
25	5.903	1417	1419	1421	rBV2	281	166	0.03%	0.004%
26	6.038	1459	1461	1465	rBV	151	89	0.01%	0.002%
27	6.067	1468	1470	1471	rBV	132	58	0.01%	0.001%
28	6.176	1502	1504	1507	rVB2	176	120	0.02%	0.003%
29	6.243	1511	1525	1555	rVV	187076	347462	54.45%	7.523%
30	6.388	1566	1570	1573	rBV2	178	158	0.02%	0.003%
31	6.481	1598	1599	1601	rBV2	213	62	0.01%	0.001%
32	6.520	1608	1611	1612	rBV	357	197	0.03%	0.004%
33	6.597	1633	1635	1636	rBV	131	38	0.01%	0.001%
34	6.684	1648	1662	1682	rBV	147383	289121	45.31%	6.260%
35	6.806	1696	1700	1703	rVB	264	194	0.03%	0.004%
36	6.854	1714	1715	1717	rVB	233	47	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
 Data File : VU053280.D
 Acq On : 17 Mar 2023 20:47
 Operator : JC/MD
 Sample : VU0317WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK053

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.874	1719	1721	1723	rVB	135	52	0.01%	0.001%
38	6.903	1728	1730	1738	rBV	260	342	0.05%	0.007%
39	6.931	1738	1739	1740	rBV	120	29	0.00%	0.001%
40	7.076	1778	1784	1785	rBV	286	288	0.05%	0.006%
41	7.144	1802	1805	1809	rBV	219	244	0.04%	0.005%
42	7.185	1809	1818	1827	rVB4	1161	2044	0.32%	0.044%
43	7.243	1834	1836	1839	rBB	189	125	0.02%	0.003%
44	7.263	1840	1842	1847	rBV	199	211	0.03%	0.005%
45	7.321	1858	1860	1864	rBB	145	126	0.02%	0.003%
46	7.356	1864	1871	1872	rBV	267	308	0.05%	0.007%
47	7.394	1880	1883	1886	rBV	173	107	0.02%	0.002%
48	7.562	1923	1935	1953	rBV	83985	144407	22.63%	3.127%
49	7.848	2021	2024	2025	rBV	266	133	0.02%	0.003%
50	7.893	2025	2038	2066	rVV	292950	500237	78.39%	10.831%
51	8.025	2077	2079	2080	rBV	242	118	0.02%	0.003%
52	8.073	2092	2094	2095	rBV	215	46	0.01%	0.001%
53	8.173	2115	2125	2147	rVB	57322	96225	15.08%	2.083%
54	8.250	2147	2149	2150	rBV	199	76	0.01%	0.002%
55	8.317	2168	2170	2171	rBV	136	60	0.01%	0.001%
56	8.404	2194	2197	2199	rVB	140	59	0.01%	0.001%
57	8.626	2255	2266	2294	rBV	147640	267937	41.99%	5.801%
58	8.780	2312	2314	2316	rBV	144	72	0.01%	0.002%
59	8.880	2343	2345	2348	rVB2	152	85	0.01%	0.002%
60	8.941	2361	2364	2368	rBV	194	222	0.03%	0.005%
61	9.025	2387	2390	2392	rBV	166	113	0.02%	0.002%
62	9.092	2409	2411	2414	rBV	146	61	0.01%	0.001%
63	9.227	2450	2453	2455	rBV	138	98	0.02%	0.002%
64	9.279	2463	2469	2473	rBV	235	349	0.05%	0.008%
65	9.330	2483	2485	2488	rVB	173	55	0.01%	0.001%
66	9.414	2498	2511	2534	rBV	252223	414325	64.93%	8.971%
67	9.571	2556	2560	2564	rBV	379	418	0.07%	0.009%
68	9.668	2584	2590	2594	rBV	255	368	0.06%	0.008%
69	9.803	2630	2632	2636	rVB	280	181	0.03%	0.004%
70	9.825	2636	2639	2640	rBV	302	221	0.03%	0.005%
71	9.980	2684	2687	2689	rBV	182	149	0.02%	0.003%
72	10.005	2694	2695	2696	rBV	246	82	0.01%	0.002%
73	10.034	2700	2704	2705	rBV	204	129	0.02%	0.003%
74	10.099	2721	2724	2728	rBV2	369	363	0.06%	0.008%
75	10.144	2736	2738	2740	rBV	130	57	0.01%	0.001%
76	10.324	2792	2794	2796	rBV	156	104	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
 Data File : VU053280.D
 Acq On : 17 Mar 2023 20:47
 Operator : JC/MD
 Sample : VU0317WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK053

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.478	2839	2842	2844	rBV	235	203	0.03%	0.004%
78	10.751	2914	2927	2948	rVB	192744	304282	47.68%	6.588%
79	10.922	2976	2980	2983	rVB	172	124	0.02%	0.003%
80	11.086	3027	3031	3040	rBV2	695	844	0.13%	0.018%
81	11.176	3056	3059	3061	rBV	140	106	0.02%	0.002%
82	11.735	3231	3233	3236	rBV3	416	289	0.05%	0.006%
83	11.809	3244	3256	3274	rBV	243237	387561	60.73%	8.391%
84	11.967	3302	3305	3306	rBV	193	115	0.02%	0.002%
85	12.143	3356	3360	3362	rBV	221	195	0.03%	0.004%
86	12.188	3362	3374	3396	rVV	258125	413239	64.76%	8.947%
87	13.603	3812	3814	3817	rBV	209	98	0.02%	0.002%
88	13.838	3882	3887	3897	rVB5	1892	2541	0.40%	0.055%
89	14.092	3957	3966	3976	rBV3	3653	5579	0.87%	0.121%
90	14.150	3982	3984	3986	rBV	137	43	0.01%	0.001%
91	14.198	3996	3999	4002	rVB	229	143	0.02%	0.003%
92	14.330	4034	4040	4048	rBV3	2163	2713	0.43%	0.059%
93	14.713	4157	4159	4162	rVB	342	170	0.03%	0.004%




Sum of corrected areas: 4618720

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
Data File : VU053280.D
Acq On : 17 Mar 2023 20:47
Operator : JC/MD
Sample : VU0317WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK053

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

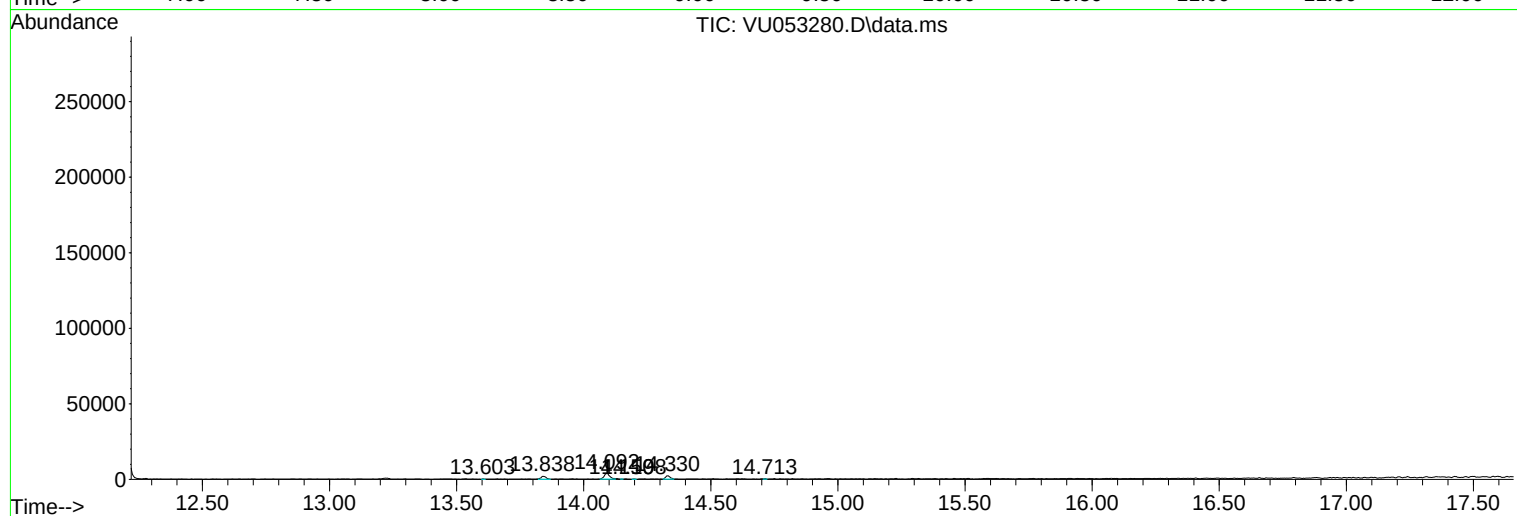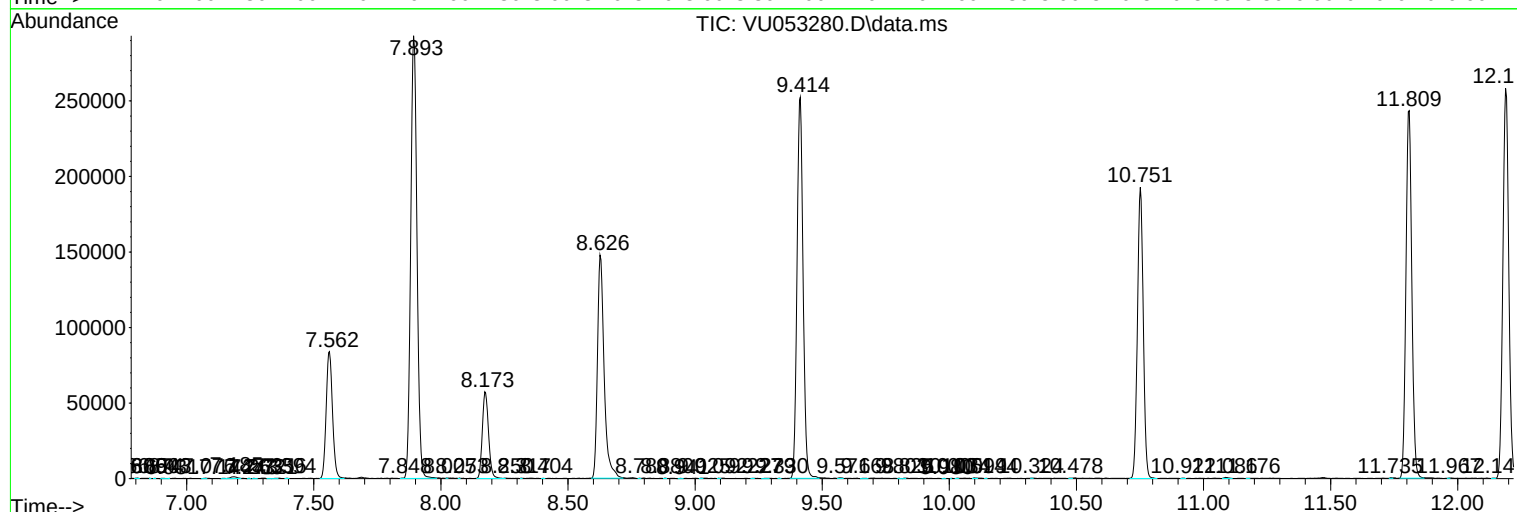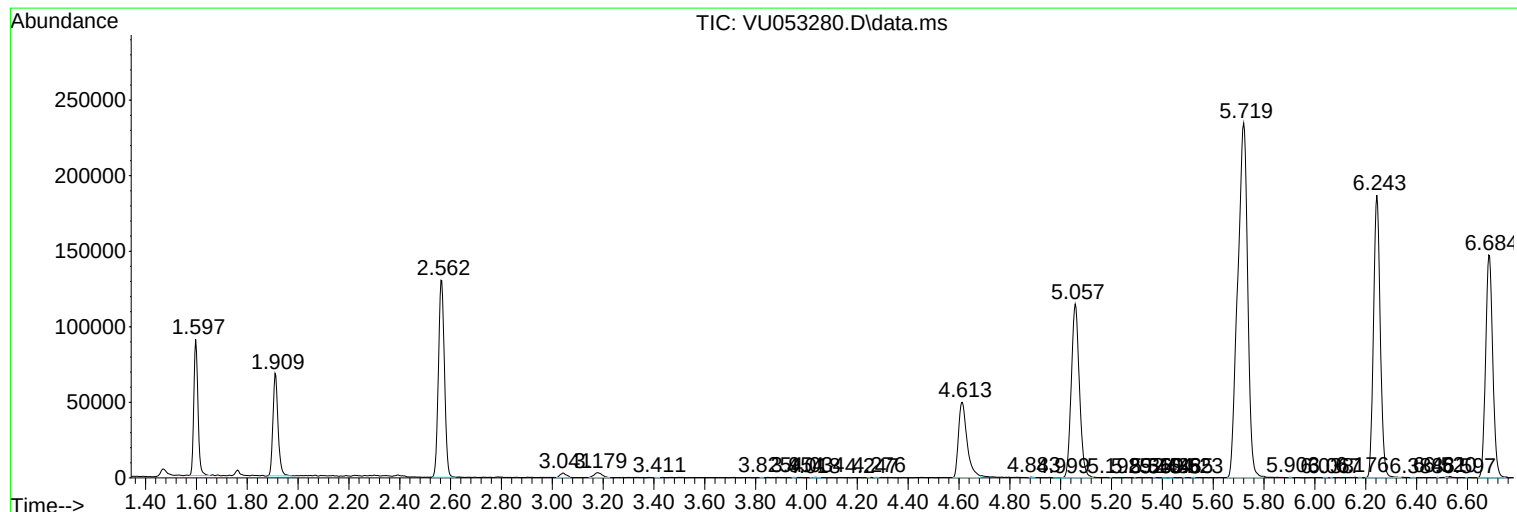

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
Data File : VU053280.D
Acq On : 17 Mar 2023 20:47
Operator : JC/MD
Sample : VU0317WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK053

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
Data File : VU053280.D
Acq On : 17 Mar 2023 20:47
Operator : JC/MD
Sample : VU0317WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK053

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------