

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
 Data File : VU053284.D
 Acq On : 17 Mar 2023 22:22
 Operator : JC/MD
 Sample : 01961-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053284.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.465	33	39	50	rBV	7463	13667	2.33%	0.316%
2	1.597	73	80	97	rVB	80840	90933	15.50%	2.101%
3	1.912	170	178	192	rVB	61537	83032	14.15%	1.918%
4	2.565	369	381	394	rBV	116240	186108	31.72%	4.299%
5	2.787	448	450	453	rBV2	316	206	0.04%	0.005%
6	3.160	564	566	568	rVB	257	101	0.02%	0.002%
7	3.179	568	572	578	rBV3	320	403	0.07%	0.009%
8	3.327	616	618	622	rBV	167	75	0.01%	0.002%
9	3.510	673	675	676	rBV	154	45	0.01%	0.001%
10	3.816	769	770	771	rBV	138	37	0.01%	0.001%
11	3.961	812	815	818	rVB	244	139	0.02%	0.003%
12	4.076	849	851	853	rBV	192	68	0.01%	0.002%
13	4.192	881	887	889	rBV	214	276	0.05%	0.006%
14	4.440	960	964	967	rBV	356	357	0.06%	0.008%
15	4.472	971	974	976	rVB	168	92	0.02%	0.002%
16	4.613	1005	1018	1046	rBV	45006	112908	19.24%	2.608%
17	4.851	1090	1092	1095	rBV	224	89	0.02%	0.002%
18	4.948	1120	1122	1125	rBV	251	191	0.03%	0.004%
19	4.970	1126	1129	1132	rVB2	239	177	0.03%	0.004%
20	5.057	1140	1156	1180	rBV	102986	238818	40.70%	5.517%
21	5.160	1187	1188	1189	rBV	111	24	0.00%	0.001%
22	5.176	1191	1193	1196	rVB2	201	91	0.02%	0.002%
23	5.215	1202	1205	1210	rBV2	290	358	0.06%	0.008%
24	5.279	1222	1225	1230	rVB	457	343	0.06%	0.008%
25	5.308	1230	1234	1237	rBV	225	240	0.04%	0.006%
26	5.327	1237	1240	1241	rBV	147	67	0.01%	0.002%
27	5.401	1261	1263	1266	rVB2	174	91	0.02%	0.002%
28	5.472	1283	1285	1286	rBV2	262	128	0.02%	0.003%
29	5.504	1293	1295	1298	rBV	169	81	0.01%	0.002%
30	5.559	1309	1312	1315	rBV	247	237	0.04%	0.005%
31	5.623	1330	1332	1334	rVB	123	49	0.01%	0.001%
32	5.719	1342	1362	1384	rBV2	215181	586791	100.00%	13.556%
33	5.967	1436	1439	1440	rBV2	129	60	0.01%	0.001%
34	6.243	1511	1525	1543	rBV	178627	334045	56.93%	7.717%
35	6.517	1607	1610	1611	rBV	216	149	0.03%	0.003%
36	6.533	1611	1615	1616	rVV	157	121	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
 Data File : VU053284.D
 Acq On : 17 Mar 2023 22:22
 Operator : JC/MD
 Sample : 01961-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.600	1634	1636	1637	rBV	115	24	0.00%	0.001%
38	6.632	1643	1646	1649	rBV	249	240	0.04%	0.006%
39	6.684	1649	1662	1686	rVV	141519	271916	46.34%	6.282%
40	6.767	1686	1688	1692	rVV	171	78	0.01%	0.002%
41	6.880	1721	1723	1724	rBV	135	36	0.01%	0.001%
42	6.903	1727	1730	1733	rVB2	217	157	0.03%	0.004%
43	6.983	1748	1755	1758	rBV	327	400	0.07%	0.009%
44	7.182	1810	1817	1825	rBV4	1038	1602	0.27%	0.037%
45	7.227	1829	1831	1833	rBV	189	84	0.01%	0.002%
46	7.317	1857	1859	1860	rBV	131	35	0.01%	0.001%
47	7.343	1865	1867	1869	rBV	150	91	0.02%	0.002%
48	7.485	1909	1911	1912	rVB	118	24	0.00%	0.001%
49	7.497	1913	1915	1919	rBV	251	120	0.02%	0.003%
50	7.562	1923	1935	1950	rBV	76363	132073	22.51%	3.051%
51	7.690	1970	1975	1981	rVB3	685	740	0.13%	0.017%
52	7.787	2002	2005	2009	rBV	242	269	0.05%	0.006%
53	7.893	2025	2038	2066	rBV	270625	461267	78.61%	10.656%
54	8.086	2095	2098	2101	rVB	212	113	0.02%	0.003%
55	8.128	2109	2111	2114	rVB2	137	61	0.01%	0.001%
56	8.176	2114	2126	2151	rBV	52013	87322	14.88%	2.017%
57	8.266	2151	2154	2160	rVB	240	222	0.04%	0.005%
58	8.443	2206	2209	2213	rBV	255	208	0.04%	0.005%
59	8.468	2214	2217	2220	rBV	155	83	0.01%	0.002%
60	8.501	2225	2227	2231	rVB	199	139	0.02%	0.003%
61	8.626	2253	2266	2296	rBV2	136237	251102	42.79%	5.801%
62	8.761	2305	2308	2312	rBV	363	294	0.05%	0.007%
63	8.800	2317	2320	2321	rBV	145	80	0.01%	0.002%
64	8.928	2358	2360	2365	rVB	295	227	0.04%	0.005%
65	8.954	2365	2368	2372	rBV	221	220	0.04%	0.005%
66	8.986	2376	2378	2380	rVV	212	117	0.02%	0.003%
67	8.999	2380	2382	2387	rVB	235	214	0.04%	0.005%
68	9.353	2491	2492	2493	rBV	109	34	0.01%	0.001%
69	9.414	2499	2511	2535	rBV	245586	407287	69.41%	9.409%
70	9.533	2545	2548	2550	rVB2	233	121	0.02%	0.003%
71	9.555	2553	2555	2556	rBV2	123	36	0.01%	0.001%
72	9.603	2568	2570	2572	rBV	166	50	0.01%	0.001%
73	9.671	2589	2591	2593	rVB	192	61	0.01%	0.001%
74	9.687	2594	2596	2598	rVB	188	74	0.01%	0.002%
75	9.838	2641	2643	2646	rBV2	215	137	0.02%	0.003%
76	9.941	2673	2675	2679	rVB2	136	78	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
 Data File : VU053284.D
 Acq On : 17 Mar 2023 22:22
 Operator : JC/MD
 Sample : 01961-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.082	2716	2719	2722	rBV	196	123	0.02%	0.003%
78	10.131	2732	2734	2736	rBV	170	75	0.01%	0.002%
79	10.150	2736	2740	2743	rVV	311	218	0.04%	0.005%
80	10.369	2806	2808	2810	rBV	142	58	0.01%	0.001%
81	10.427	2824	2826	2828	rBV	132	55	0.01%	0.001%
82	10.671	2899	2902	2904	rBV2	204	112	0.02%	0.003%
83	10.751	2915	2927	2940	rBV	178905	283634	48.34%	6.553%
84	10.822	2947	2949	2951	rBV	193	71	0.01%	0.002%
85	10.951	2986	2989	2992	rVB2	148	104	0.02%	0.002%
86	11.079	3027	3029	3031	rVB	145	36	0.01%	0.001%
87	11.272	3087	3089	3090	rBV	183	76	0.01%	0.002%
88	11.468	3147	3150	3151	rBV	170	85	0.01%	0.002%
89	11.597	3187	3190	3194	rBV	186	117	0.02%	0.003%
90	11.616	3194	3196	3197	rBV	180	62	0.01%	0.001%
91	11.748	3234	3237	3240	rVB	220	134	0.02%	0.003%
92	11.809	3244	3256	3277	rVV	240671	383183	65.30%	8.852%
93	11.922	3289	3291	3293	rBV	149	47	0.01%	0.001%
94	12.189	3362	3374	3395	rBV	245507	391578	66.73%	9.046%
95	13.407	3750	3753	3755	rBV	236	130	0.02%	0.003%
96	13.803	3873	3876	3878	rBV	154	76	0.01%	0.002%
97	14.539	4102	4105	4109	rVB	248	162	0.03%	0.004%
98	15.195	4307	4309	4311	rBV	322	179	0.03%	0.004%
99	15.587	4428	4431	4432	rBV2	265	129	0.02%	0.003%
100	15.655	4449	4452	4453	rBV	243	126	0.02%	0.003%


Sum of corrected areas: 4328603

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
Data File : VU053284.D
Acq On : 17 Mar 2023 22:22
Operator : JC/MD
Sample : 01961-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

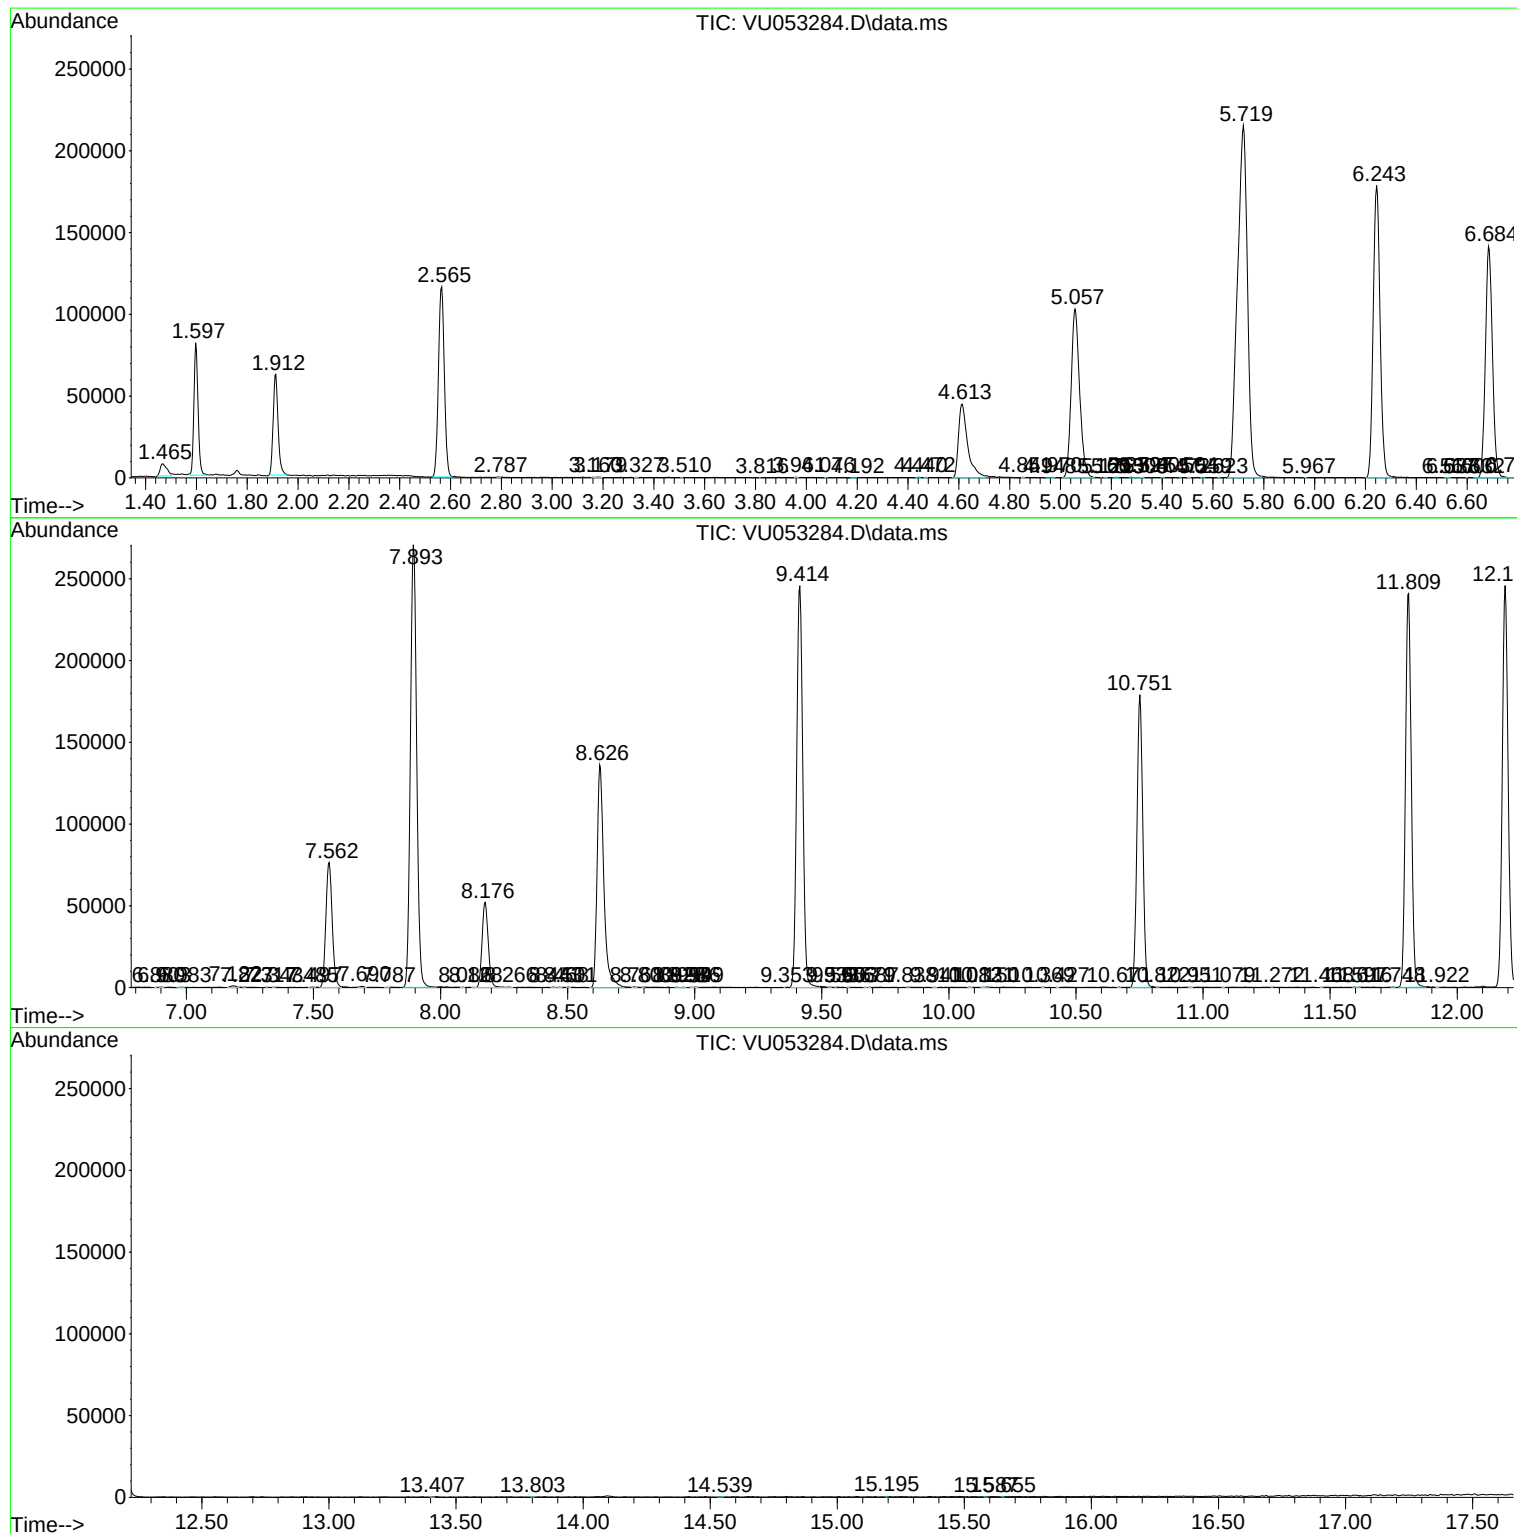

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
Data File : VU053284.D
Acq On : 17 Mar 2023 22:22
Operator : JC/MD
Sample : 01961-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031723\
Data File : VU053284.D
Acq On : 17 Mar 2023 22:22
Operator : JC/MD
Sample : 01961-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------