

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031819\
 Data File : VU030170.D
 Acq On : 18 Mar 2019 13:44
 Operator : JC/SP
 Sample : K1949-19DL 500X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1H1DL

Quant Time: Mar 19 02:44:36 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Mar 18 12:44:57 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	515535	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	499547	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	235198	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	132790	38.94	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	77.88%
7) Chloroethane-d5	1.68	69	117945	42.85	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.70%
11) 1,1-Dichloroethene-d2	2.27	63	190683	30.98	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	61.96%
21) 2-Butanone-d5	4.17	46	268650	105.15	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	105.15%
24) Chloroform-d	4.65	84	279996	45.77	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.54%
26) 1,2-Dichloroethane-d4	5.31	65	166118	47.01	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.02%
32) Benzene-d6	5.34	84	574728	44.69	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.38%
36) 1,2-Dichloropropane-d6	6.33	67	188746	47.96	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.92%
41) Toluene-d8	7.56	98	513759	42.67	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.34%
43) trans-1,3-Dichloropropene-	7.85	79	81917	42.97	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.94%
47) 2-Hexanone-d5	8.31	63	217241	98.65	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	98.65%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	298380	49.34	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.68%
64) 1,2-Dichlorobenzene-d4	11.86	152	217899	47.82	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.64%


Target Compounds					Ovalue
46) Tetrachloroethene	8.22	164	143538	43.779 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031819\
Data File : VU030170.D
Acq On : 18 Mar 2019 13:44
Operator : JC/SP
Sample : K1949-19DL 500X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1H1DL

Quant Time: Mar 19 02:44:36 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 18 12:44:57 2019
Response via : Initial Calibration

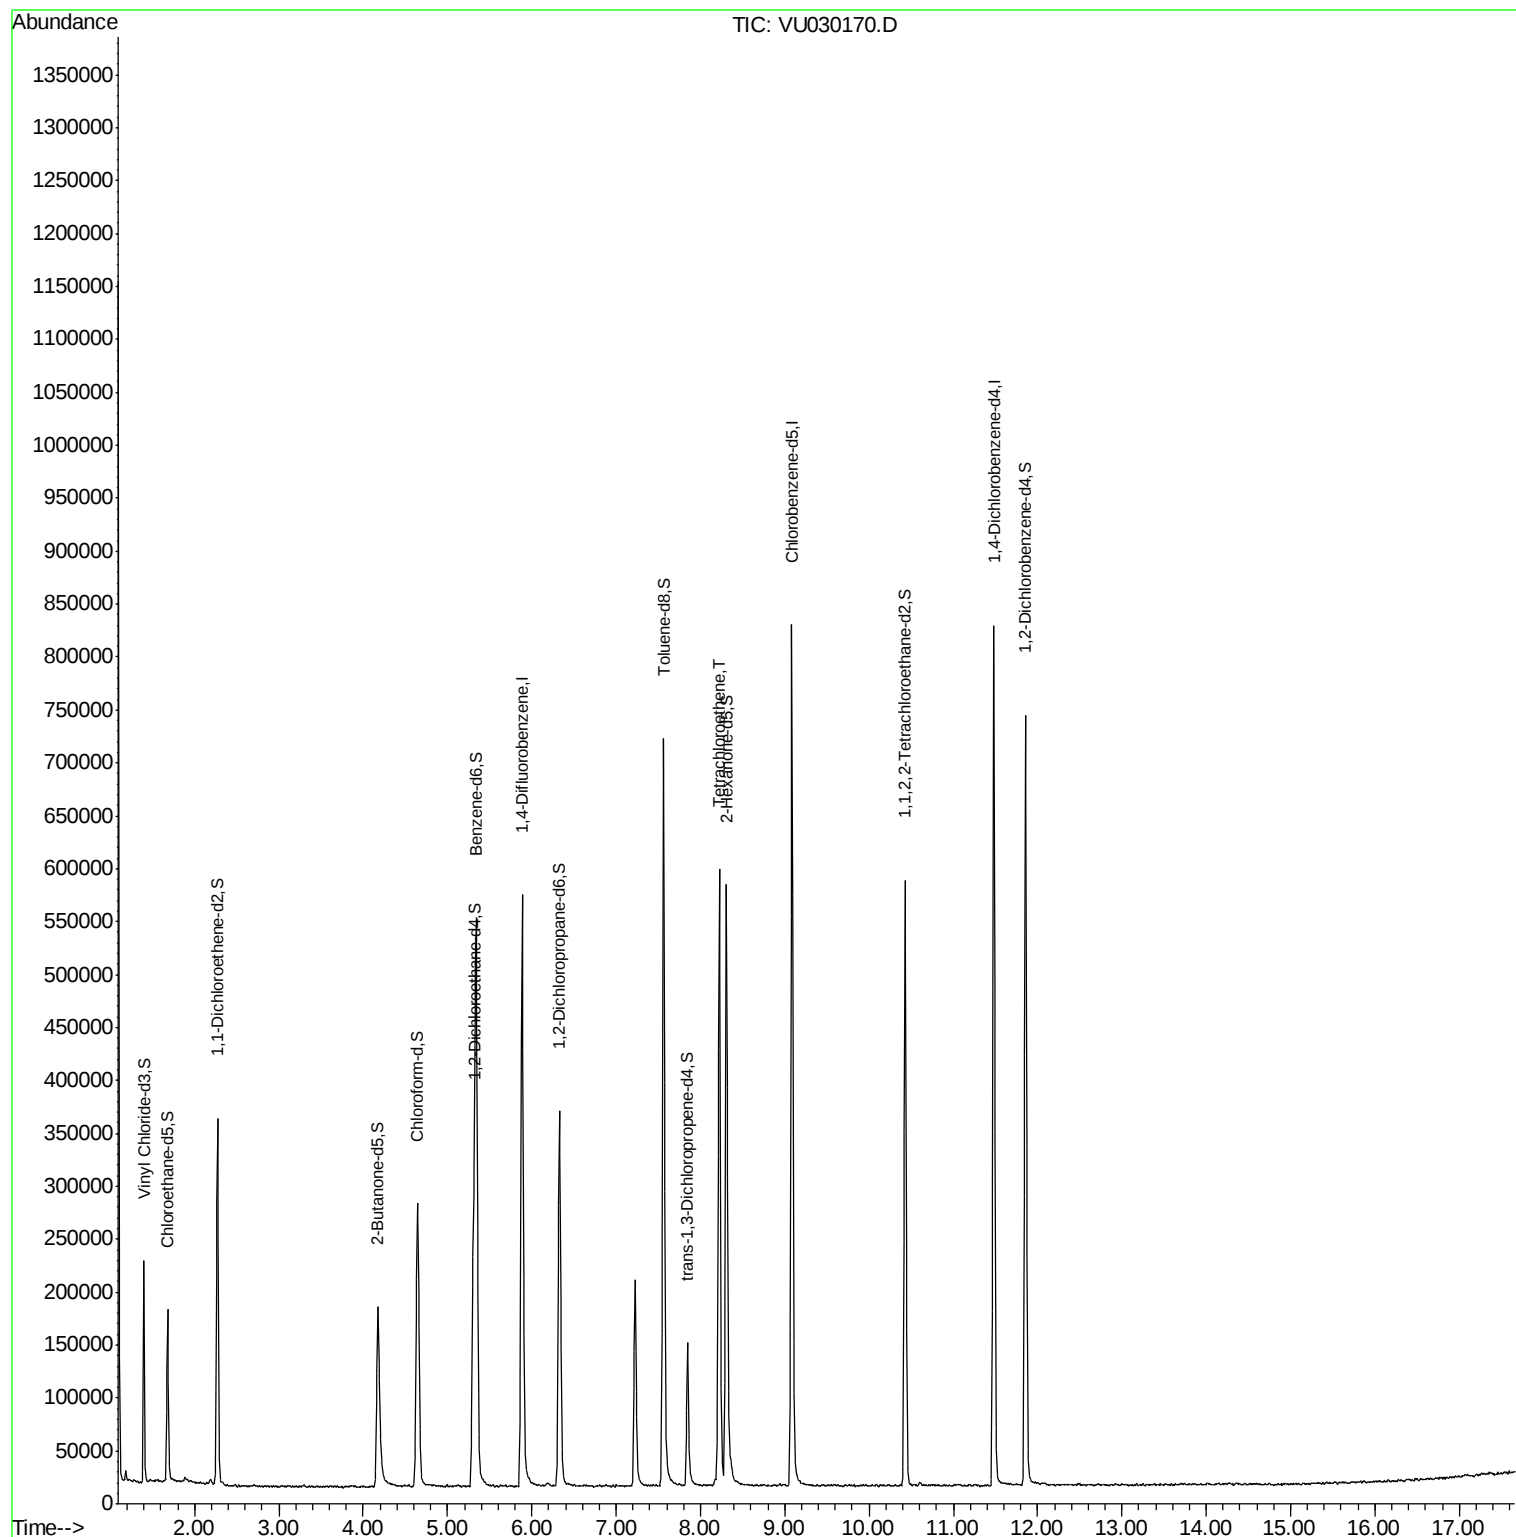

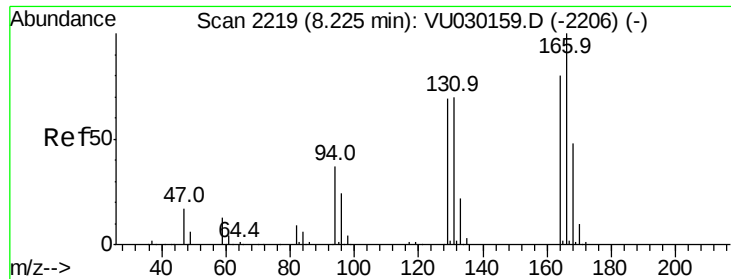

#46

Tetrachloroethene

Concen: 43.779 ug/L

RT: 8.22 min Scan# 2219

Delta R.T. 0.00 min

Lab File: VU030170.D


Acq: 18 Mar 2019 13:44

Instrument :

MSVOA_U

ClientSampleId :

BF1H1DL

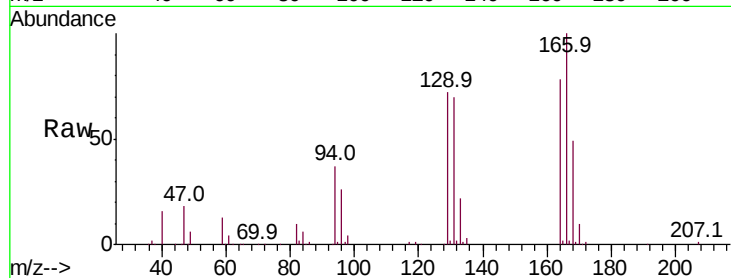

Tot Ion:164 Resp: 143538

Ion Ratio Lower Upper

164 100

129 93.0 63.3 117.7

131 90.0 62.0 115.2

166 128.8 90.5 168.1

Abundance Ion 164.00 (163.70 to 164.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

Ion 166.00 (165.70 to 166.70): V

